

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042822\
 Data File : PD069285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2022 11:31
 Operator : AR\AJ
 Sample : N2469-08MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFF8MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/30/2022
 Supervised By : mohammad ahmed 05/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 01:11:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.186	25878357	257.2E6	20.425	21.312
27)	SA Decachlor...	8.200	9.379	49137644	258.3E6	36.952	36.726m
Target Compounds							
2)	A alpha-BHC	3.883	4.582	114.1E6	921.4E6	63.810	56.046m
3)	MA gamma-BHC...	4.166	4.872	111.2E6	858.3E6	61.504	55.091m
4)	MA Heptachlor	4.464	5.400	107.3E6	806.3E6	63.188	53.264m
5)	MB Aldrin	4.712	5.714	100.6E6	795.8E6	63.161	55.751
6)	B beta-BHC	4.417	5.035	49121905	308.2E6	63.418	45.940m#
7)	B delta-BHC	4.621	5.262	50146973	235.1E6	31.416	20.024m#
8)	B Heptachlo...	5.155	6.100	98678134	600.7E6	67.034	53.919m
9)	A Endosulfan I	5.494	6.464	84348842	619.7E6	57.803	52.173
10)	B trans-Chl...	5.381	6.337	118.1E6	778.6E6	78.798	61.371m
11)	B cis-Chlor...	5.440	6.414	105.8E6	759.9E6	70.885	61.015
12)	B 4,4'-DDE	5.606	6.562	216.1E6	1364.7E6	161.144	125.445m
13)	MA Dieldrin	5.736	6.722	221.7E6	1379.4E6	142.440m	114.360m
14)	MA Endrin	5.996	6.942	186.6E6	1076.1E6	133.363	110.651m
15)	B Endosulfa...	6.270	7.148	165.2E6	1036.1E6	128.198	108.106
16)	A 4,4'-DDD	6.124	7.054	151.7E6	1058.8E6	124.461	113.067
17)	MA 4,4'-DDT	6.363	7.357	185.7E6	1215.2E6	151.371	134.998
18)	B Endrin al...	6.439	7.271	115.1E6	752.0E6	115.920	105.255m
19)	B Endosulfa...	6.652	7.496	149.0E6	855.4E6	118.929	97.483m
20)	A Methoxychlor	6.914	7.811	425.4E6	2298.2E6	626.825	557.682
21)	B Endrin ke...	7.145	7.973	177.7E6	1017.1E6	123.001	110.175

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042822\
Data File : PD069285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2022 11:31
Operator : AR\AJ
Sample : N2469-08MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:11:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

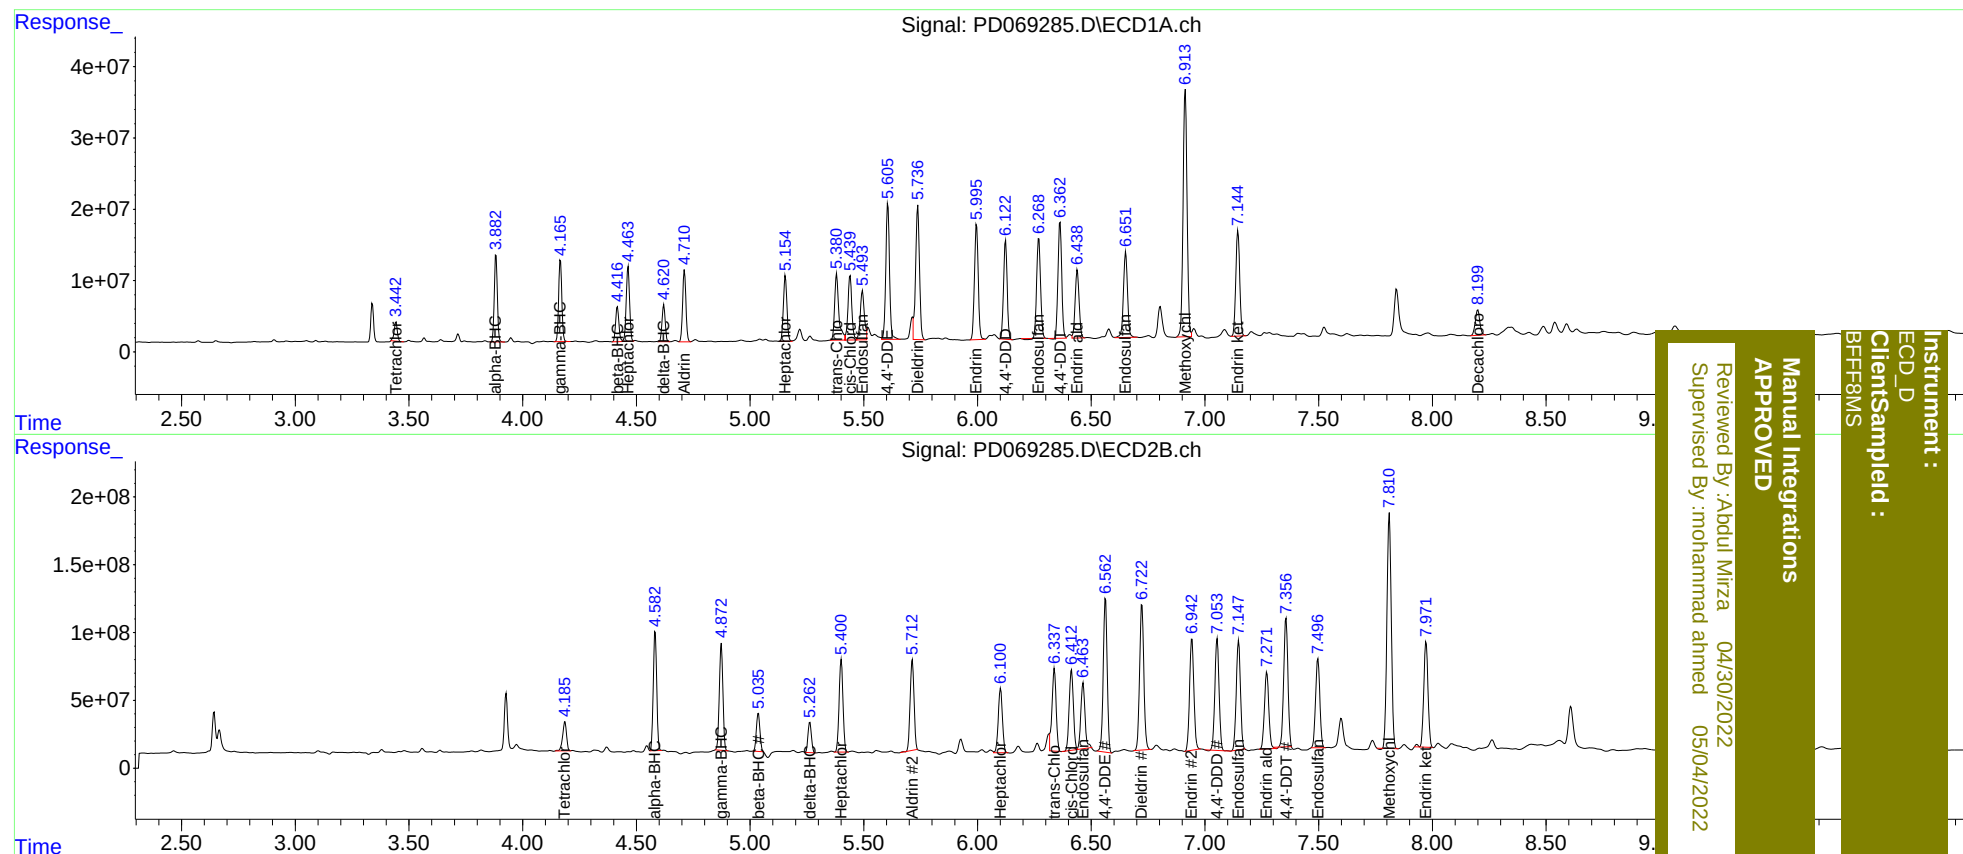

Instrument :
ECD_D
ClientSampled :
BFF8MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 04/30/2022
Supervised By: mohammad ahmed 05/04/2022