

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042822\
 Data File : PD069286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2022 11:45
 Operator : AR\AJ
 Sample : N2469-09MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFF8MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/29/2022
 Supervised By :mohammad ahmed 04/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 01:12:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.170	26099221	241.9E6	20.600	20.046
27)	SA Decachlor...	8.199	9.363	46731317	238.0E6	35.142	33.842m
Target Compounds							
2)	A alpha-BHC	3.883	4.565	112.7E6	874.4E6	63.054	53.191m
3)	MA gamma-BHC...	4.166	4.857	111.0E6	821.3E6	61.377	52.716
4)	MA Heptachlor	4.464	5.385	106.5E6	760.2E6	62.720	50.219
5)	MB Aldrin	4.711	5.697	99213219	774.9E6	62.281	54.286
6)	B beta-BHC	4.416	5.020	48966884	318.8E6	63.218	47.527
7)	B delta-BHC	4.620	5.247	49736293	227.6E6	31.159	19.387 #
8)	B Heptachlo...	5.155	6.085	96500871	539.8E6	65.555	48.448 #
9)	A Endosulfan I	5.494	6.448	77011846	654.3E6	52.775	55.087
10)	B trans-Chl...	5.381	6.321	115.5E6	726.6E6	77.031	57.271m#
11)	B cis-Chlor...	5.440	6.398	100.2E6	742.0E6	67.154	59.573
12)	B 4,4'-DDE	5.606	6.546	208.4E6	1267.4E6	155.389	116.501 #
13)	MA Dieldrin	5.738	6.707	218.9E6	1304.2E6	140.620	108.124
14)	MA Endrin	5.995	6.927	184.4E6	1003.5E6	131.807	103.181
15)	B Endosulfa...	6.269	7.133	162.8E6	1012.8E6	126.309	105.674
16)	A 4,4'-DDD	6.123	7.039	149.2E6	1025.6E6	122.353	109.520
17)	MA 4,4'-DDT	6.363	7.341	180.8E6	1198.2E6	147.390	133.108
18)	B Endrin al...	6.439	7.256	111.3E6	743.9E6	112.127	104.117
19)	B Endosulfa...	6.651	7.481	144.1E6	845.2E6	114.979	96.321
20)	A Methoxychlor	6.913	7.795	418.9E6	2215.1E6	617.302	537.518
21)	B Endrin ke...	7.144	7.955	175.0E6	952.5E6	121.104	103.171m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042822\
Data File : PD069286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2022 11:45
Operator : AR\AJ
Sample : N2469-09MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:12:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

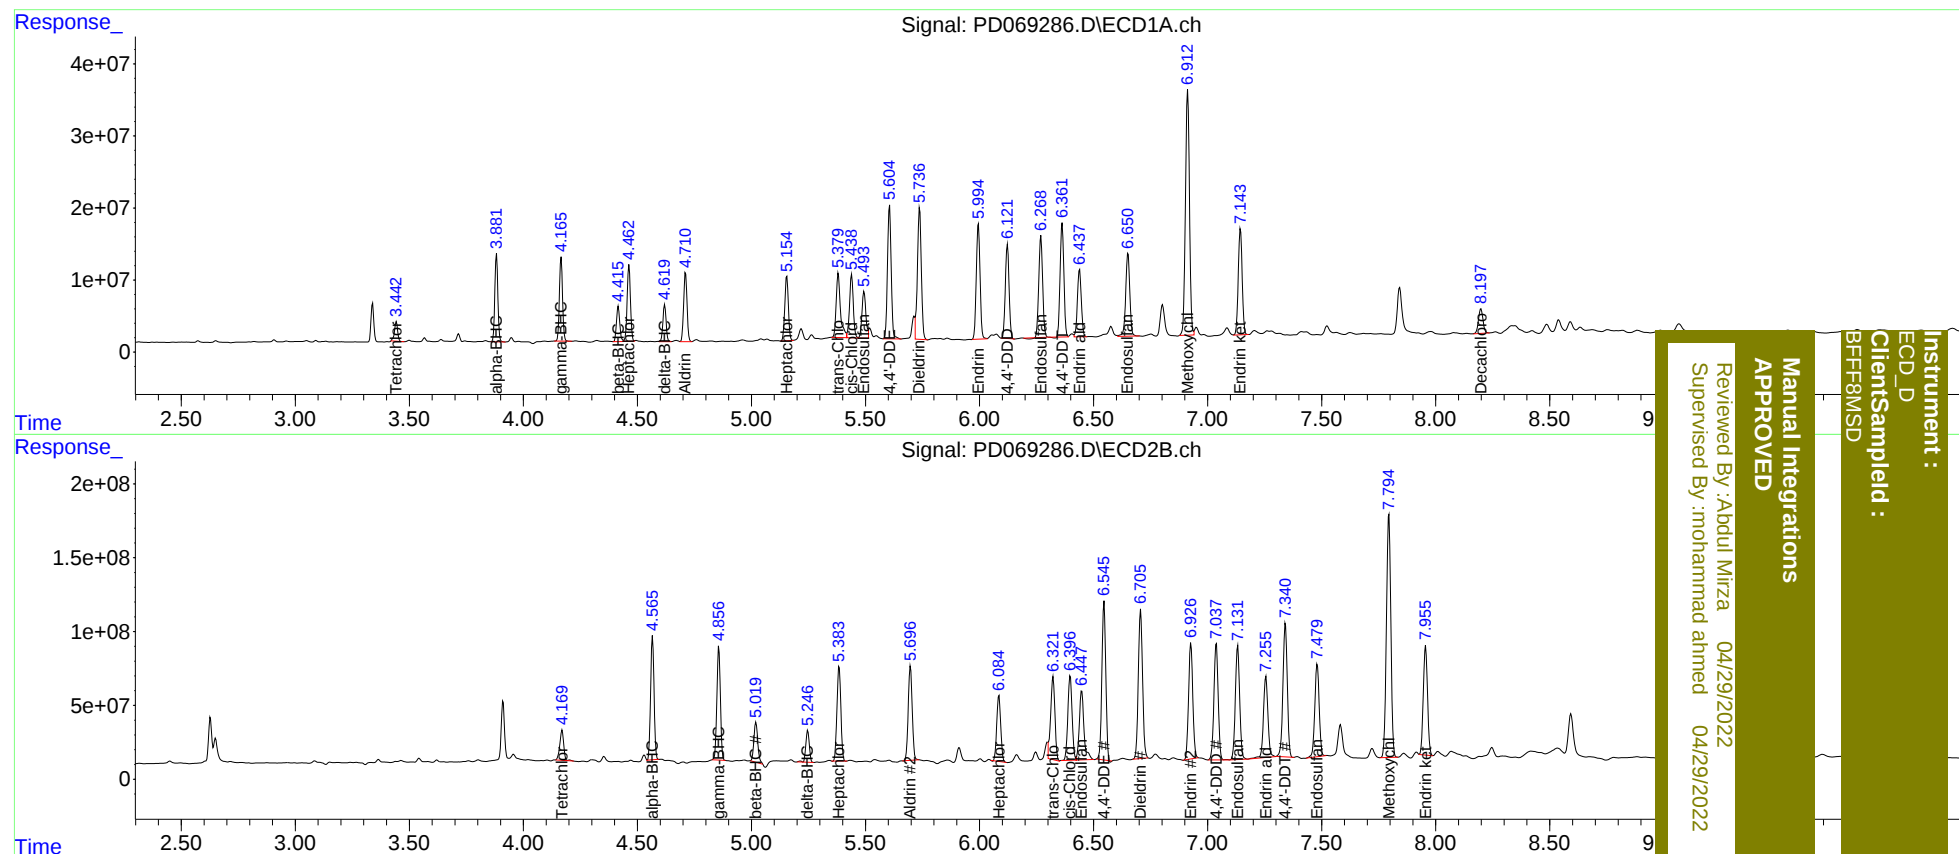

Reviewed By: Abdul Miza 04/29/2022
Supervised By: mohammad ahmed 04/29/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BFFF8MSD