

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
 Data File : PD075040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2023 19:15
 Operator : AR\AJ
 Sample : 02417-24MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW906MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/01/2023
 Supervised By : Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 22:17:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.771	32160228	14934523	14.397m	14.406
27) SA Decachlor...	9.088	7.918	65679808	18891744	27.499	19.667 #
Target Compounds						
2) A alpha-BHC	4.003	3.273	160.2E6	60330046	43.651m	41.897
3) MA gamma-BHC...	4.336	3.602	136.4E6	51619536	39.900m	37.096m
4) MA Heptachlor	4.929	3.945	144.9E6	57167164	41.814	40.987
5) MB Aldrin	5.273	4.225	145.7E6	57035703	43.491	43.374
6) B beta-BHC	4.533	3.899	54410474	24713618	36.912	36.315
7) B delta-BHC	4.782	4.130	106.0E6	44620634	35.401	31.720
8) B Heptachlo...	5.700	4.727	217.9E6	46618190	72.570	37.969 #
9) A Endosulfan I	6.086	5.099	113.1E6	30231878	38.843	26.497 #
10) B trans-Chl...	5.954	4.978	340.5E6	47040245	113.742	38.830 #
11) B cis-Chlor...	6.036	5.042	117.2E6	46429095	37.609	37.498
12) B 4,4'-DDE	6.207	5.232	229.9E6	87518496	78.260	77.370
13) MA Dieldrin	6.361	5.362	275.4E6	106.3E6	86.658m	84.674m
14) MA Endrin	6.593	5.648	232.4E6	511.7E6	85.771	462.966 #
15) B Endosulfa...	6.811	5.932	224.5E6	85610461	77.506	78.481
16) A 4,4'-DDD	6.726	5.786	201.3E6	72550264	83.259	75.090
17) MA 4,4'-DDT	7.040	6.037	222.4E6	77015099	88.508	77.637
18) B Endrin al...	6.941	6.111	169.6E6	50880559	75.773	57.290
19) B Endosulfa...	7.177	6.334	199.1E6	74493603	76.374	72.452
20) A Methoxychlor	7.517	6.613	588.6E6	212.8E6	408.270	385.310
21) B Endrin ke...	7.663	6.840	228.1E6	87969359	78.859	73.775

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
Data File : PD075040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2023 19:15
Operator : AR\AJ
Sample : 02417-24MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 22:17:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

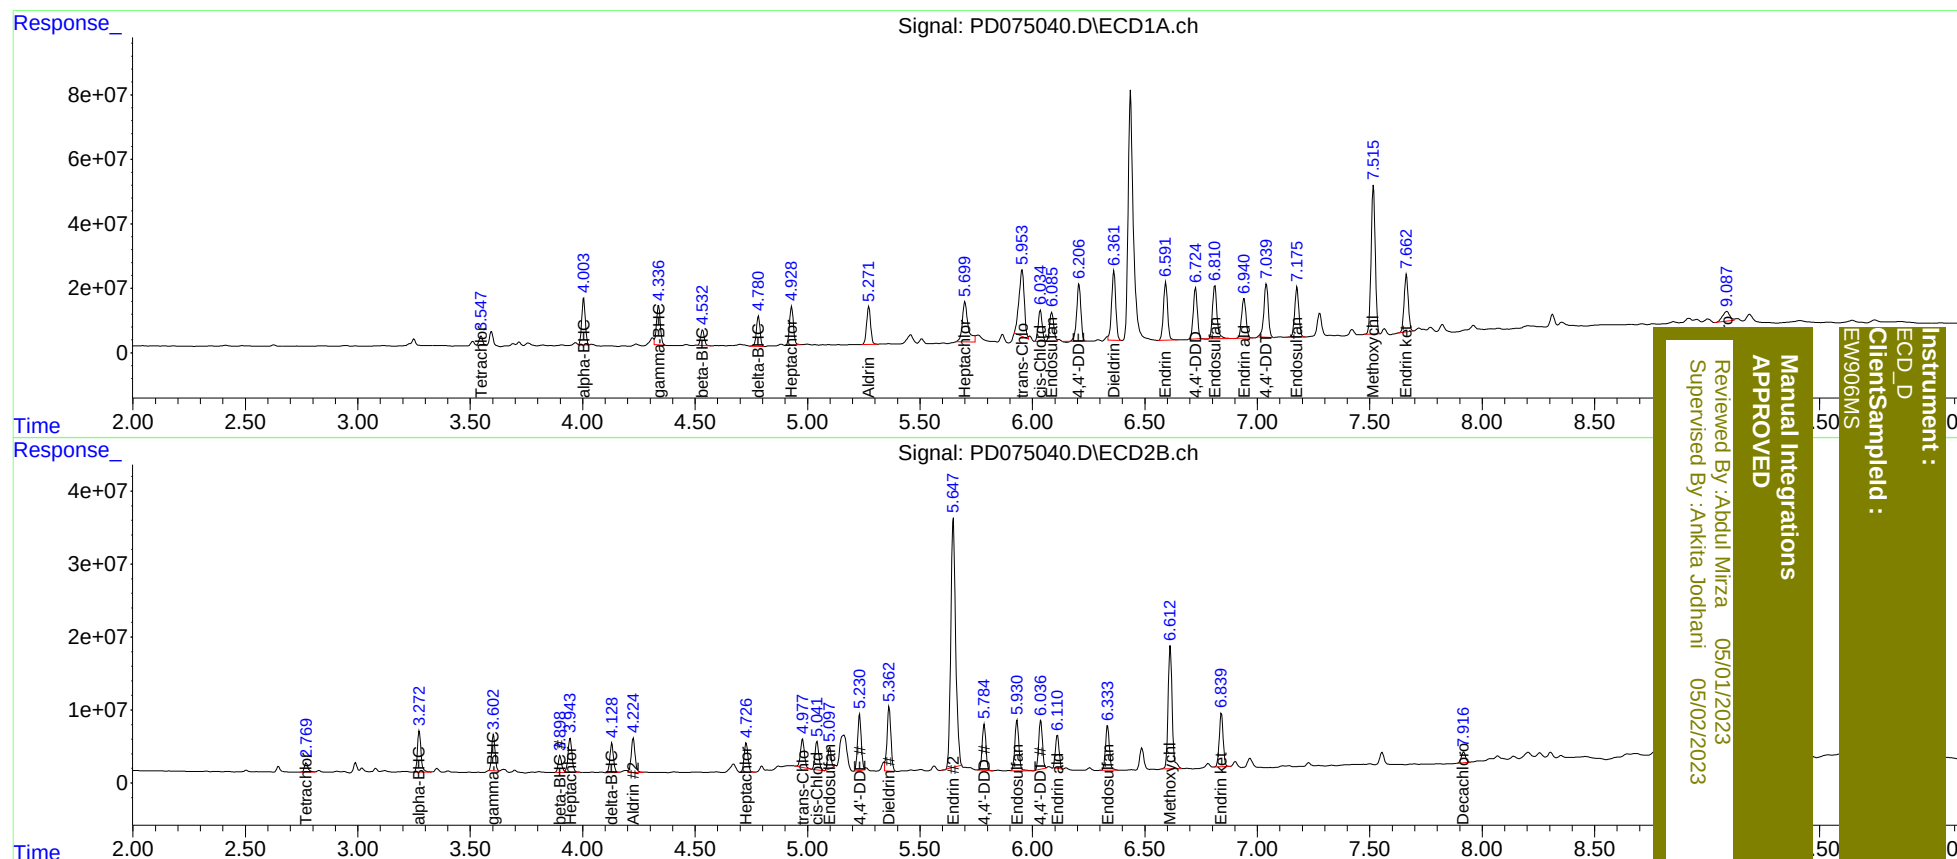

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/01/2023
Supervised By: Ankita Jodhani 05/02/2023

Instrument :
ECD_D
Client Sampled :
EW/06MS