

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
 Data File : PD075052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2023 01:47
 Operator : AR\AJ
 Sample : 02419-29MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW925MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/02/2023
 Supervised By : Ankita Jodhani 05/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 04:34:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.771	68477659	9333035	30.655m	9.003m#
27)	SA Decachlor...	9.085	7.915	236.4E6	74320494	98.965	77.368
Target Compounds							
2)	A alpha-BHC	4.002	3.274	153.7E6	56884795	41.868m	39.504
3)	MA gamma-BHC...	4.340	3.603	903.4E6	93114089	264.224m	66.915 #
4)	MA Heptachlor	4.927	3.945	169.2E6	2736.4E6	48.851m	1961.959m#
5)	MB Aldrin	5.297	4.241	7994.3E6	2679.1E6	2386.958m	2037.343
6)	B beta-BHC	4.512	3.899	3905.1E6	13823295	2649.273m	20.312m#
7)	B delta-BHC	4.802	4.140	7211.8E6	2716.2E6	2409.373m	1930.907
8)	B Heptachlo...	5.692	4.721	10576.3E6	131.6E6	3521.684	107.195m#
9)	A Endosulfan I	6.069	5.096	645.1E6	62364678	221.547	54.659 #
10)	B trans-Chl...	5.947	4.954	3606.5E6	2684.4E6	1204.809m	2215.905m#
11)	B cis-Chlor...	6.034	5.052	169.2E6	1314.4E6	54.287	1061.551 #
12)	B 4,4'-DDE	6.204	5.230	6663.6E6	84182507	2268.568m	74.421 #
13)	MA Dieldrin	6.358	5.364	1387.6E6	4544.3E6	436.567m	3620.281 #
14)	MA Endrin	6.589	5.606	9538.3E6	2966.2E6	3520.869	2683.785m
15)	B Endosulfa...	6.815	5.920	367.1E6	2542.1E6	126.741m	2330.394 #
16)	A 4,4'-DDD	6.734	5.784	4755.2E6	88143724	1966.410m	91.229m#
17)	MA 4,4'-DDT	7.013	6.031	10185.5E6	3203.8E6	4053.777m	3229.624m
18)	B Endrin al...	6.948	6.081	882.6E6	215.5E6	394.347m	242.601m#
19)	B Endosulfa...	7.163	6.331	420.3E6	328.6E6	161.211m	319.568m#
20)	A Methoxychlor	7.516	6.608	500.5E6	226.5E6	347.149	410.049m
21)	B Endrin ke...	7.656	6.838	189.3E6	46566133	65.437m	39.052m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
Data File : PD075052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2023 01:47
Operator : AR\AJ
Sample : 02419-29MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 04:34:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

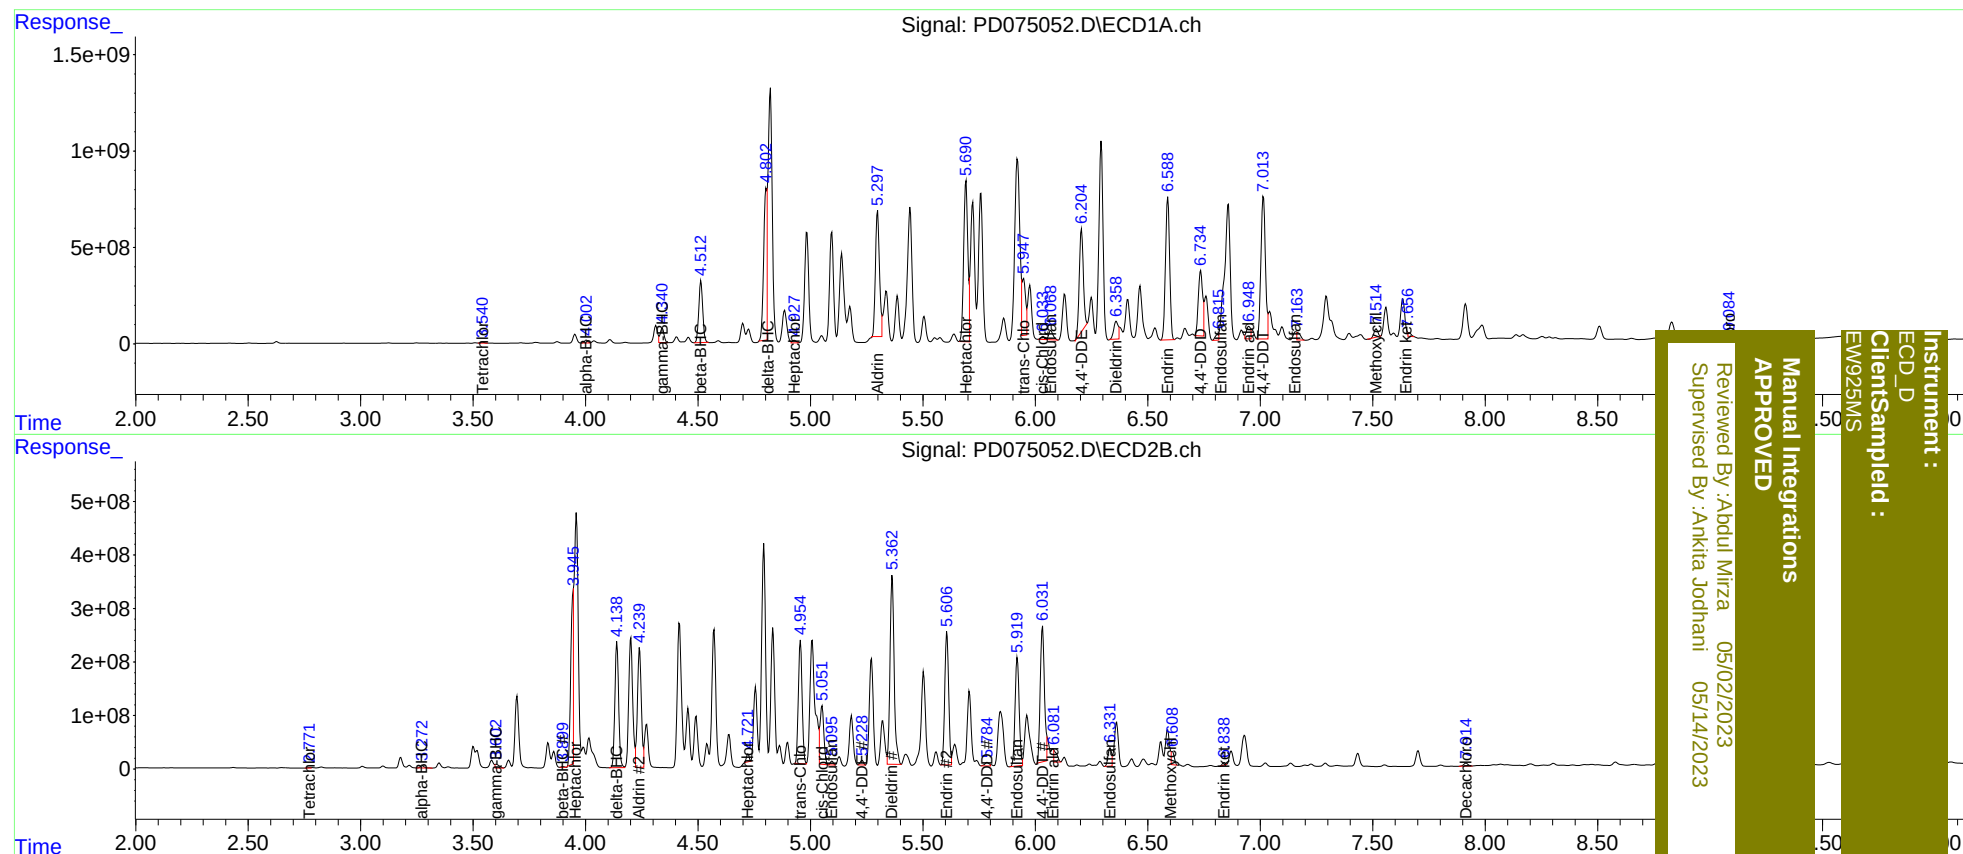

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/02/2023
Supervised By: Ankita Jodhani 05/14/2023

Instrument :
ECD_D
Client Sampled :
EW/25MS