

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
 Data File : PD075041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2023 19:42
 Operator : AR\AJ
 Sample : 02417-25MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW906MSD

Manual Integrations APPROVED

Reviewed By :Abdul

Mirza

05/01/2023

Supervised By :Ankita

Jodhani

05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 22:17:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.771	33355964	15101329	14.932m	14.567
2)	SA Decachlor...	9.086	7.918	62562620	19980757	26.194	20.800
Target Compounds							
2)	A alpha-BHC	4.003	3.273	160.0E6	60960657	43.597m	42.335
3)	MA gamma-BHC...	4.336	3.602	146.1E6	52793004	42.735m	37.939m
4)	MA Heptachlor	4.929	3.944	146.2E6	57849776	42.195	41.477
5)	MB Aldrin	5.272	4.224	147.3E6	57598542	43.980	43.802
6)	B beta-BHC	4.533	3.899	54588785	25004567	37.033	36.742
7)	B delta-BHC	4.780	4.129	107.1E6	44944737	35.781	31.951
8)	B Heptachlo...	5.700	4.726	220.4E6	47201596	73.379	38.444 #
9)	A Endosulfan I	6.086	5.098	114.9E6	30626794	39.456	26.843 #
10)	B trans-Chl...	5.954	4.977	341.4E6	47366248	114.065	39.099 #
11)	B cis-Chlor...	6.036	5.041	117.9E6	46610099	37.838	37.645
12)	B 4,4'-DDE	6.207	5.231	233.7E6	88813993	79.545	78.515
13)	MA Dieldrin	6.361	5.362	270.7E6	107.6E6	85.165m	85.714m
14)	MA Endrin	6.592	5.648	234.1E6	518.0E6	86.431	468.707 #
15)	B Endosulfa...	6.811	5.932	229.0E6	86434454	79.053	79.236
16)	A 4,4'-DDD	6.725	5.786	204.0E6	73378383	84.358	75.947
17)	MA 4,4'-DDT	7.040	6.037	226.2E6	77895223	90.019	78.524
18)	B Endrin al...	6.941	6.111	170.5E6	51456998	76.188	57.939
19)	B Endosulfa...	7.176	6.334	202.8E6	75653732	77.793	73.580
20)	A Methoxychlor	7.516	6.613	592.5E6	215.4E6	410.959	390.014
21)	B Endrin ke...	7.662	6.841	245.4E6	89300478	84.813	74.891

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
Data File : PD075041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2023 19:42
Operator : AR\AJ
Sample : 02417-25MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 22:17:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

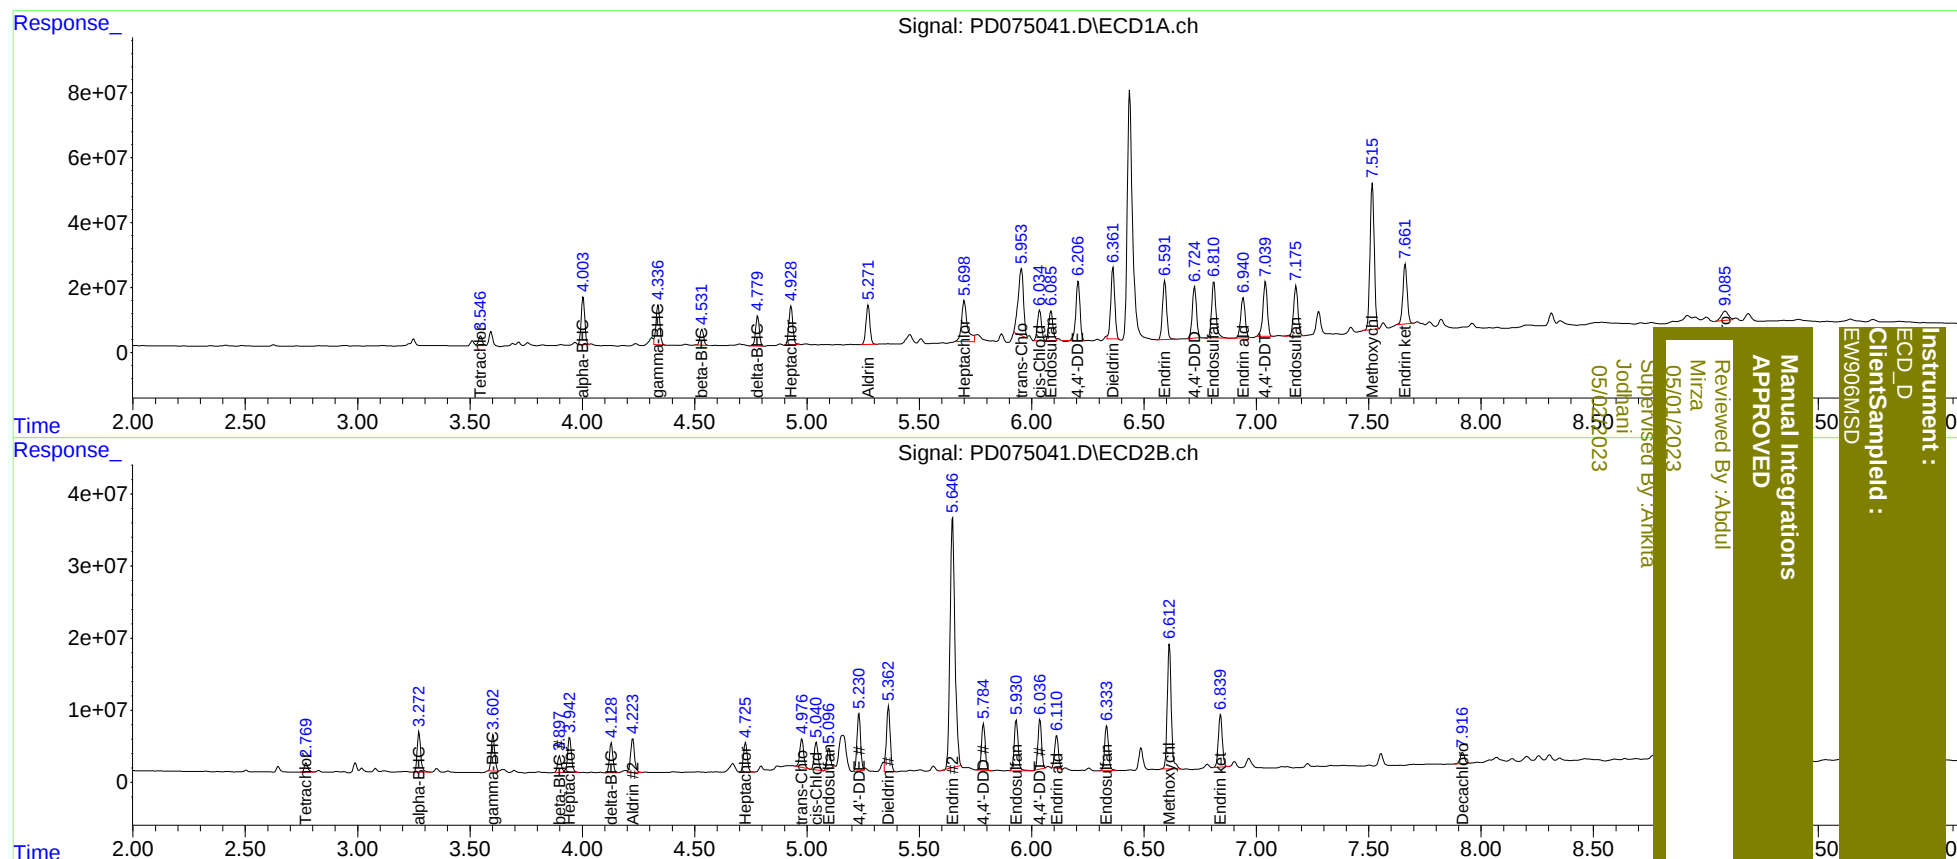

Instrument :
ECD_D
Client Sampled :
EW/06MSD

Manual Integrations
APPROVED

Reviewed By: Abdul
Mirza

05/01/2023

Supervised By: Arikita
Jodhani

05/02/2023