

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
 Data File : PD075057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2023 04:02
 Operator : AR\AJ
 Sample : 02419-34
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW929

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/02/2023
 Supervised By : Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 08:52:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	38992824	13066816	17.456	12.605 #
2)	SA Decachlor...	9.100	7.917	66937034	27215330	28.026	28.331
Target Compounds							
14)	MA Endrin	6.604	5.606	3772.7E6	1345.4E6	1392.616m	1217.318m
17)	MA 4,4'-DDT	7.029	6.031	4096.8E6	1437.9E6	1630.501m	1449.502m
19)	B Endosulfa...	7.173	6.332	194.0E6	114.5E6	74.419	111.371m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
Data File : PD075057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2023 04:02
Operator : AR\AJ
Sample : 02419-34
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 08:52:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

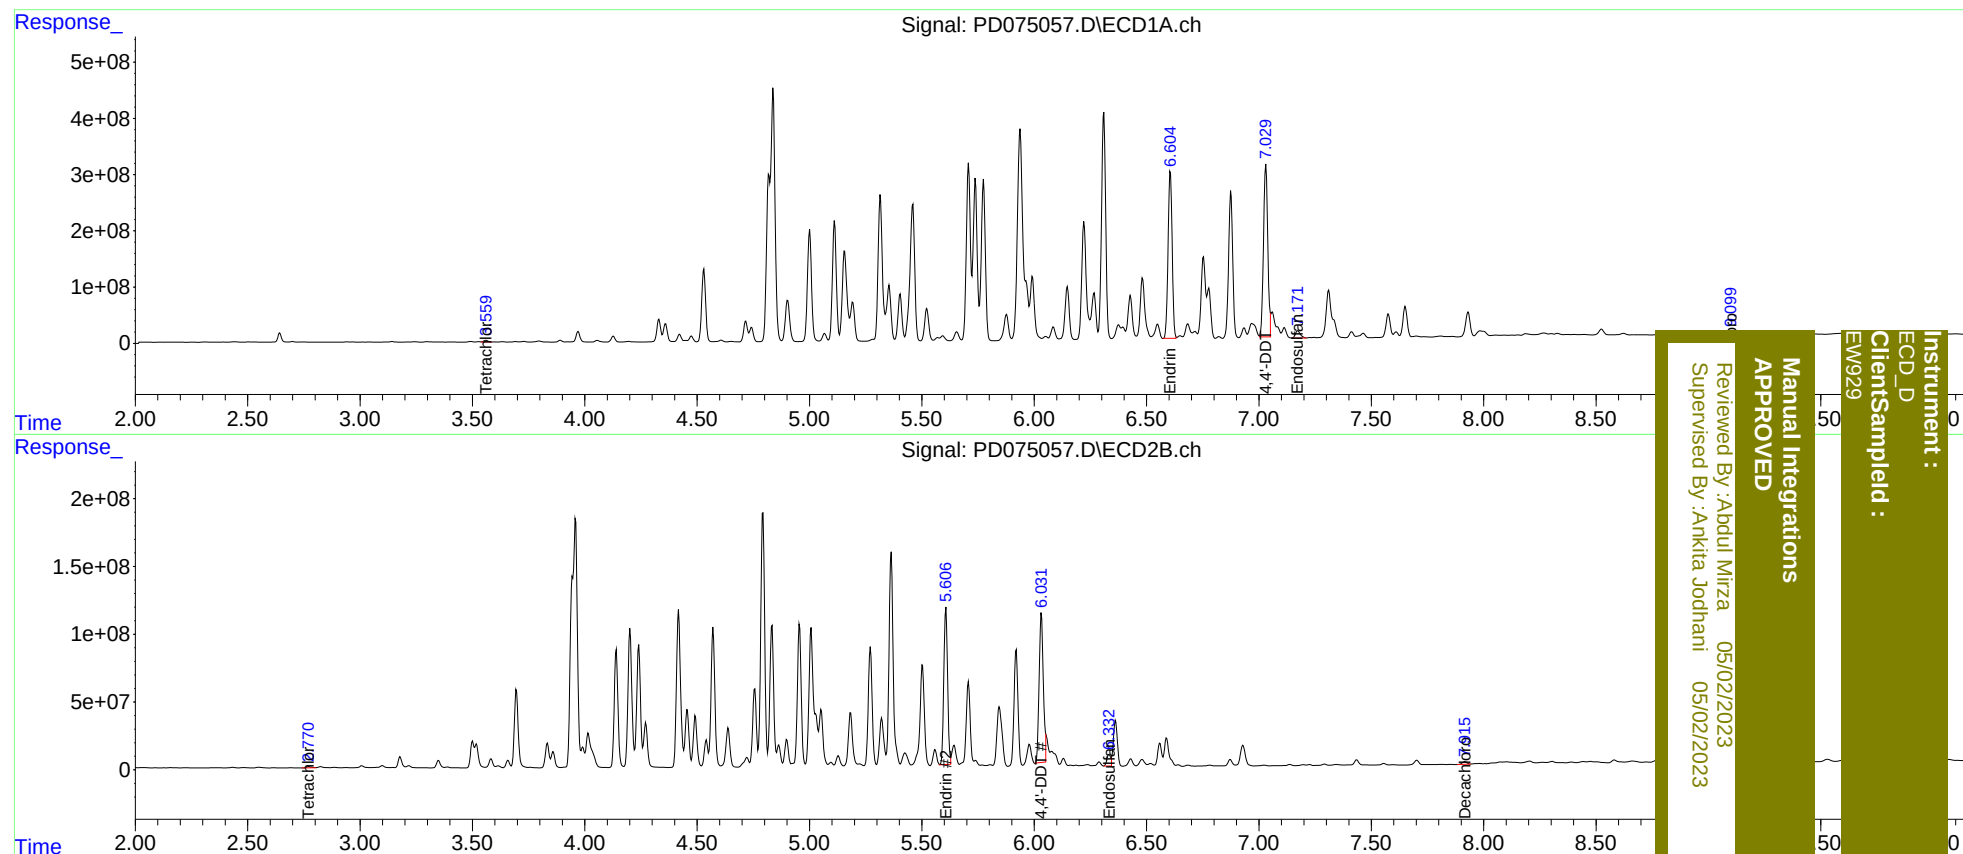

Instrument :
ECD_D
ClientSampled :
EW/929

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

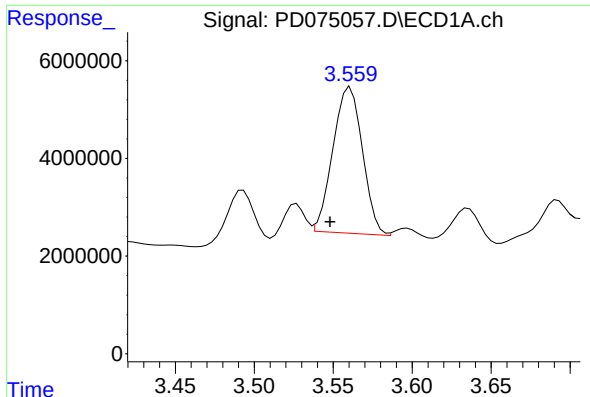


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.013 min
Response: 38992824
Conc: 17.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW929


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

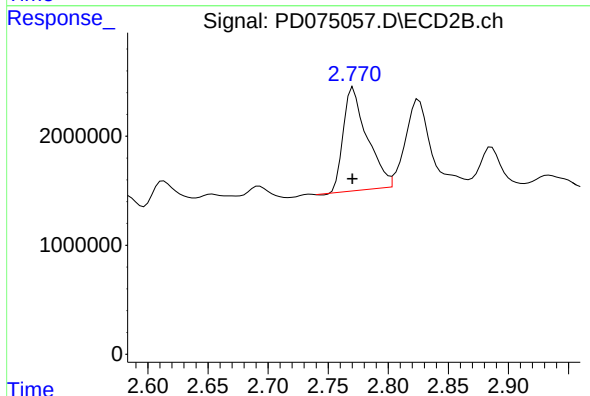


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 13066816
Conc: 12.60 ng/ml

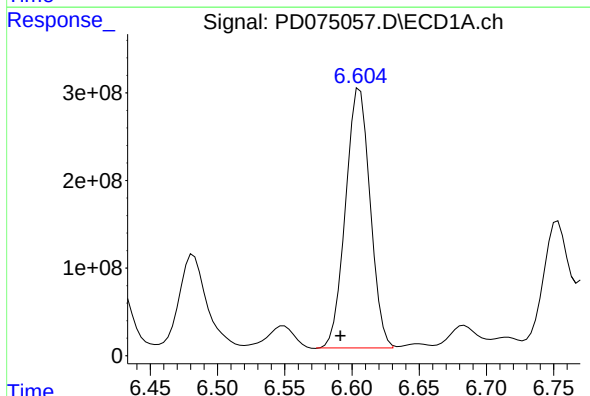


#14 Endrin

R.T.: 6.604 min
Delta R.T.: 0.013 min
Response: 3772717488
Conc: 1392.62 ng/ml m

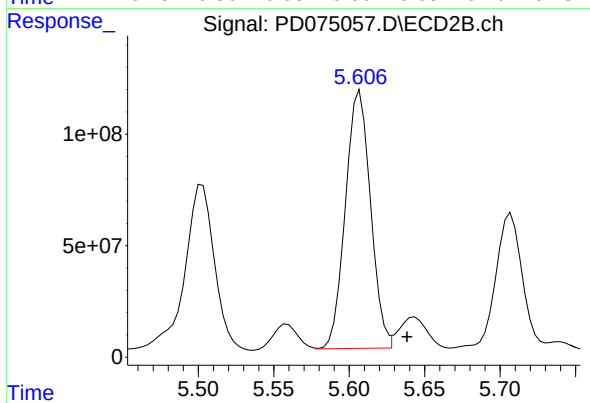

#14 Endrin

R.T.: 5.606 min
Delta R.T.: -0.032 min
Response: 1345423478
Conc: 1217.32 ng/ml m

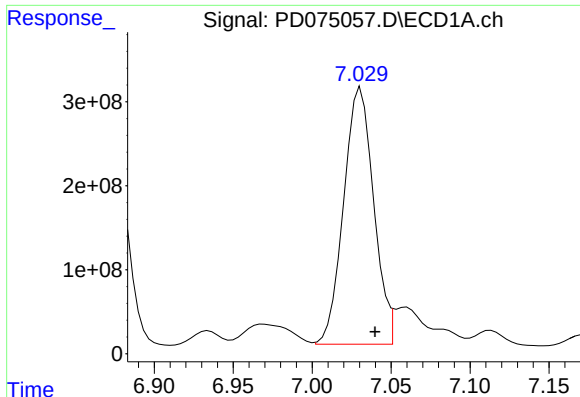


#17 4,4'-DDT

R.T.: 7.029 min
Delta R.T.: -0.010 min
Response: 4096781770
Conc: 1630.50 ng/m

Instrument :
ECD_D
ClientSampleId :
EW929


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

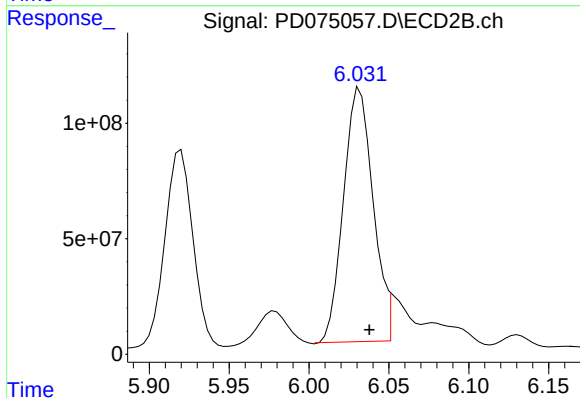


#17 4,4'-DDT

R.T.: 6.031 min
Delta R.T.: -0.007 min
Response: 1437899700
Conc: 1449.50 ng/ml m

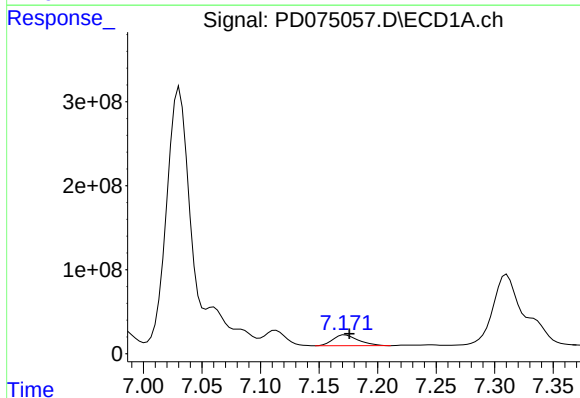


#19 Endosulfan Sulfate

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 194024457
Conc: 74.42 ng/ml

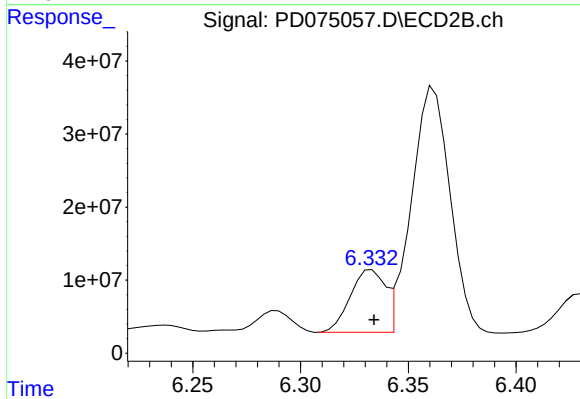

#19 Endosulfan Sulfate

R.T.: 6.332 min
Delta R.T.: -0.003 min
Response: 114510444
Conc: 111.37 ng/ml m

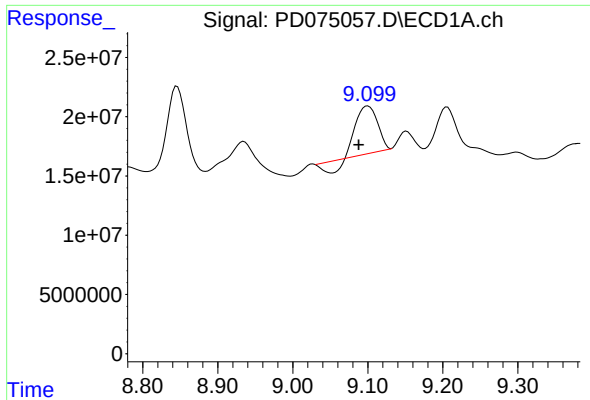


#27 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.012 min
Response: 66937034
Conc: 28.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW929

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

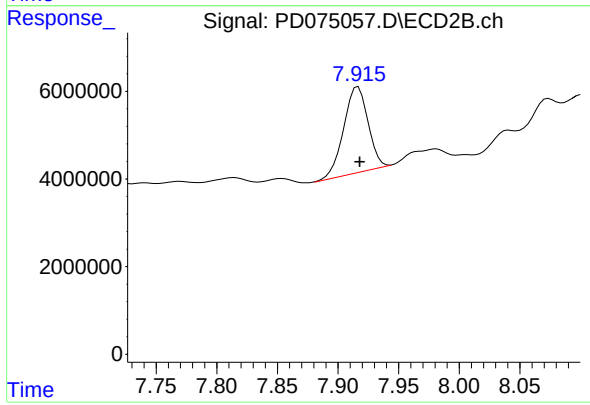

#27 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: -0.001 min
Response: 27215330
Conc: 28.33 ng/ml