

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
 Data File : PD075061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2023 06:05
 Operator : AR\AJ
 Sample : INDA400
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3201

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 08:53:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.770	49929016	22978717	22.352	22.166
2) SA Decachlor...	9.088	7.918	92544582	34230101	38.747	35.634
Target Compounds						
2) A alpha-BHC	4.004	3.273	83482850	32353502	22.748	22.468
3) MA gamma-BHC...	4.337	3.603	77865430	30845836	22.774	22.167
4) MA Heptachlor	4.928	3.944	76519701	29453703	22.088	21.118
9) A Endosulfan I	6.086	5.097	62831539	24052571	21.577	21.081
13) MA Dieldrin	6.362	5.362	140.0E6	56677431	44.041	45.153
14) MA Endrin	6.591	5.638	113.9E6	42945886	42.034	38.857
16) A 4,4'-DDD	6.725	5.785	110.0E6	43179620	45.488	44.691
17) MA 4,4'-DDT	7.040	6.037	93386827	35947052	37.168	36.237
20) A Methoxychlor	7.516	6.613	261.0E6	99390364	181.026	179.936

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042823\
Data File : PD075061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2023 06:05
Operator : AR\AJ
Sample : INDA400
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 08:53:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

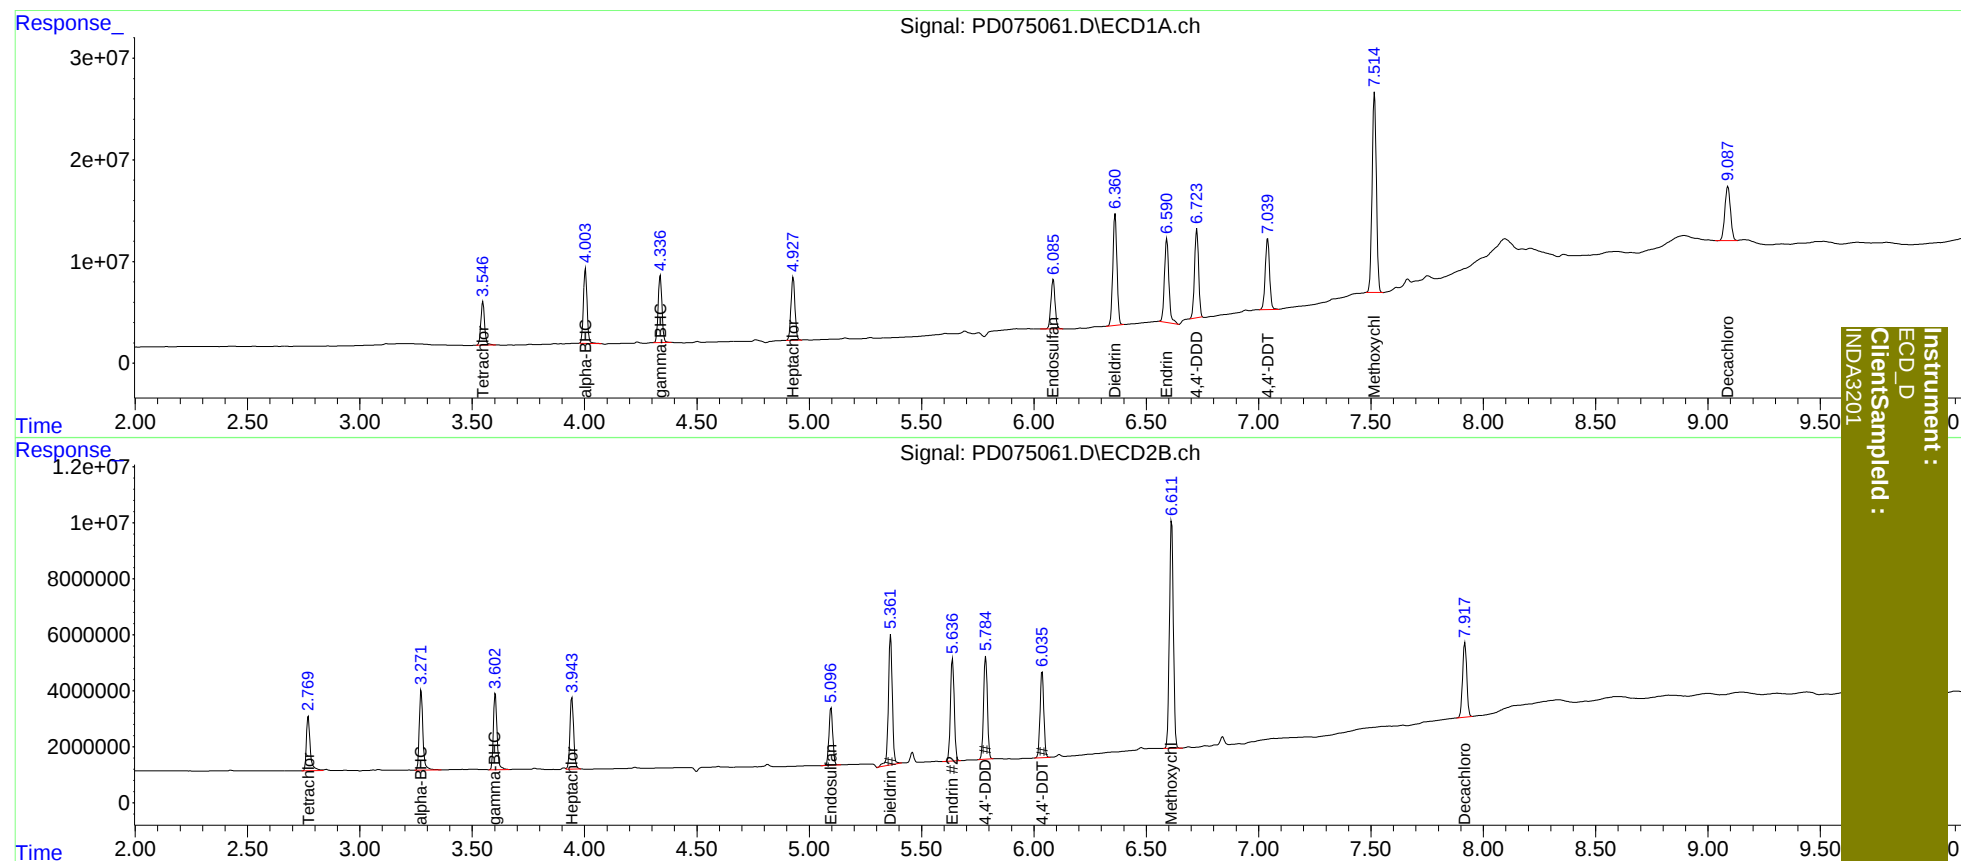

Instrument :
ECD_D
ClientSampled :
INDA3201