

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
 Data File : PD057841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2020 05:30
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 07:18:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 30 06:57:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.896	32084742	52258933	37.913	37.444
27)	SA Decachlor...	7.872	8.899	69929612	101.9E6	72.914	70.603
Target Compounds							
2)	A alpha-BHC	3.651	4.280	48419971	77470977	41.188	40.135
3)	MA gamma-BHC...	3.923	4.560	45859028	73064118	40.181	39.750
4)	MA Heptachlor	4.204	5.062	42024927	73833640	39.894	38.548
9)	A Endosulfan I	5.200	6.100	36324880	61012884	40.306	38.364
13)	MA Dieldrin	5.439	6.354	84095863	137.1E6	81.100	78.828
14)	MA Endrin	5.690	6.570	71190369	113.8E6	77.533	70.298
16)	A 4,4'-DDD	5.827	6.697	66647833	108.9E6	81.258	79.585
17)	MA 4,4'-DDT	6.061	6.994	68000428	114.2E6	81.610	78.725
20)	A Methoxychlor	6.609	7.454	168.7E6	287.0E6	383.110	355.766


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 05:30
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 07:18:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 30 06:57:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

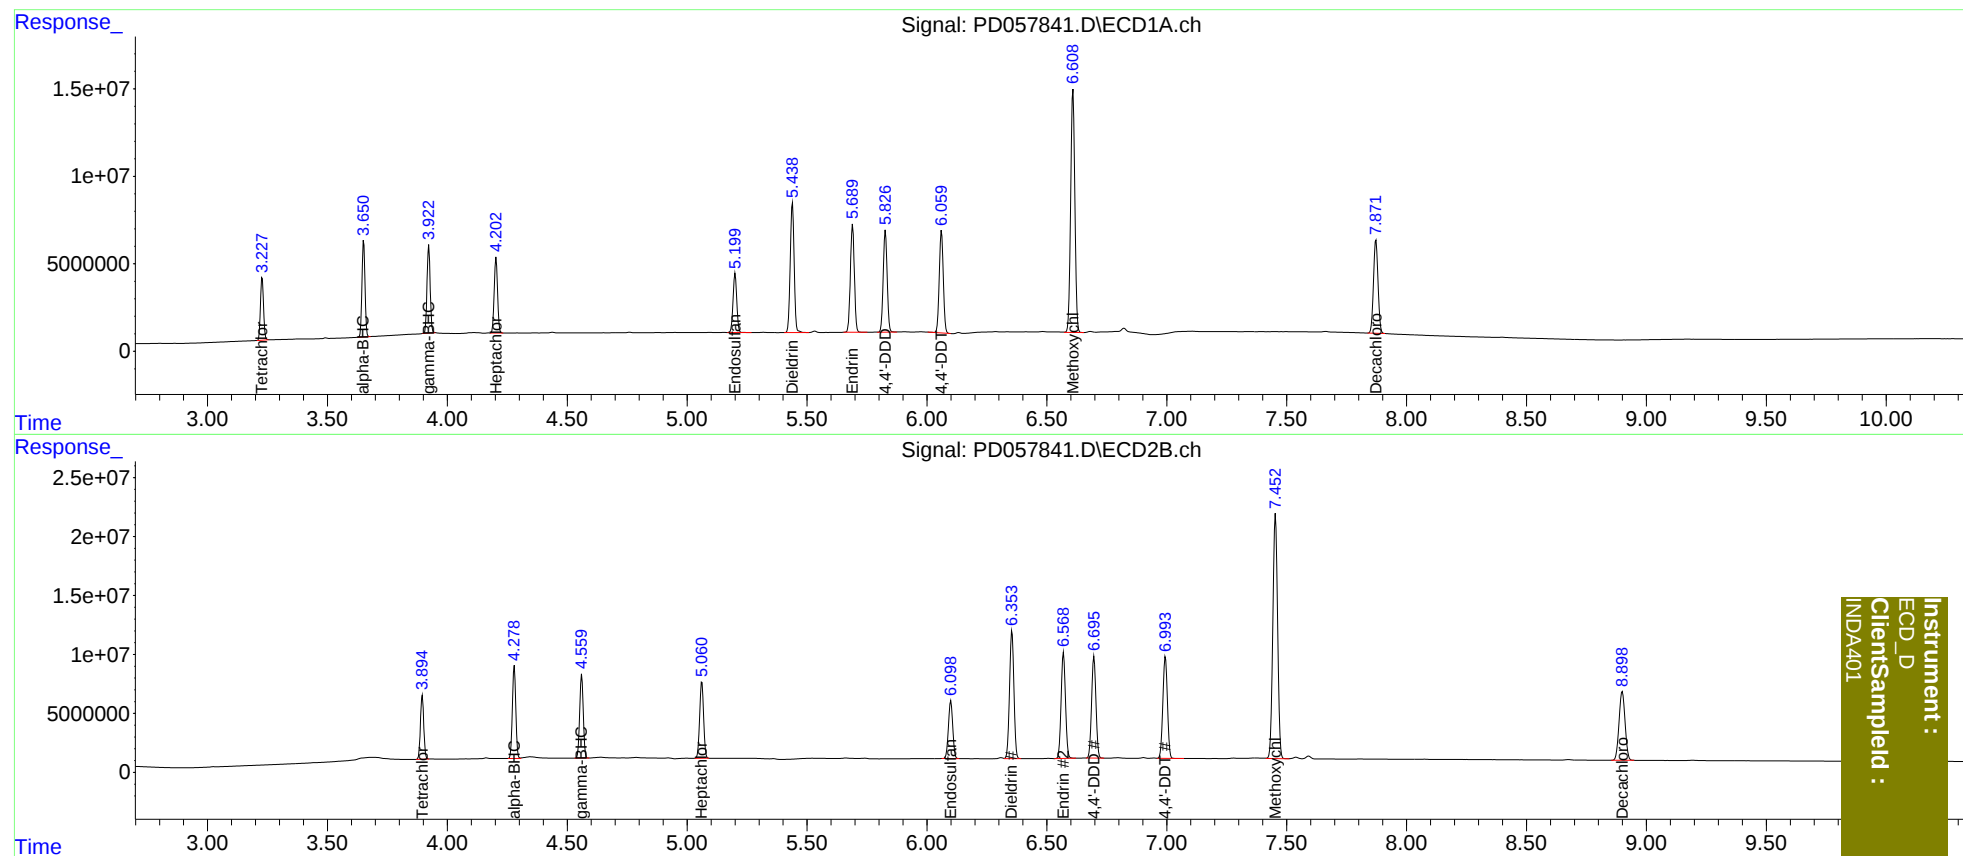


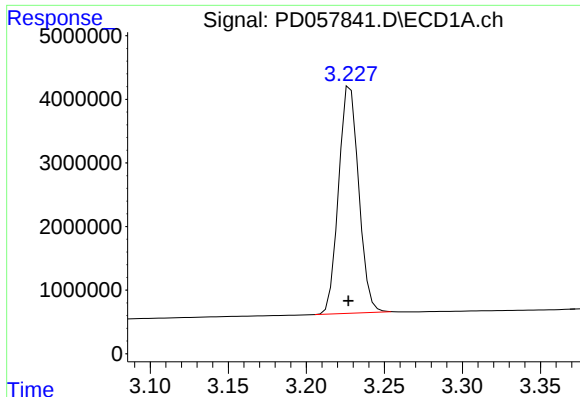

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.001 min
Response: 32084742
Conc: 37.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

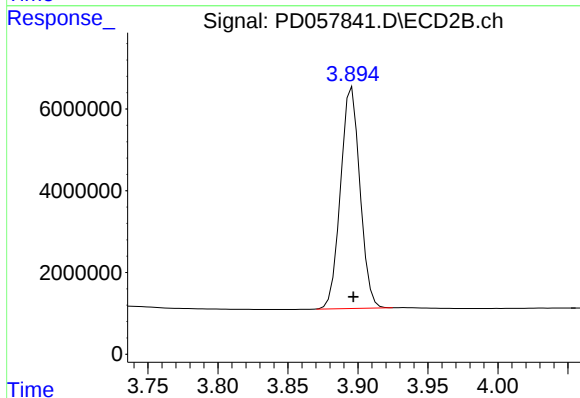


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: -0.001 min
Response: 52258933
Conc: 37.44 ng/ml

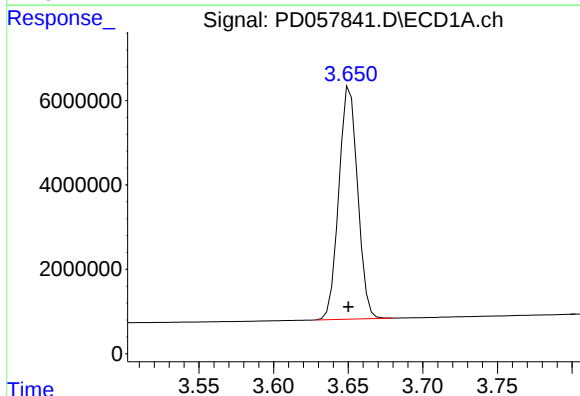


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.001 min
Response: 48419971
Conc: 41.19 ng/ml

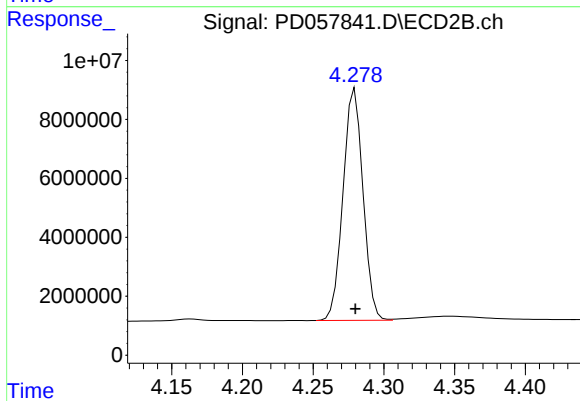

#2 alpha-BHC


R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 77470977
Conc: 40.13 ng/ml

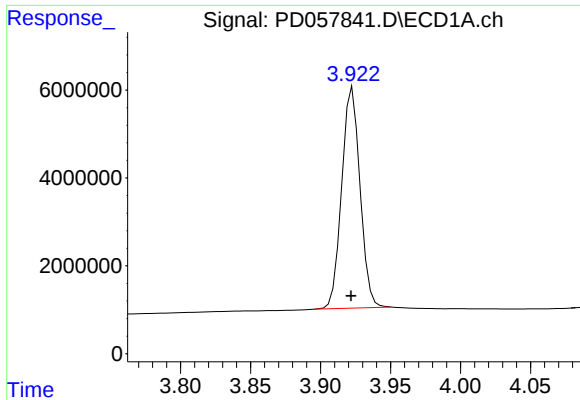

#3 gamma-BHC (Lindane)


R.T.: 3.923 min
Delta R.T.: 0.001 min
Response: 45859028
Conc: 40.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

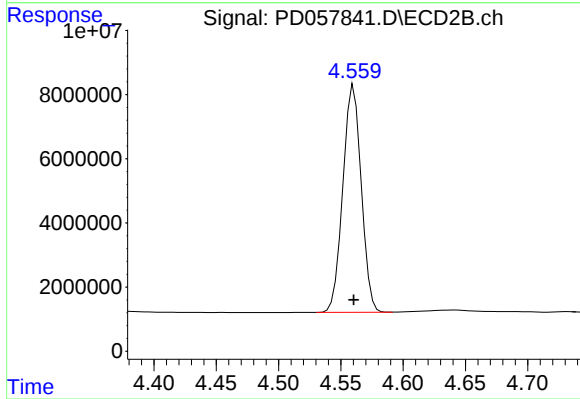


#3 gamma-BHC (Lindane)

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 73064118
Conc: 39.75 ng/ml

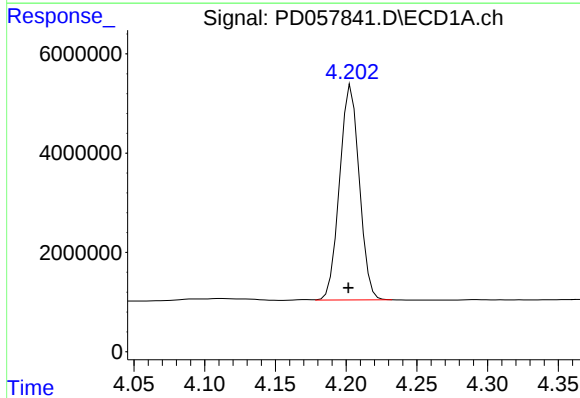


#4 Heptachlor

R.T.: 4.204 min
Delta R.T.: 0.002 min
Response: 42024927
Conc: 39.89 ng/ml

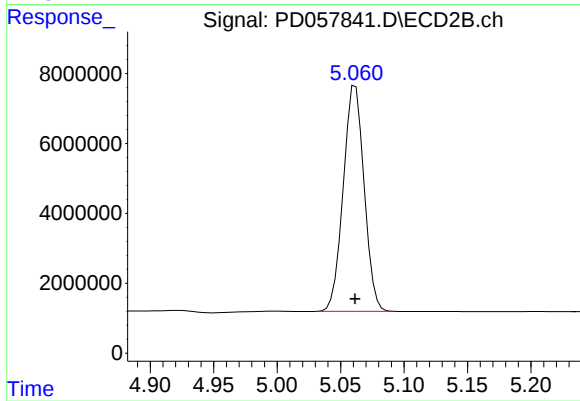

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 73833640
Conc: 38.55 ng/ml

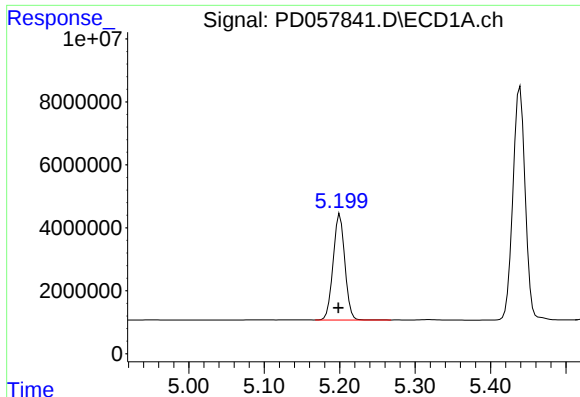

#9 Endosulfan I


R.T.: 5.200 min
Delta R.T.: 0.002 min
Response: 36324880
Conc: 40.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

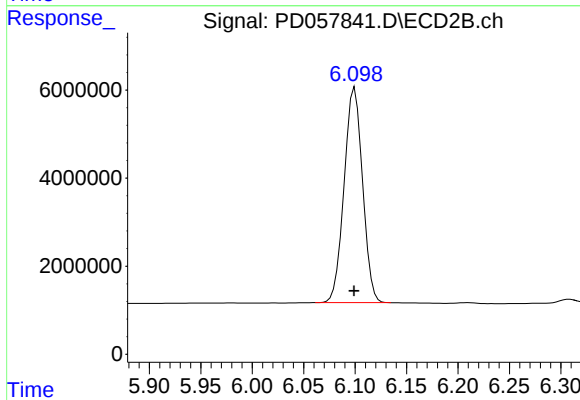


#9 Endosulfan I

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 61012884
Conc: 38.36 ng/ml

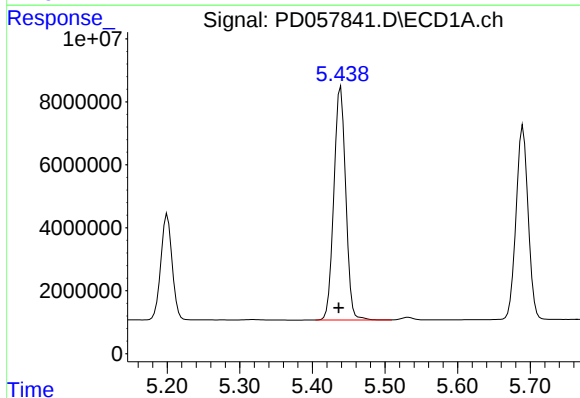


#13 Dieldrin

R.T.: 5.439 min
Delta R.T.: 0.003 min
Response: 84095863
Conc: 81.10 ng/ml

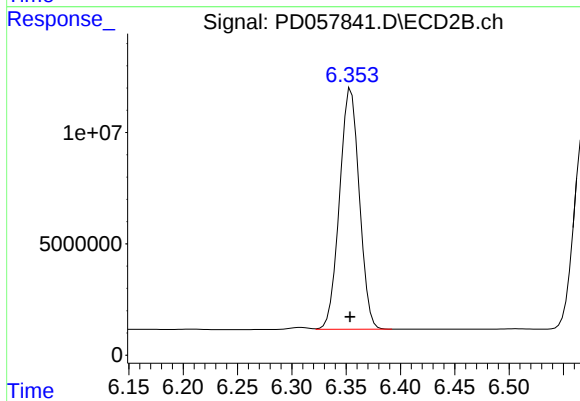

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 137092057
Conc: 78.83 ng/ml

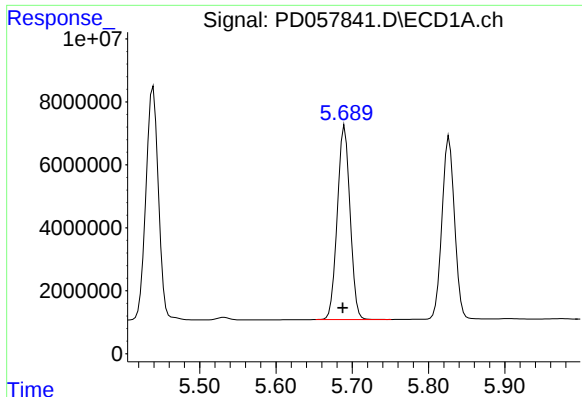

#14 Endrin


R.T.: 5.690 min
Delta R.T.: 0.002 min
Response: 71190369
Conc: 77.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

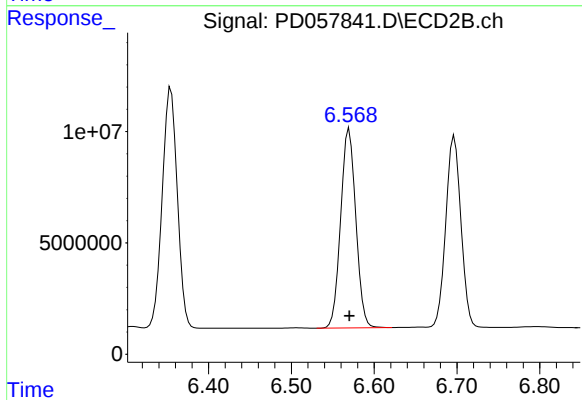


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 113770969
Conc: 70.30 ng/ml

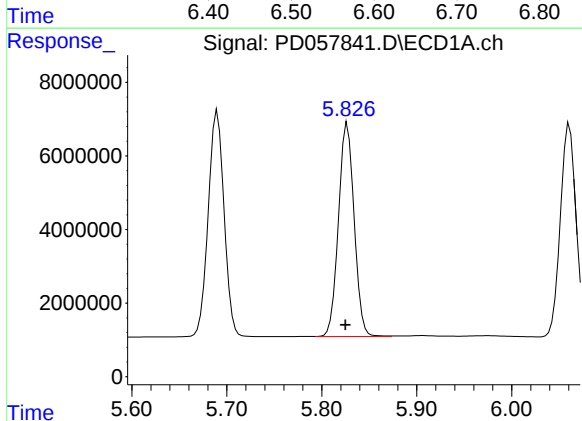


#16 4,4'-DDD

R.T.: 5.827 min
Delta R.T.: 0.002 min
Response: 66647833
Conc: 81.26 ng/ml

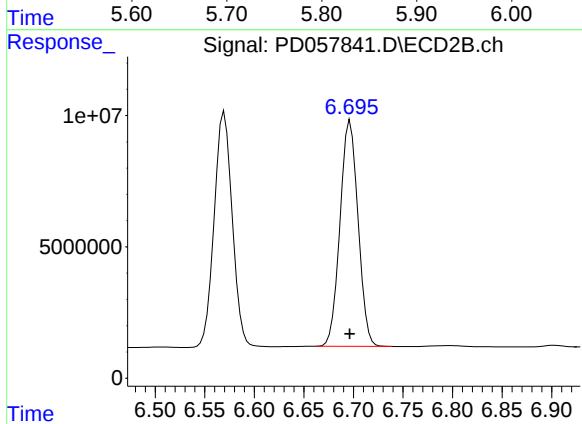

#16 4,4'-DDD


R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 108923809
Conc: 79.58 ng/ml

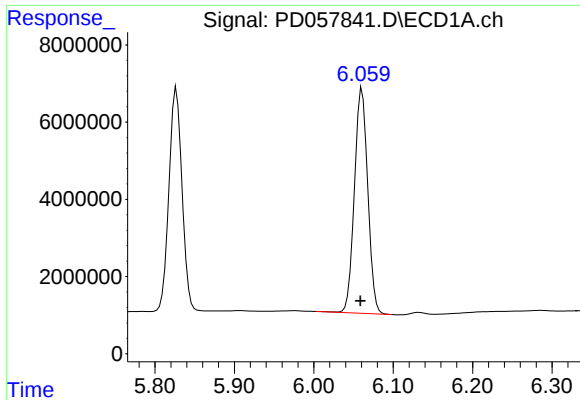

#17 4,4'-DDT


R.T.: 6.061 min
Delta R.T.: 0.002 min
Response: 68000428
Conc: 81.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

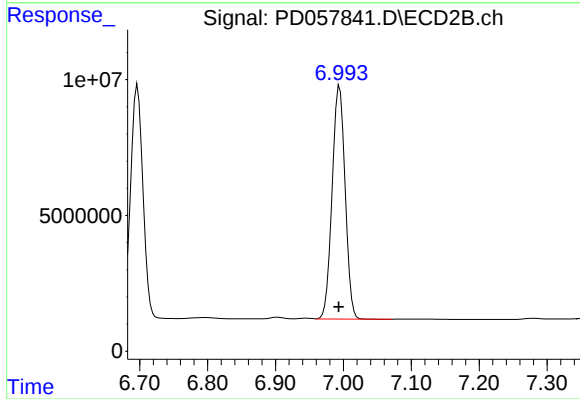


#17 4,4'-DDT

R.T.: 6.994 min
Delta R.T.: 0.000 min
Response: 114240642
Conc: 78.73 ng/ml

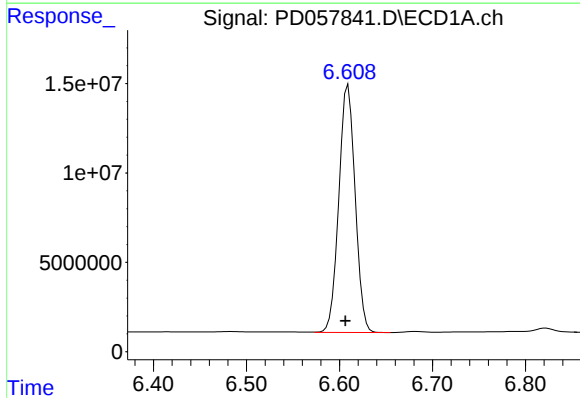


#20 Methoxychlor

R.T.: 6.609 min
Delta R.T.: 0.003 min
Response: 168742476
Conc: 383.11 ng/ml

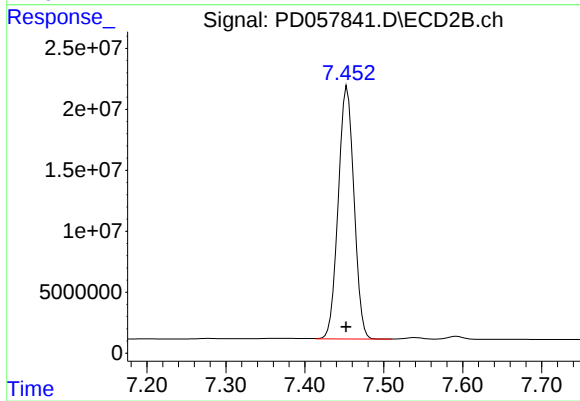

#20 Methoxychlor


R.T.: 7.454 min
Delta R.T.: 0.001 min
Response: 287036912
Conc: 355.77 ng/ml

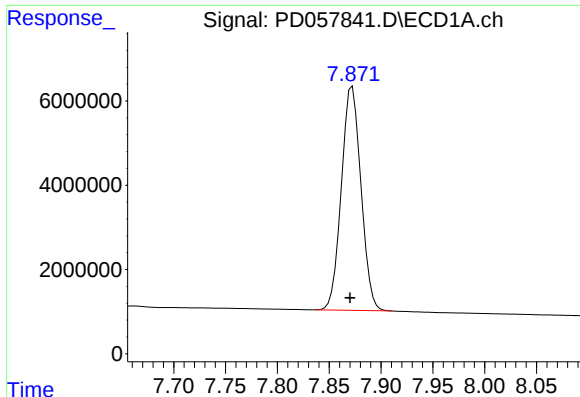

#27 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.002 min
Response: 69929612
Conc: 72.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

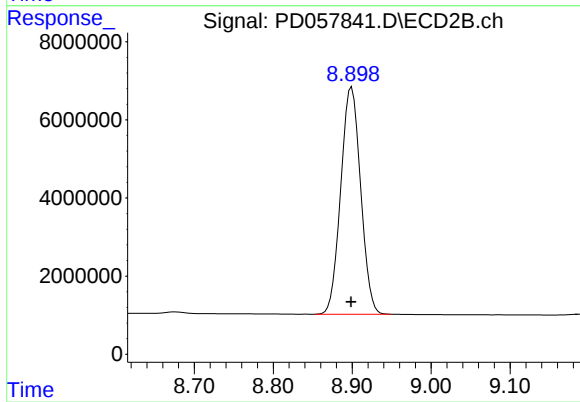

#27 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.000 min
Response: 101862946
Conc: 70.60 ng/ml