

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
 Data File : PD057842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2020 05:44
 Operator : AJ\MA
 Sample : INDB401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDB401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 06:03:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 30 05:55:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.229	3.896	31229565	52013162	39.456	40.206
27)	SA Decachlor...	7.873	8.899	67583260	99383902	76.149	74.581
Target Compounds							
5)	MB Aldrin	4.440	5.362	40744868	71316398	41.002	40.773
6)	B beta-BHC	4.172	4.730	19304501	32491100	39.186	39.821
7)	B delta-BHC	4.364	4.943	45933907	71289111	41.295	42.372
8)	B Heptachlo...	4.873	5.746	37483620	65488339	40.145	39.690
10)	B trans-Chl...	5.093	5.978	38326508	66850880	40.456	40.592
11)	B cis-Chlor...	5.150	6.050	38551480	66954562	40.282	40.293
12)	B 4,4'-DDE	5.319	6.209	76845263	130.8E6	83.009	83.281
15)	B Endosulfa...	5.963	6.779	68433030	111.8E6	80.584	80.495
18)	B Endrin al...	6.132	6.903	57845510	95669766	79.835	79.278
19)	B Endosulfa...	6.341	7.125	69146996	113.2E6	79.936	79.687
21)	B Endrin ke...	6.823	7.592	79392885	121.1E6	80.657	79.514

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 05:44
Operator : AJ\MA
Sample : INDB401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 06:03:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 30 05:55:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

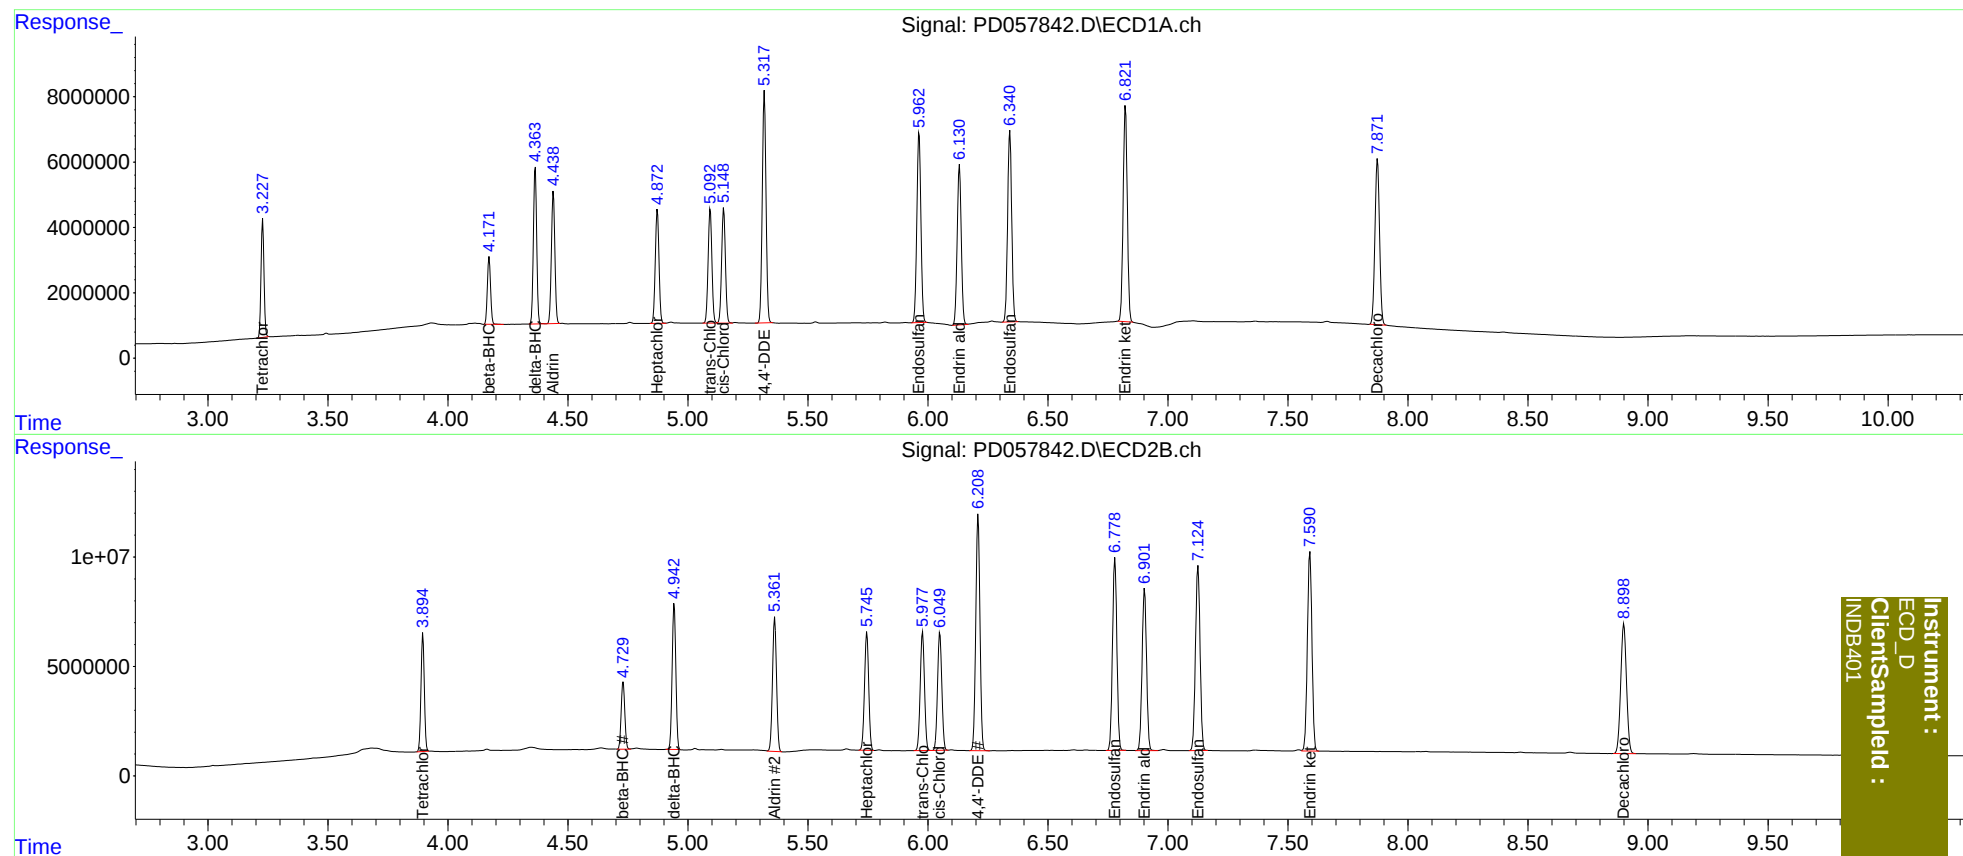


Instrument :
ECD_D
ClientSample :
INDB401

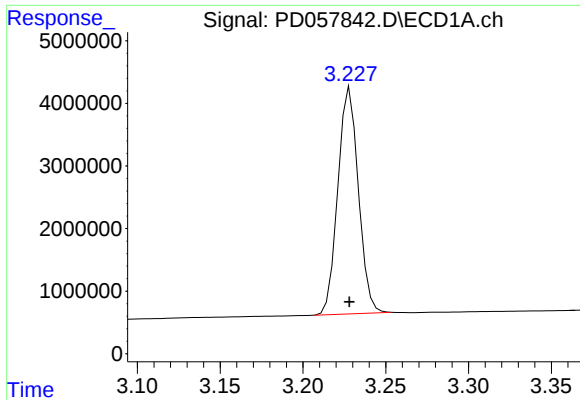

#1 Tetrachloro-m-xylene


R.T.: 3.229 min
Delta R.T.: 0.000 min
Response: 31229565
Conc: 39.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

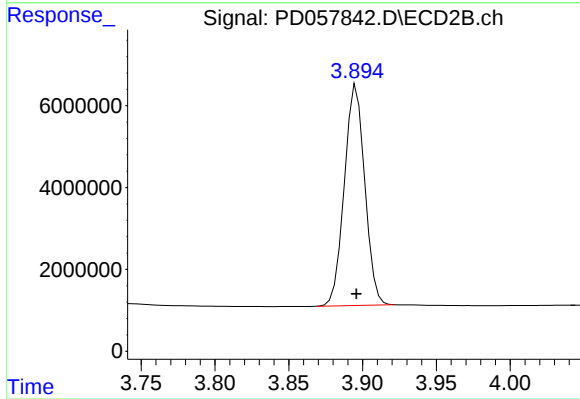


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 52013162
Conc: 40.21 ng/ml

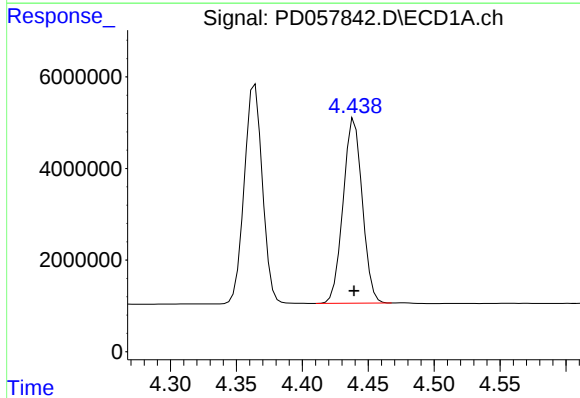


#5 Aldrin

R.T.: 4.440 min
Delta R.T.: 0.000 min
Response: 40744868
Conc: 41.00 ng/ml

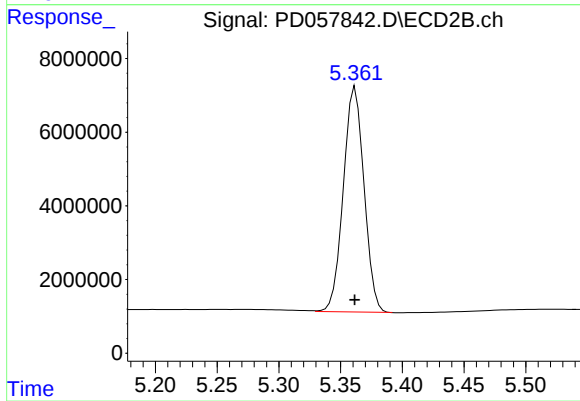

#5 Aldrin


R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 71316398
Conc: 40.77 ng/ml

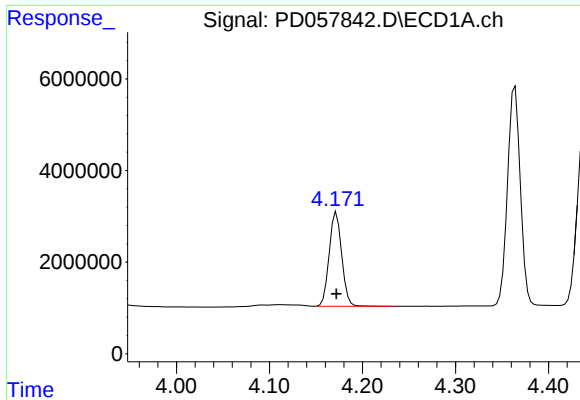

#6 beta-BHC


R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 19304501
Conc: 39.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

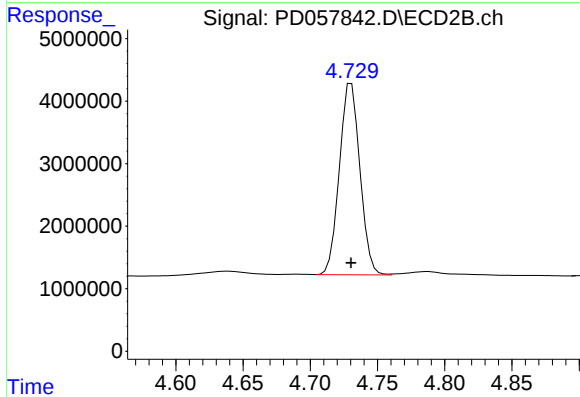


#6 beta-BHC

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 32491100
Conc: 39.82 ng/ml

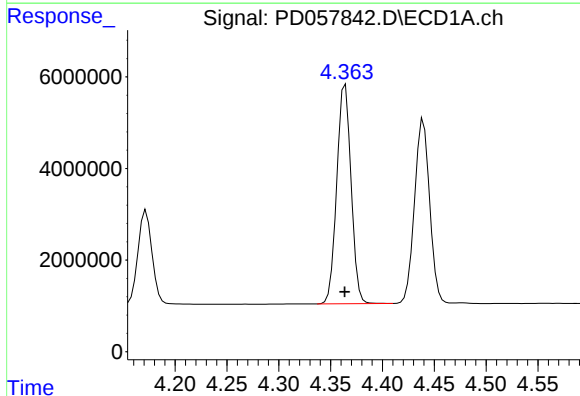


#7 delta-BHC

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 45933907
Conc: 41.30 ng/ml

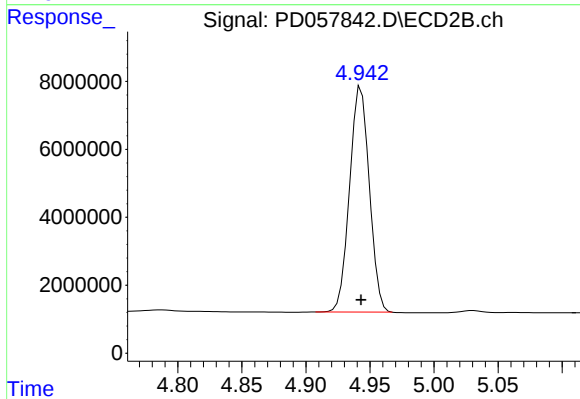

#7 delta-BHC


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 71289111
Conc: 42.37 ng/ml

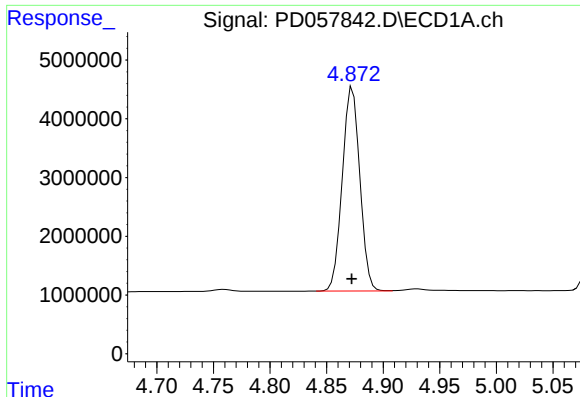

#8 Heptachlor epoxide


R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 37483620
Conc: 40.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

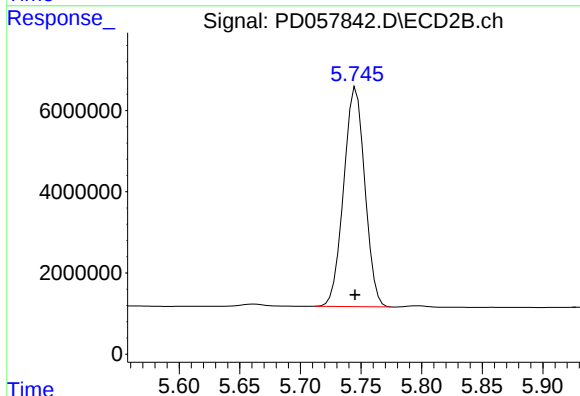


#8 Heptachlor epoxide

R.T.: 5.746 min
Delta R.T.: 0.000 min
Response: 65488339
Conc: 39.69 ng/ml

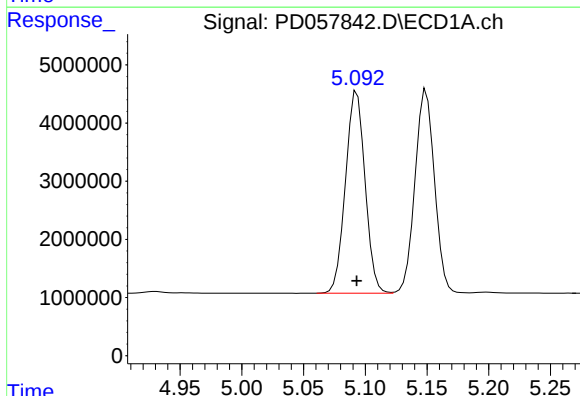


#10 trans-Chlordane

R.T.: 5.093 min
Delta R.T.: 0.000 min
Response: 38326508
Conc: 40.46 ng/ml

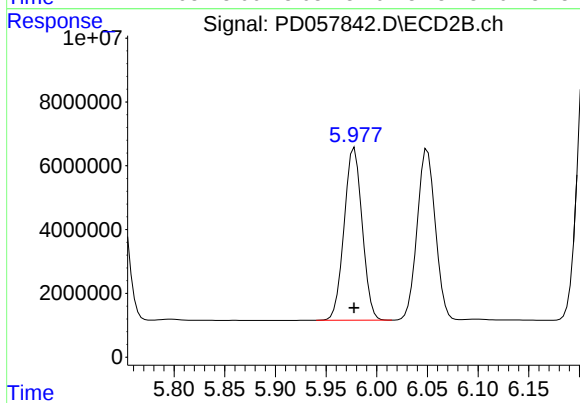

#10 trans-Chlordane


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 66850880
Conc: 40.59 ng/ml

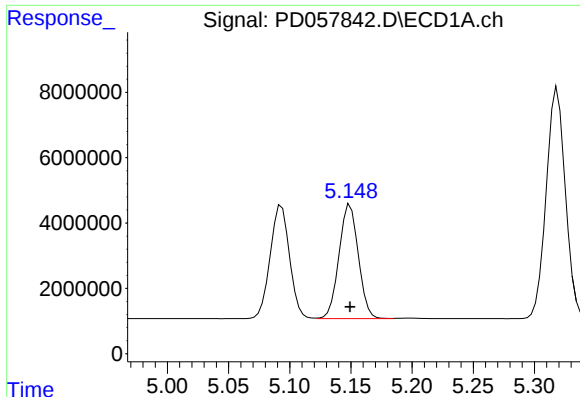

#11 cis-Chlordane


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 38551480
Conc: 40.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

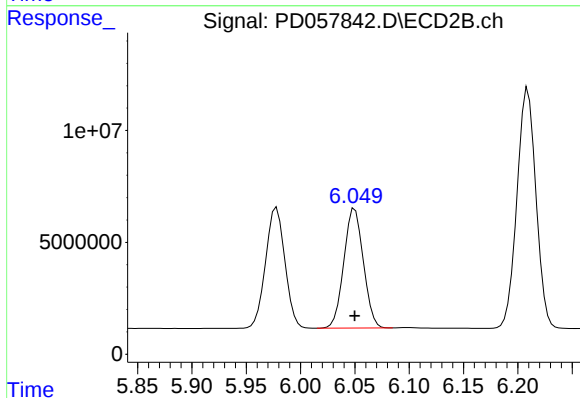


#11 cis-Chlordane

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 66954562
Conc: 40.29 ng/ml

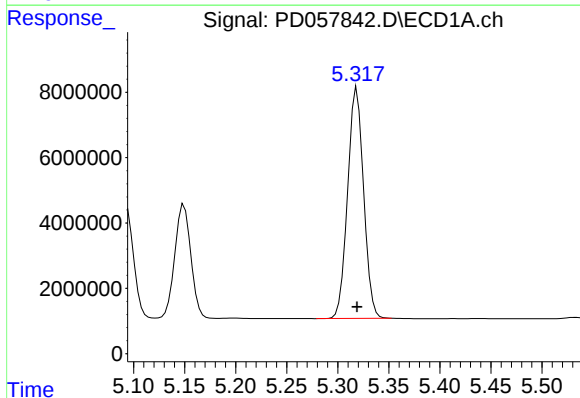


#12 4,4'-DDE

R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 76845263
Conc: 83.01 ng/ml

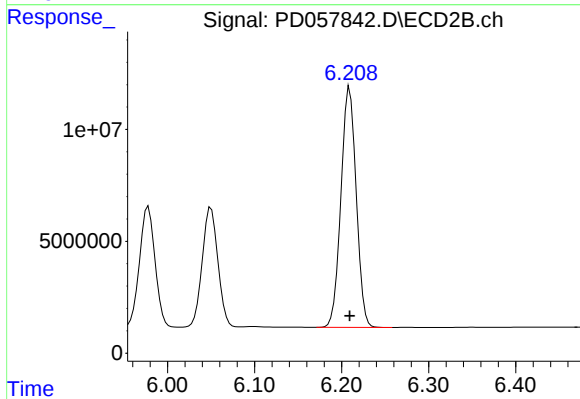

#12 4,4'-DDE


R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 130810116
Conc: 83.28 ng/ml

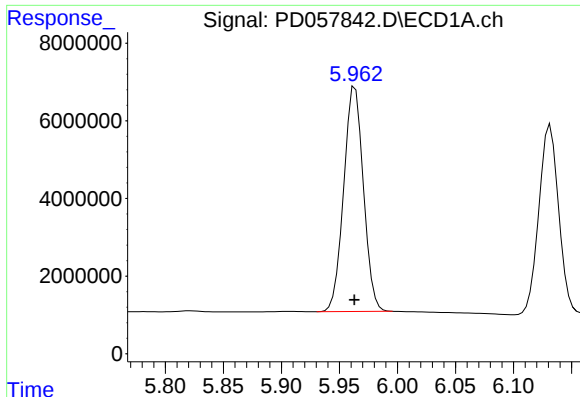

#15 Endosulfan II


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 68433030
Conc: 80.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

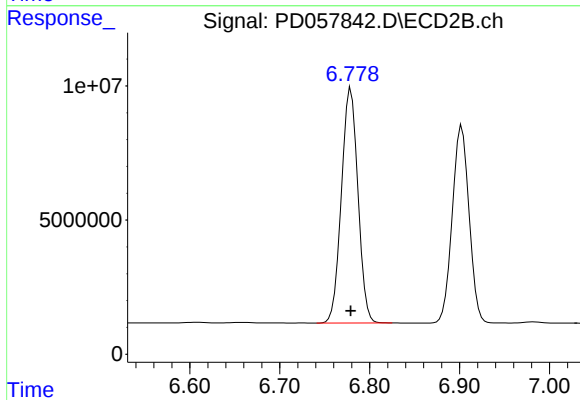


#15 Endosulfan II

R.T.: 6.779 min
Delta R.T.: 0.000 min
Response: 111821685
Conc: 80.50 ng/ml

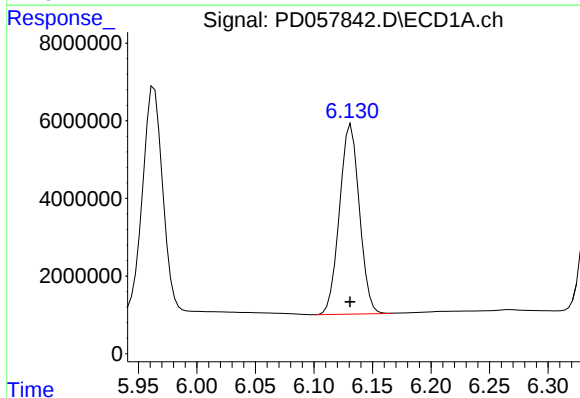


#18 Endrin aldehyde

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 57845510
Conc: 79.84 ng/ml

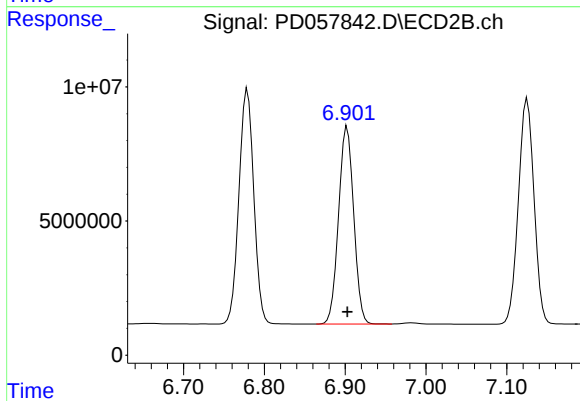

#18 Endrin aldehyde


R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 95669766
Conc: 79.28 ng/ml

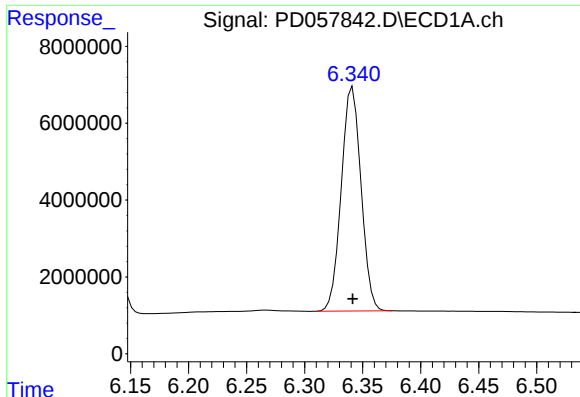

#19 Endosulfan Sulfate


R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 69146996
Conc: 79.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

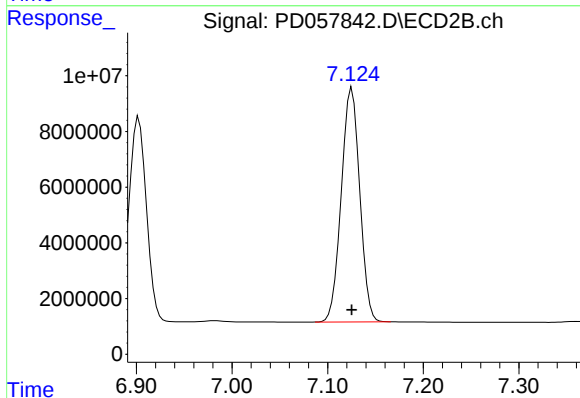


#19 Endosulfan Sulfate

R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 113183444
Conc: 79.69 ng/ml

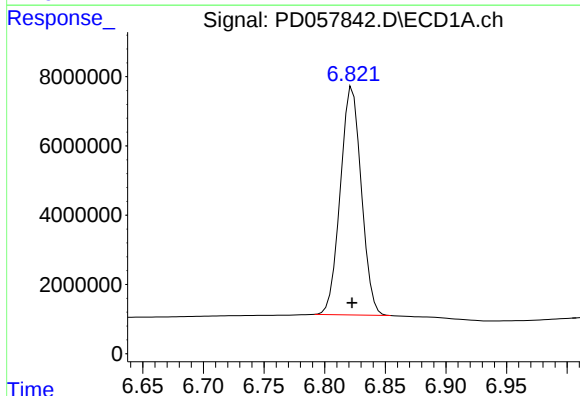


#21 Endrin ketone

R.T.: 6.823 min
Delta R.T.: 0.000 min
Response: 79392885
Conc: 80.66 ng/ml

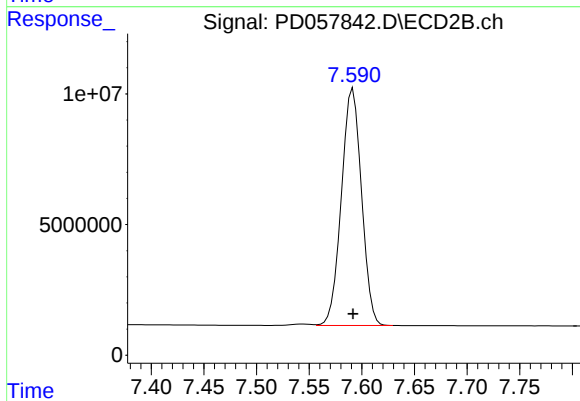

#21 Endrin ketone


R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 121055928
Conc: 79.51 ng/ml

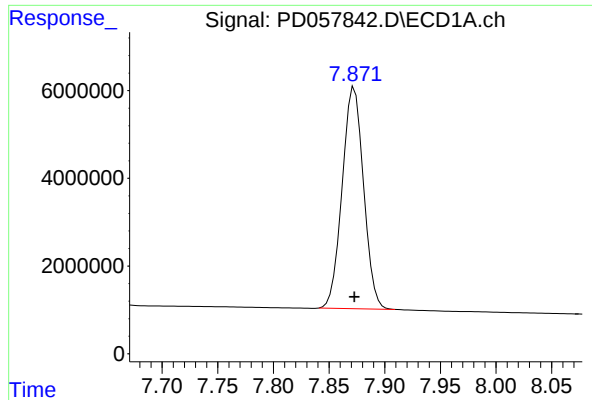

#27 Decachlorobiphenyl

R.T.: 7.873 min
Delta R.T.: 0.000 min
Response: 67583260
Conc: 76.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDB401

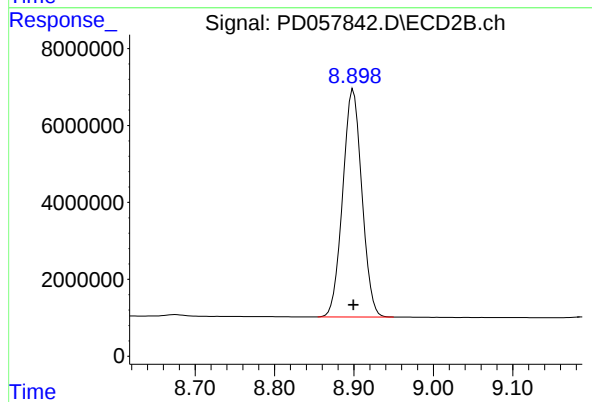

#27 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.000 min
Response: 99383902
Conc: 74.58 ng/ml