

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
 Data File : PD057843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2020 05:58
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 07:18:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 30 06:57:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.896	62879838	102.4E6	74.301	73.405
27)	SA Decachlor...	7.872	8.900	132.4E6	190.0E6	138.017	131.720
Target Compounds							
2)	A alpha-BHC	3.651	4.279	100.9E6	160.6E6	85.833	83.201
3)	MA gamma-BHC...	3.923	4.560	93699282	149.5E6	82.099	81.339
4)	MA Heptachlor	4.203	5.062	85698085	149.4E6	81.353	78.001
9)	A Endosulfan I	5.200	6.100	71857796	122.1E6	79.734	76.784
13)	MA Dieldrin	5.438	6.354	170.9E6	276.9E6	164.851	159.195
14)	MA Endrin	5.690	6.571	145.7E6	234.7E6	158.722	144.992
16)	A 4,4'-DDD	5.827	6.697	134.7E6	218.0E6	164.186	159.275
17)	MA 4,4'-DDT	6.061	6.995	139.9E6	231.0E6	167.927	159.211
20)	A Methoxychlor	6.609	7.453	325.5E6	555.0E6	739.037	687.856


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 05:58
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 07:18:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 30 06:57:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

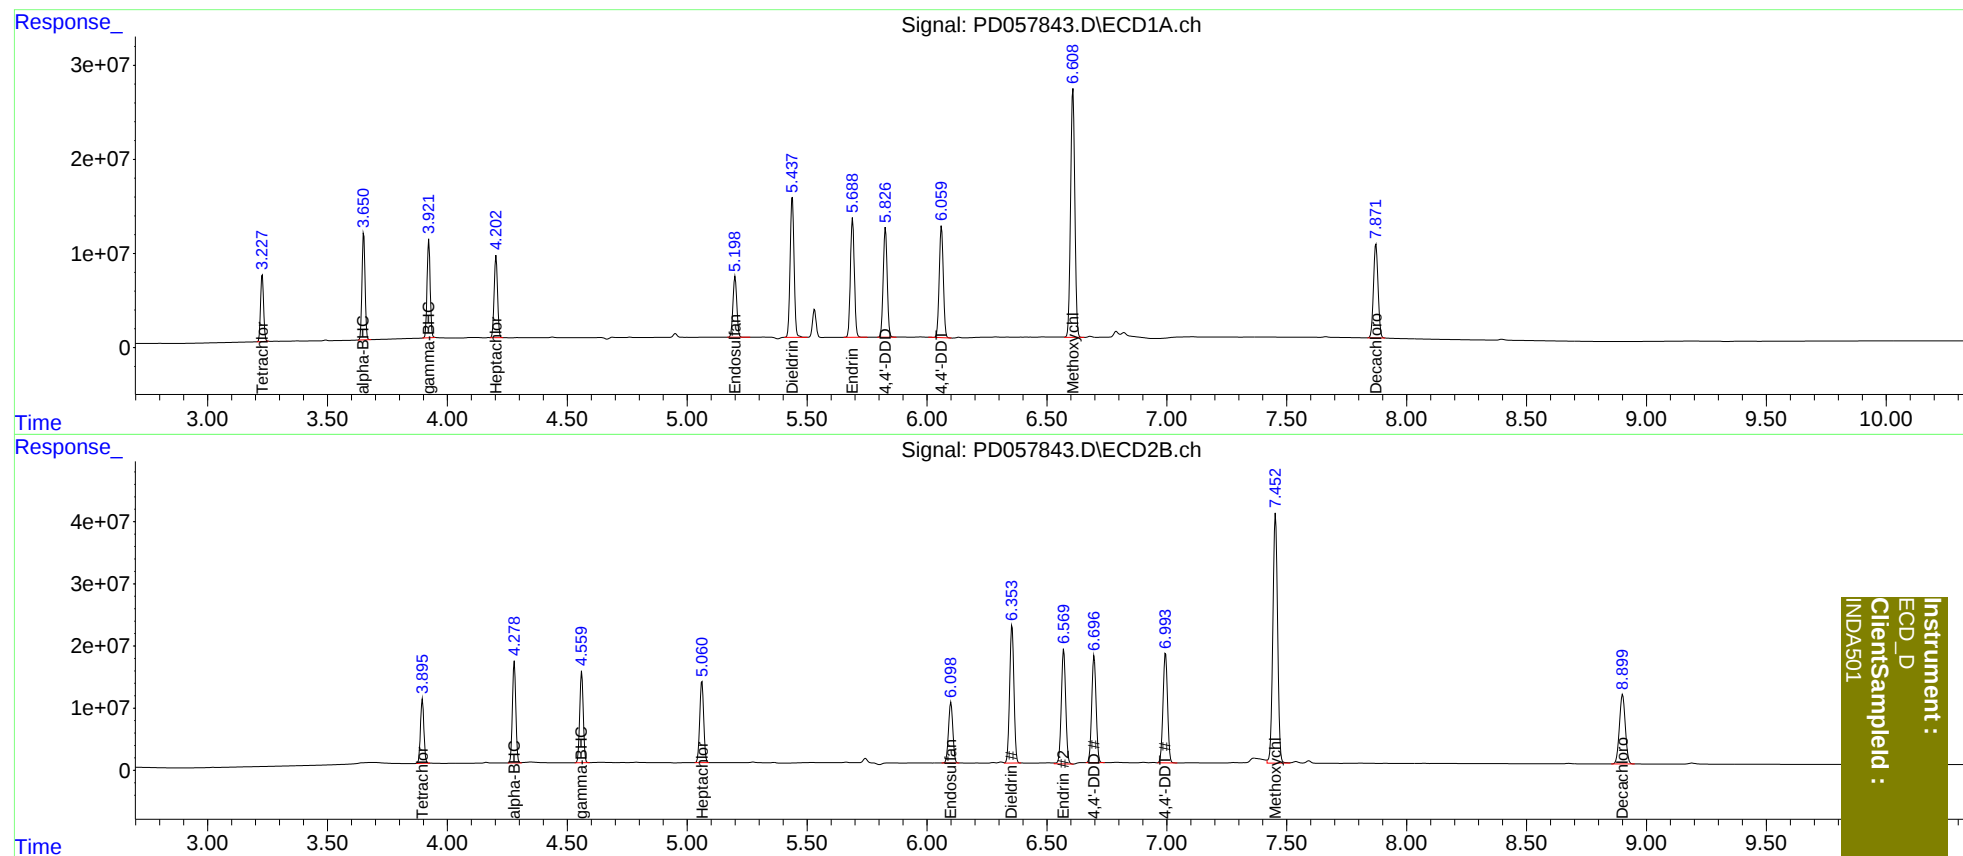


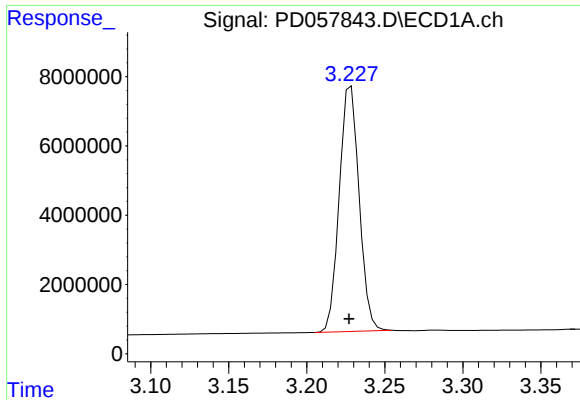

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.001 min
Response: 62879838
Conc: 74.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

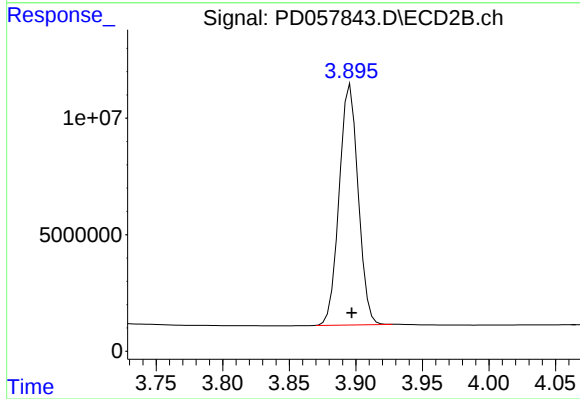


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 102448266
Conc: 73.40 ng/ml

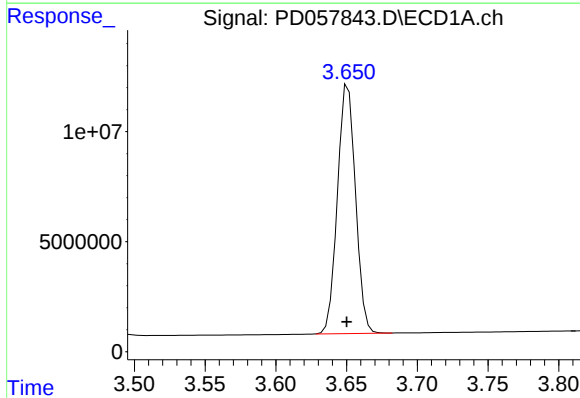


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.001 min
Response: 100903221
Conc: 85.83 ng/ml

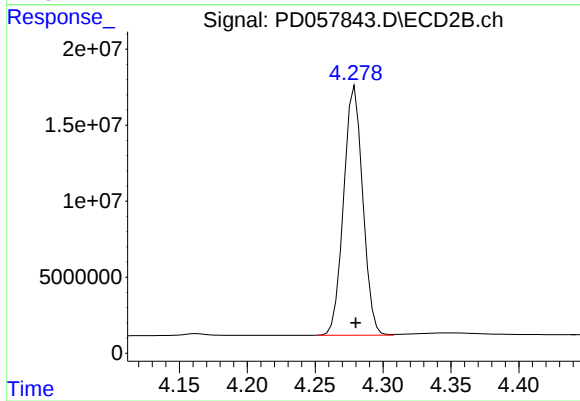

#2 alpha-BHC


R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 160601891
Conc: 83.20 ng/ml

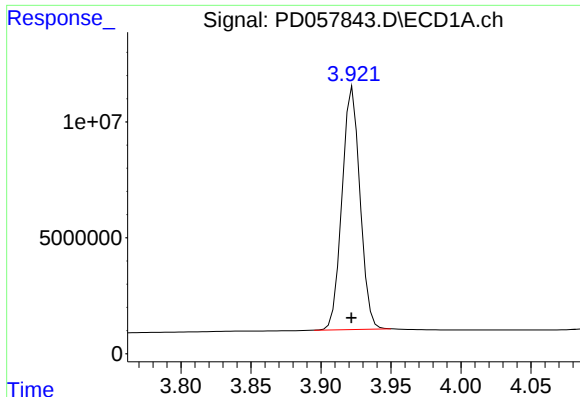

#3 gamma-BHC (Lindane)


R.T.: 3.923 min
Delta R.T.: 0.001 min
Response: 93699282
Conc: 82.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

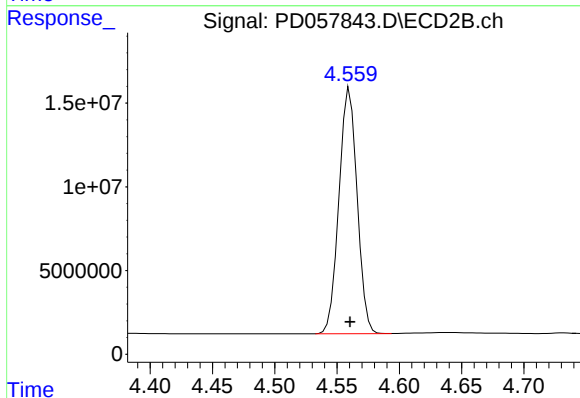


#3 gamma-BHC (Lindane)

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 149510065
Conc: 81.34 ng/ml

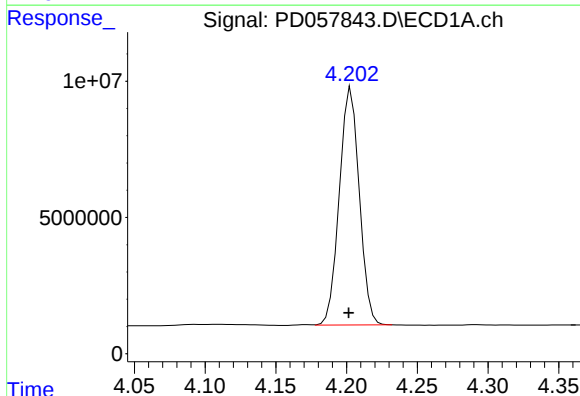


#4 Heptachlor

R.T.: 4.203 min
Delta R.T.: 0.002 min
Response: 85698085
Conc: 81.35 ng/ml

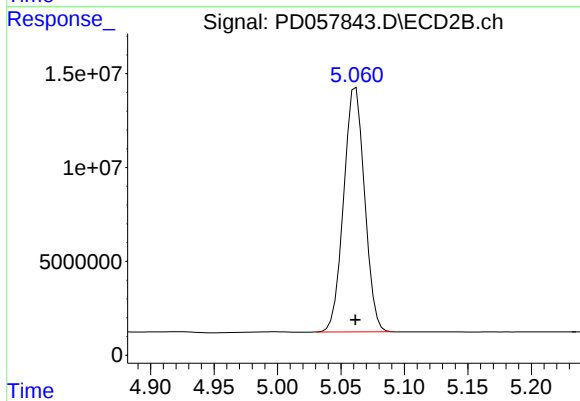

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 149401286
Conc: 78.00 ng/ml

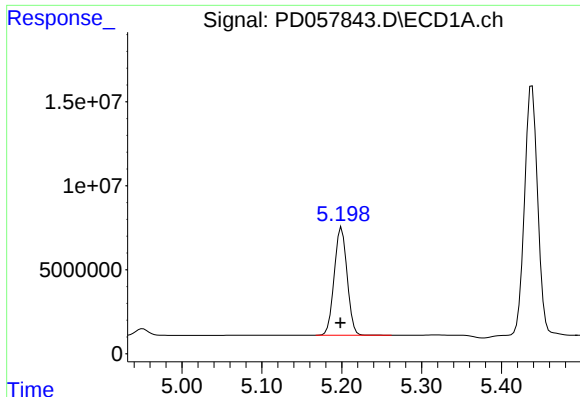

#9 Endosulfan I


R.T.: 5.200 min
Delta R.T.: 0.002 min
Response: 71857796
Conc: 79.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

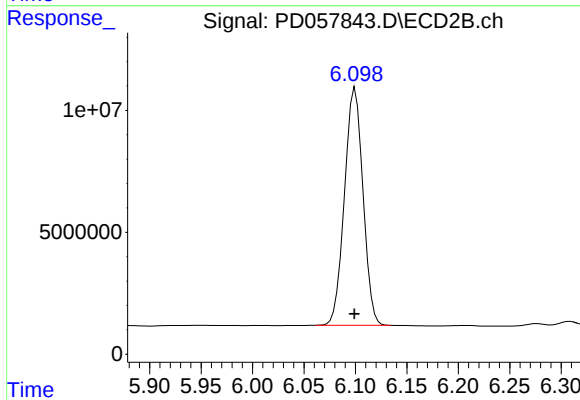


#9 Endosulfan I

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 122115434
Conc: 76.78 ng/ml

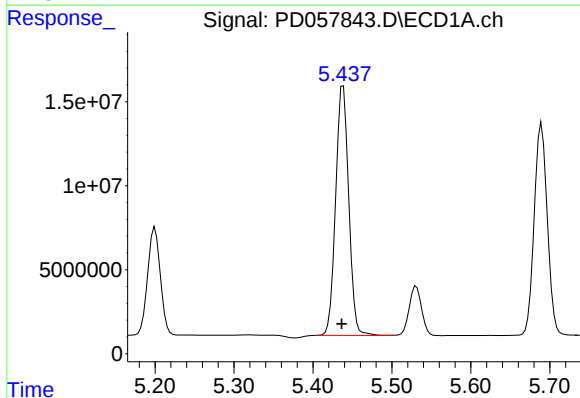


#13 Dieldrin

R.T.: 5.438 min
Delta R.T.: 0.002 min
Response: 170941088
Conc: 164.85 ng/ml

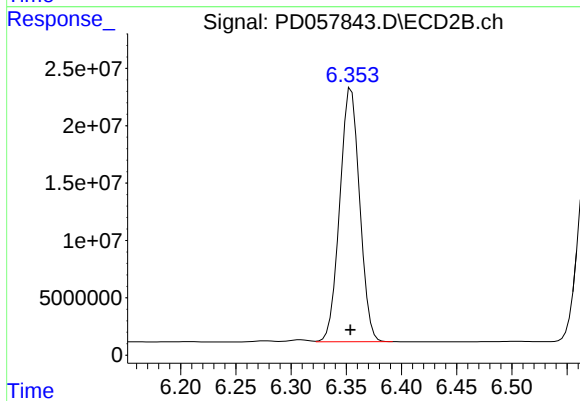

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 276861528
Conc: 159.19 ng/ml

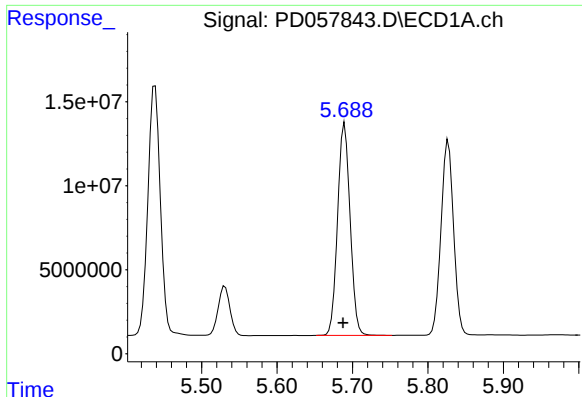

#14 Endrin


R.T.: 5.690 min
Delta R.T.: 0.002 min
Response: 145738306
Conc: 158.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

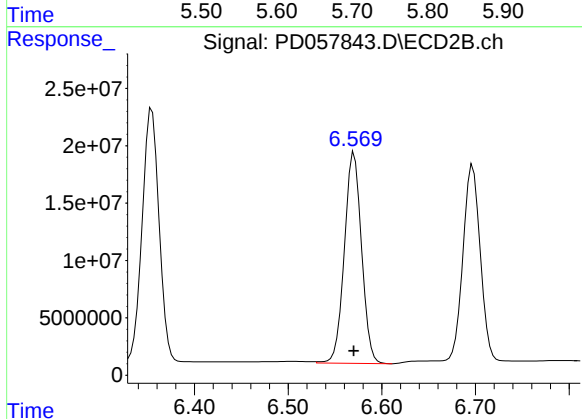


#14 Endrin

R.T.: 6.571 min
Delta R.T.: 0.000 min
Response: 234657504
Conc: 144.99 ng/ml

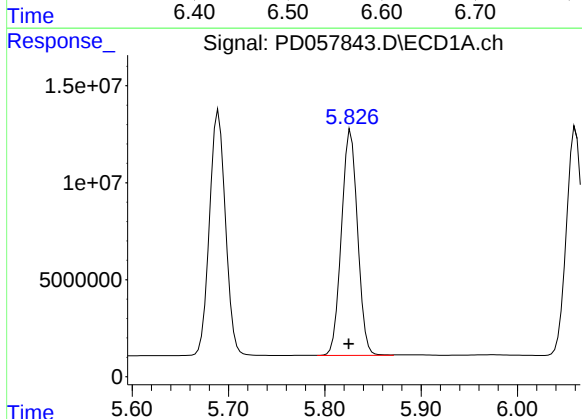


#16 4,4'-DDD

R.T.: 5.827 min
Delta R.T.: 0.002 min
Response: 134665681
Conc: 164.19 ng/ml

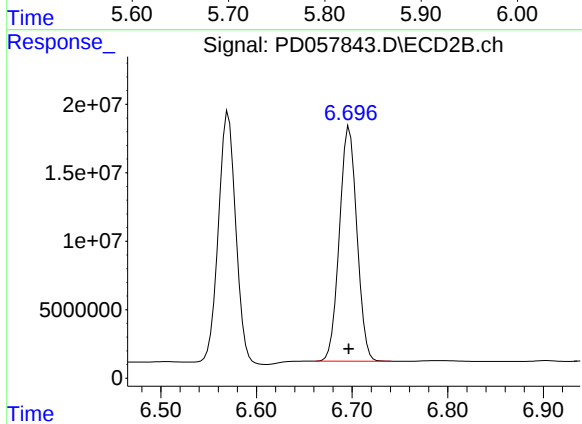

#16 4,4'-DDD


R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 217992062
Conc: 159.28 ng/ml

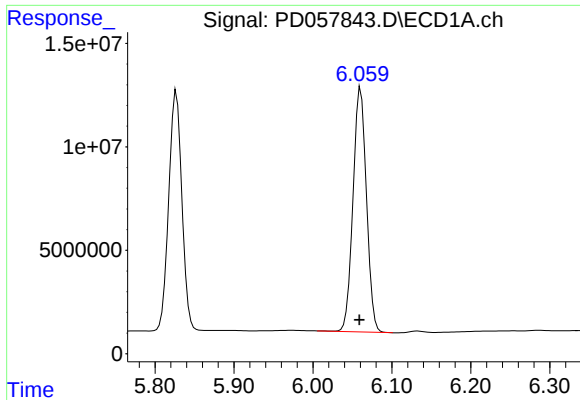

#17 4,4'-DDT


R.T.: 6.061 min
Delta R.T.: 0.002 min
Response: 139922737
Conc: 167.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

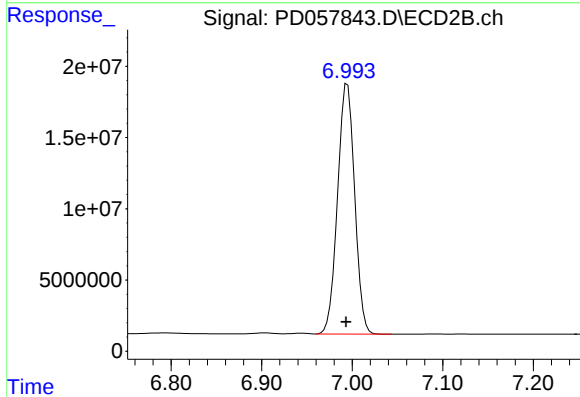


#17 4,4'-DDT

R.T.: 6.995 min
Delta R.T.: 0.001 min
Response: 231035678
Conc: 159.21 ng/ml

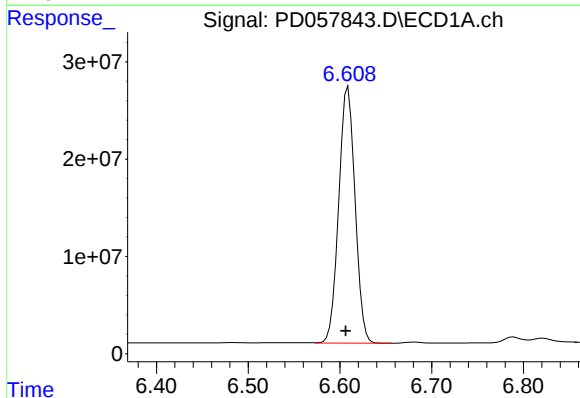


#20 Methoxychlor

R.T.: 6.609 min
Delta R.T.: 0.002 min
Response: 325511901
Conc: 739.04 ng/ml

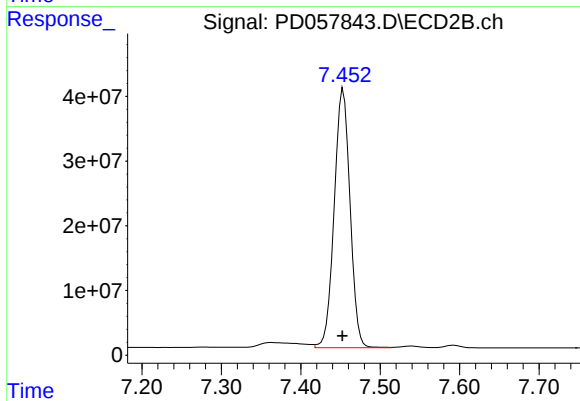

#20 Methoxychlor


R.T.: 7.453 min
Delta R.T.: 0.001 min
Response: 554971492
Conc: 687.86 ng/ml

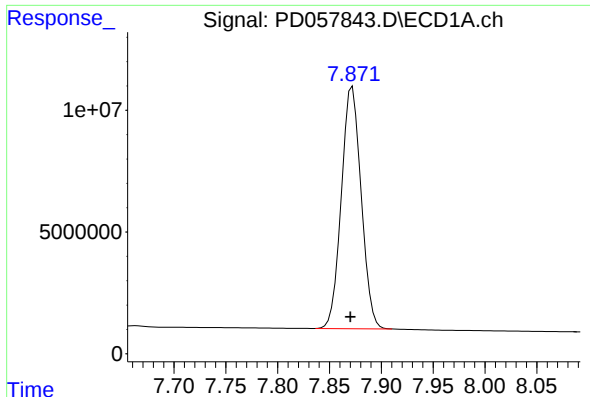

#27 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.002 min
Response: 132367865
Conc: 138.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

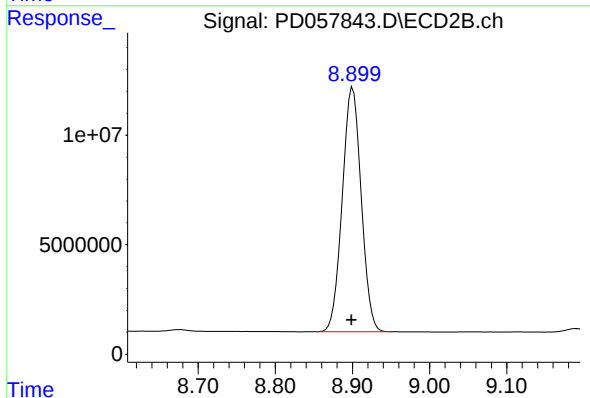

#27 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.002 min
Response: 190040033
Conc: 131.72 ng/ml