

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
 Data File : PD057828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2020 02:27
 Operator : AJ\MA
 Sample : RESC02
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 07:36:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 30 07:30:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.229	3.895	16169296	26461985	19.365	19.272
27)	SA Decachlor...	7.874	8.898	36146123	54423128	37.604	37.585
Target Compounds							
2)	A alpha-BHC	3.652	4.278	10919705	17765547	9.387	9.351
3)	MA gamma-BHC...	3.923	4.559	10910134	17117701	9.307	9.476
4)	MA Heptachlor	4.204	5.060	9885022	17692712	9.520	9.507
5)	MB Aldrin	4.440	5.361	10178620	18073184	10.115	10.222
6)	B beta-BHC	4.173	4.730	5031422	8638366	10.283	10.610
7)	B delta-BHC	4.364	4.943	10991109	17139380	9.774	10.023
8)	B Heptachlo...	4.873	5.745	9512696	16962931	10.130	9.437
9)	A Endosulfan I	5.200	6.098	8881384	15322615	9.902	9.791
10)	B trans-Chl...	5.093	5.978	9741606	16992977	10.165	10.178
11)	B cis-Chlor...	5.150	6.049	9933406	17320273	10.255	10.289
12)	B 4,4'-DDE	5.319	6.208	18421251	31327430	19.679	19.857
13)	MA Dieldrin	5.439	6.353	19416918	32314788	18.913	18.982
14)	MA Endrin	5.691	6.570	17148391	27569788	19.066	18.174
15)	B Endosulfa...	5.964	6.778	17257467	28501489	20.158	20.272
16)	A 4,4'-DDD	5.828	6.696	15546674	25530165	19.131	19.072
17)	MA 4,4'-DDT	6.062	6.993	14684959	26863715	17.890	18.911
18)	B Endrin al...	6.132	6.902	14681938	24759997	20.202	20.224
19)	B Endosulfa...	6.342	7.124	17685529	29281794	20.264	20.363
20)	A Methoxychlor	6.610	7.452	41386515	75910750	96.175	98.078
21)	B Endrin ke...	6.824	7.591	21064546	31911439	20.537	20.830

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 02:27
Operator : AJ\MA
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 07:36:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 30 07:30:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

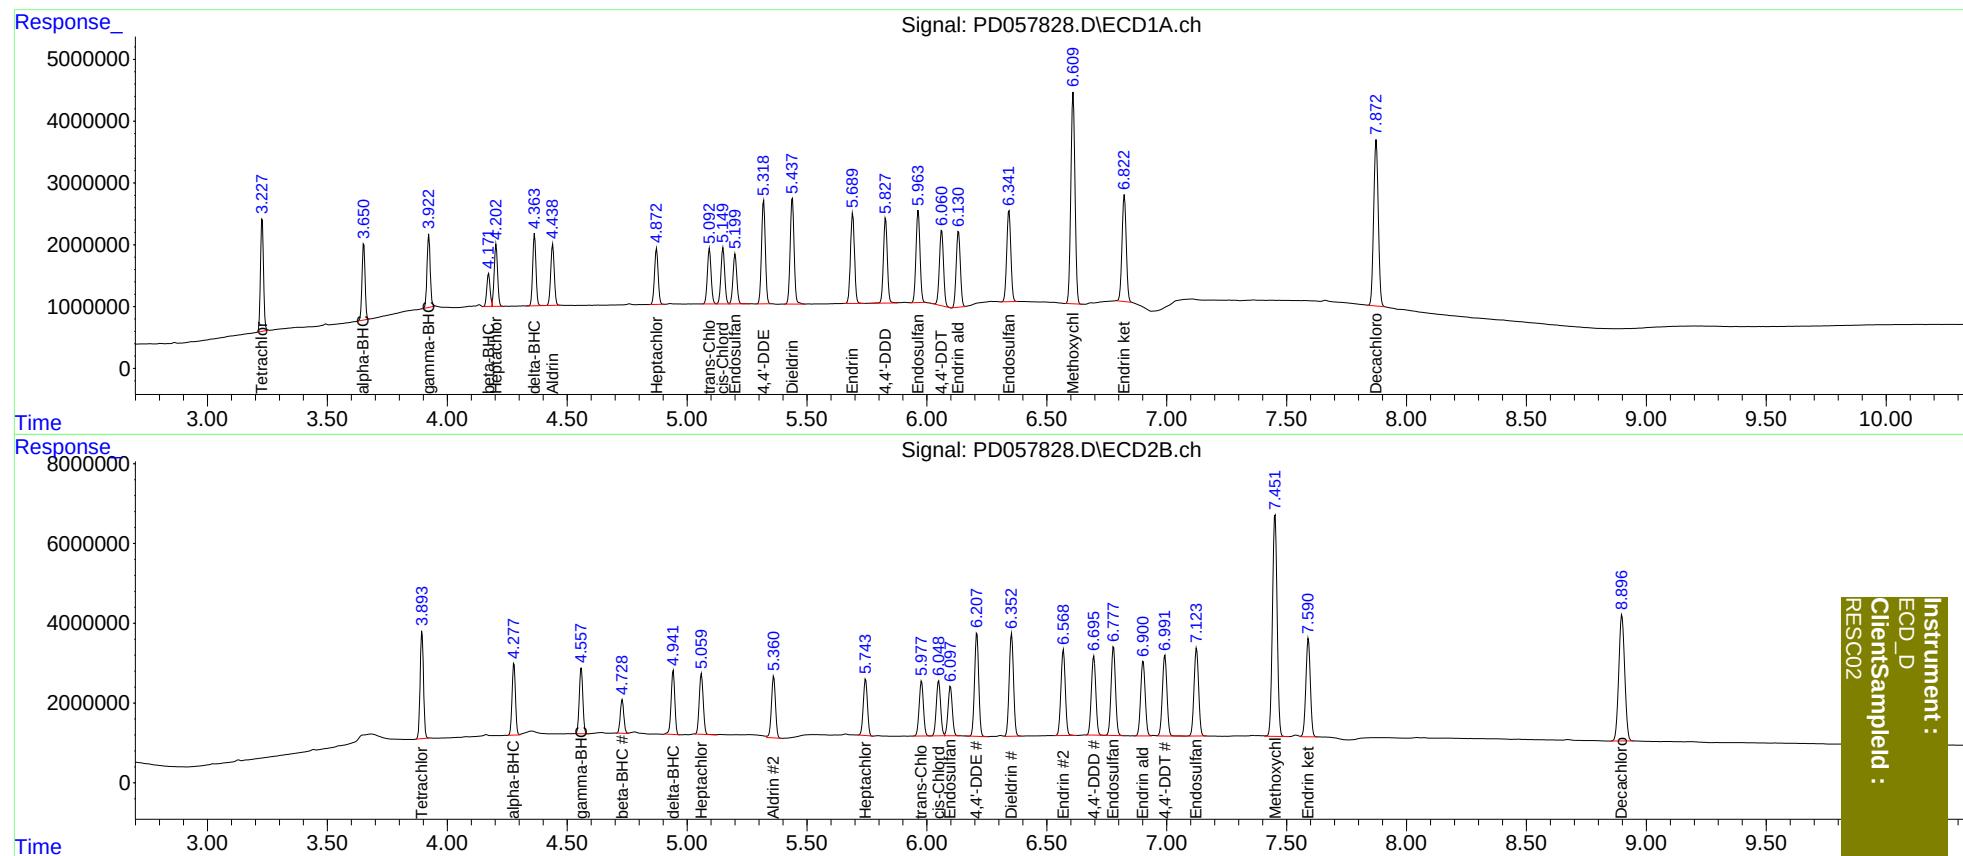

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057828.D
Acq On : 30 Apr 2020 02:27
Operator : AJ\MA
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Title : GC Extractables
Last Update : Thu Apr 30 07:30:11 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.229	3.652	100.00%
3.652	3.923	100.00%
3.923	4.173	100.00%
4.173	4.204	86.81%
4.204	4.364	100.00%
4.364	4.440	100.00%
4.440	4.873	100.00%
4.873	5.093	100.00%
5.093	5.150	100.00%
5.150	5.200	100.00%
5.200	5.319	100.00%
5.319	5.439	100.00%
5.439	5.691	100.00%
5.691	5.828	100.00%
5.828	5.964	100.00%
5.964	6.062	100.00%
6.062	6.132	100.00%
6.132	6.342	100.00%
6.342	6.610	100.00%
6.610	6.824	100.00%
6.824	7.874	100.00%

Signal #2


3.895	4.278	100.00%
4.278	4.559	100.00%
4.559	4.730	100.00%
4.730	4.943	100.00%
4.943	5.060	100.00%
5.060	5.361	100.00%
5.361	5.745	100.00%
5.745	5.978	100.00%
5.978	6.049	100.00%
6.049	6.098	97.32%
6.098	6.208	100.00%
6.208	6.353	100.00%
6.353	6.570	100.00%
6.570	6.696	100.00%
6.696	6.778	100.00%
6.778	6.902	100.00%
6.902	6.993	100.00%
6.993	7.124	100.00%
7.124	7.452	100.00%
7.452	7.591	100.00%
7.591	8.898	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 02:27
Operator : AJ\MA
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 07:36:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 30 07:30:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

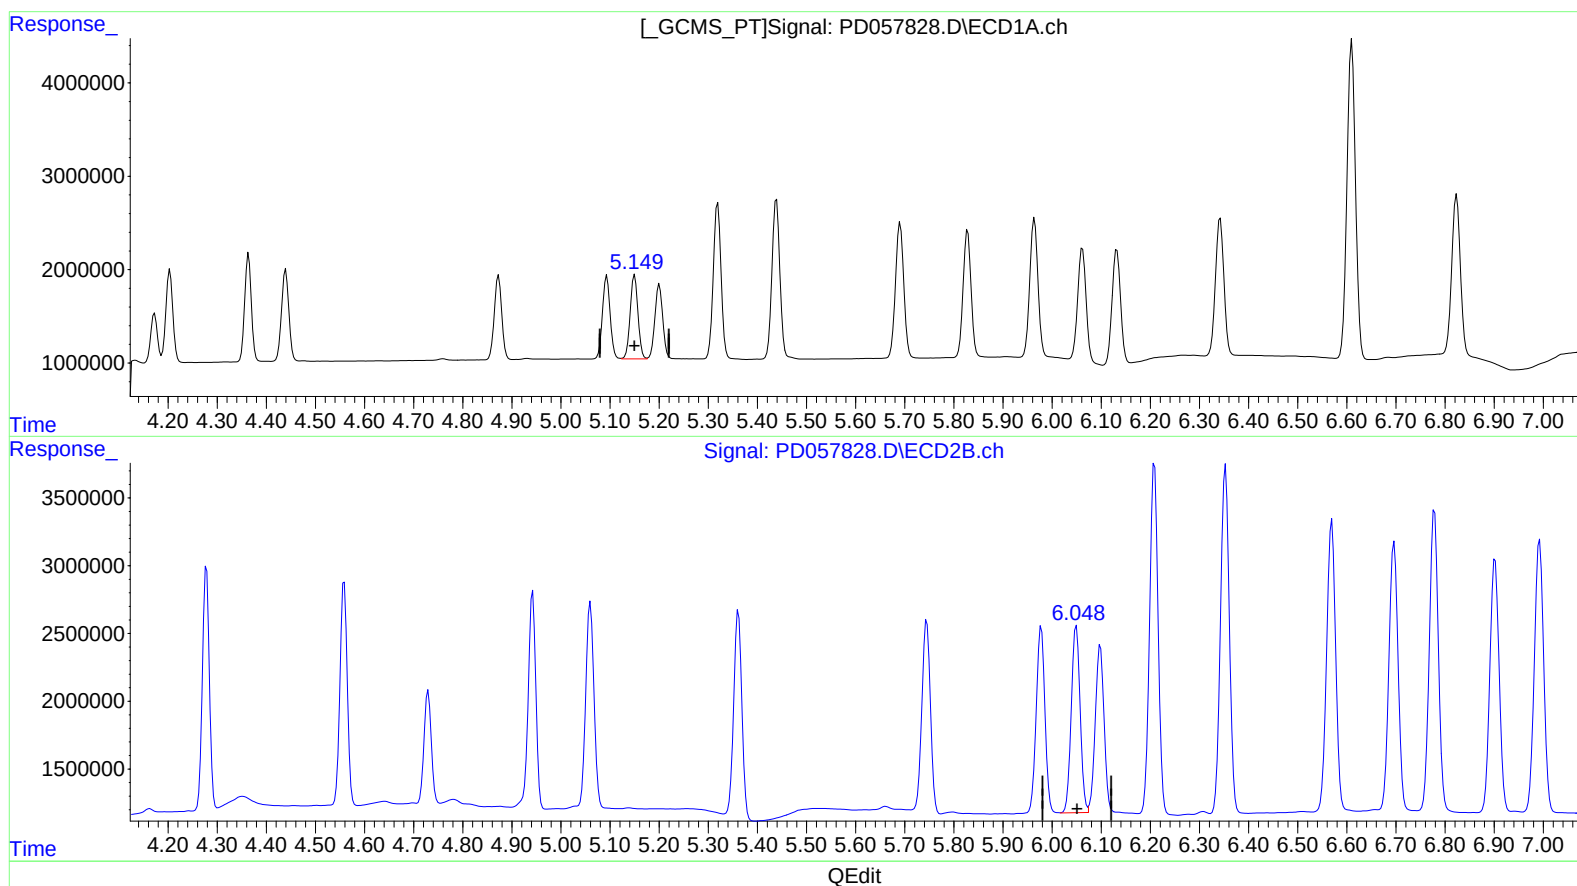

(11) cis-Chlordane (B)

5.150min 10.255 ng/ml

response 9933406

(11) cis-Chlordane #2 (B)

6.049min 10.289 ng/ml


response 17320273

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042920\
Data File : PD057828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 02:27
Operator : AJ\MA
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 07:36:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042920CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 30 07:30:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

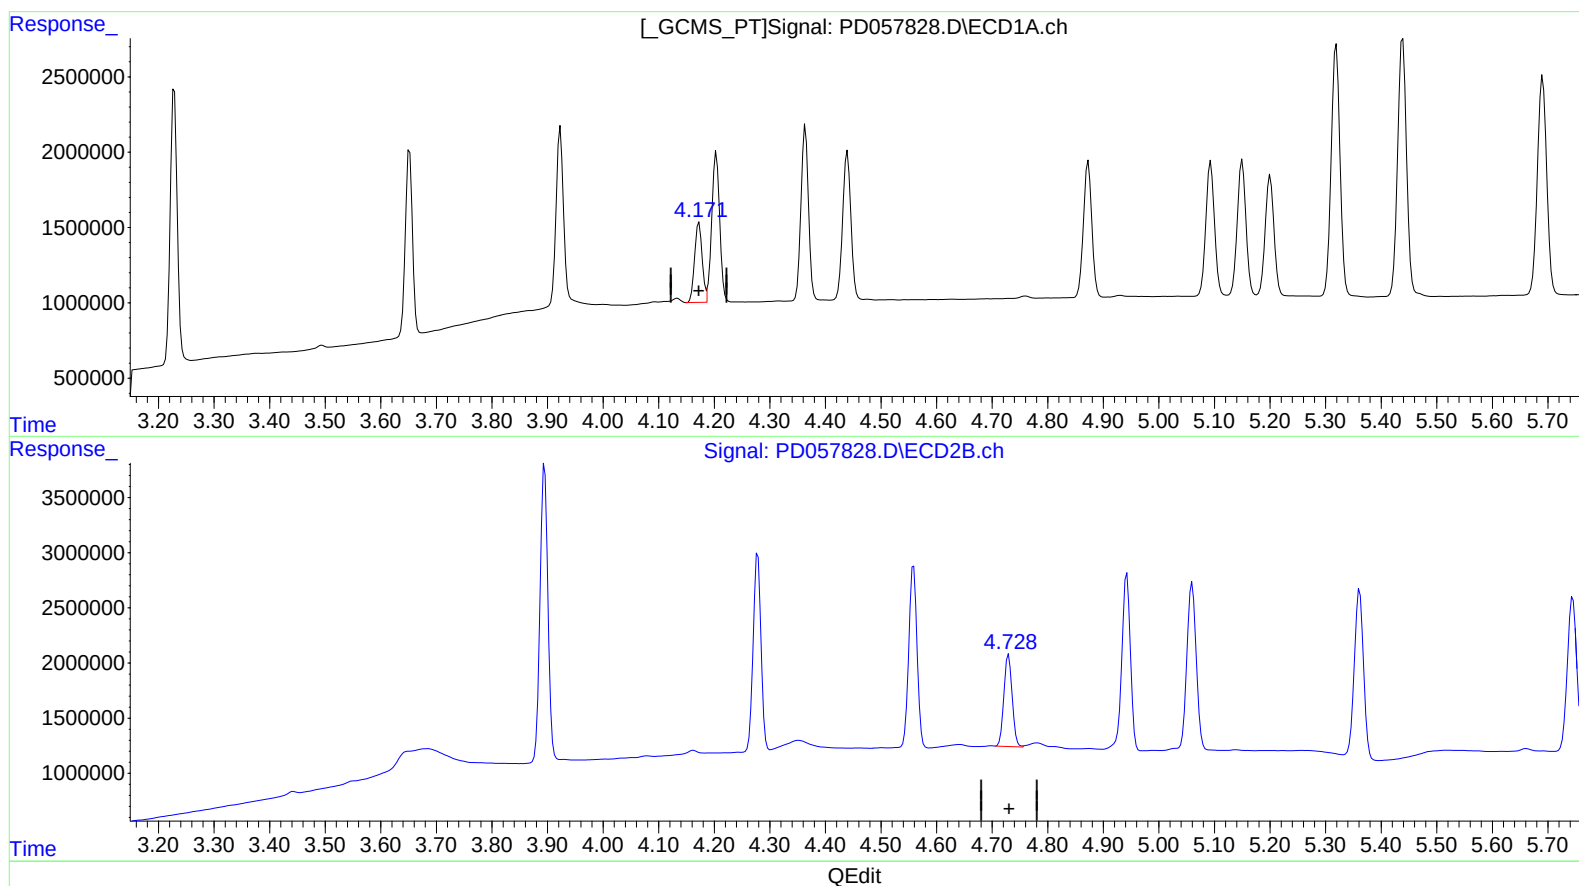

(6) beta-BHC (B)

4.173min 10.283 ng/ml

response 5031422

(6) beta-BHC #2 (B)

4.730min 10.610 ng/ml

response 8638366