

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 10:40
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 12:30:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 29 12:30:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.973	4890166	64439488	5.103	5.240
27)	SA Decachlor...	8.202	9.034	10805827	114.3E6	9.861	10.265
Target Compounds							
2)	A alpha-BHC	3.878	4.362	6671051	99684393	4.769	5.210
3)	MA gamma-BHC...	4.161	4.646	6632402	90232661	5.000	5.159
4)	MA Heptachlor	4.463	5.155	6256383	92147790	4.862	5.205
9)	A Endosulfan I	5.494	6.202	5629582	78556133	5.030	5.290
13)	MA Dieldrin	5.737	6.459	12124662	161.3E6	9.570	10.191
14)	MA Endrin	5.995	6.677	10420959	129.6E6	9.811	10.215
16)	A 4,4'-DDD	6.121	6.799	9295599	129.6E6	9.196	10.267
17)	MA 4,4'-DDT	6.363	7.098	7895809	116.6E6	8.256	9.560
20)	A Methoxychlor	6.909	7.556	26127700	300.1E6	47.397	51.352


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 10:40
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 12:30:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 29 12:30:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

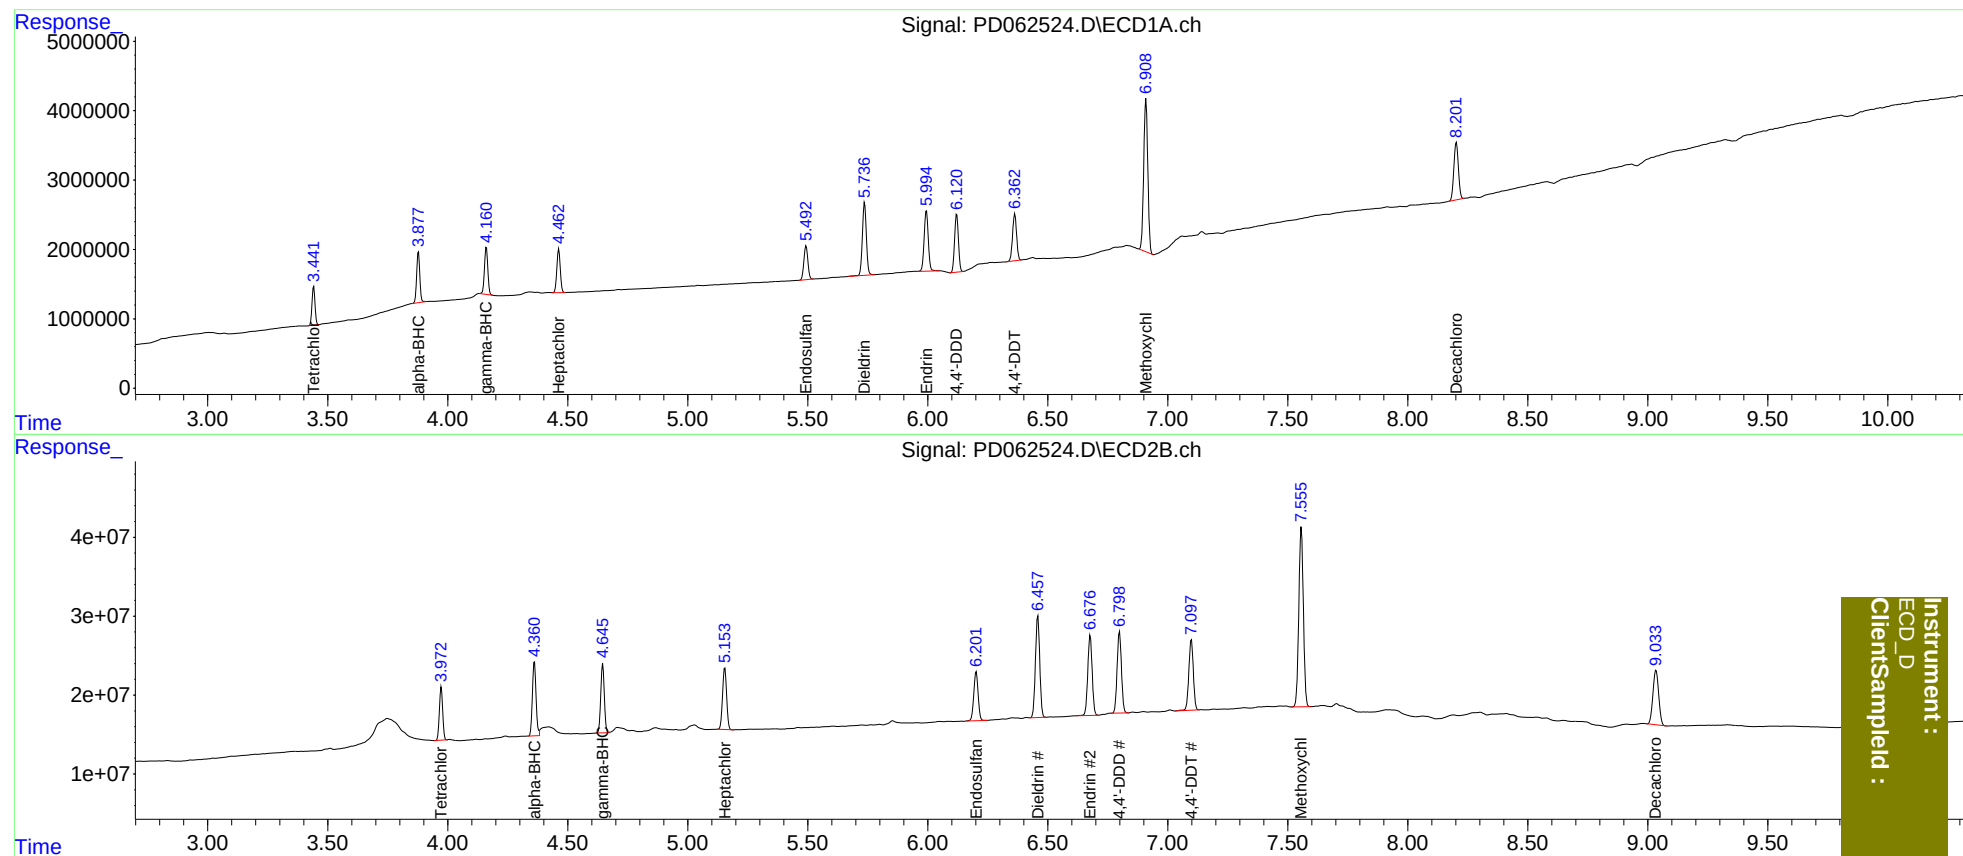


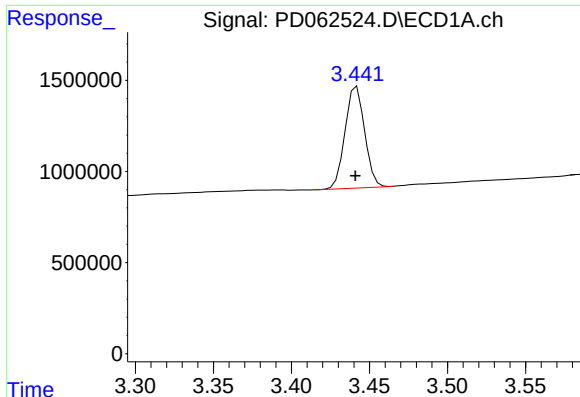

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 4890166
Conc: 5.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

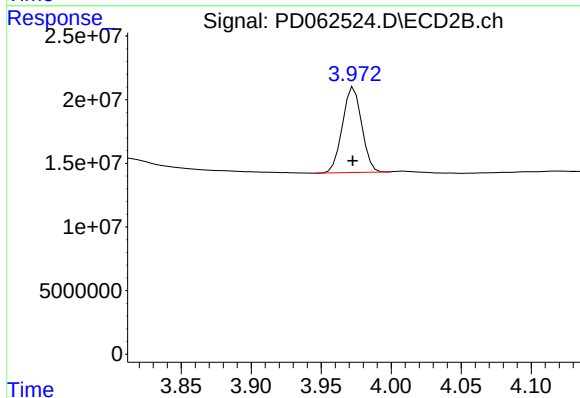


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 64439488
Conc: 5.24 ng/ml

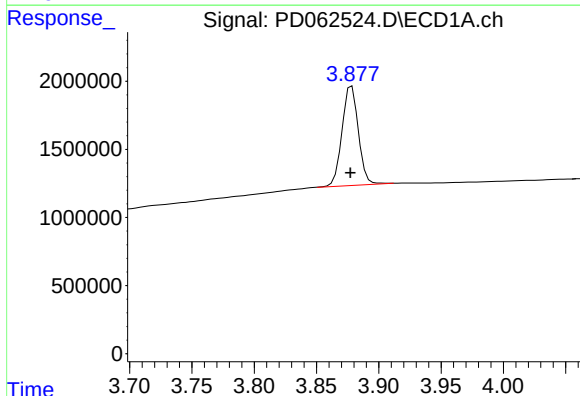


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 6671051
Conc: 4.77 ng/ml

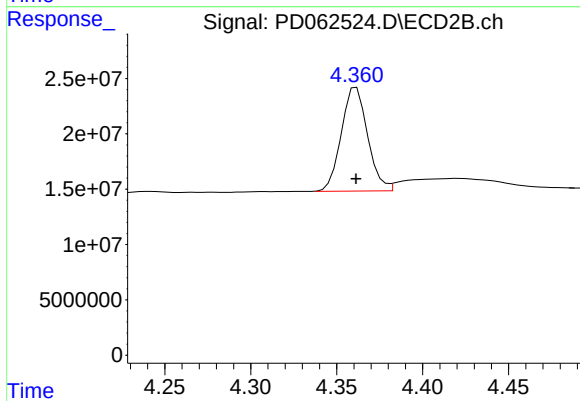

#2 alpha-BHC


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 99684393
Conc: 5.21 ng/ml

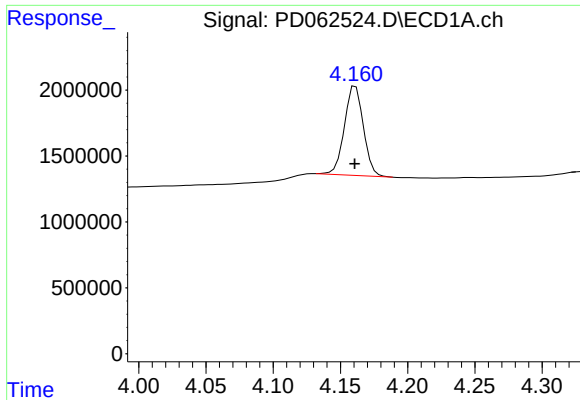

#3 gamma-BHC (Lindane)


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 6632402
Conc: 5.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

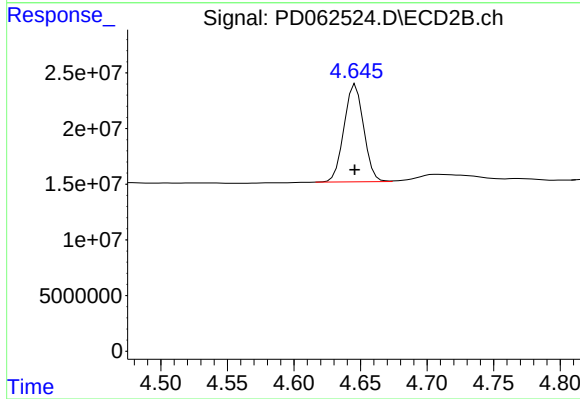


#3 gamma-BHC (Lindane)

R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 90232661
Conc: 5.16 ng/ml

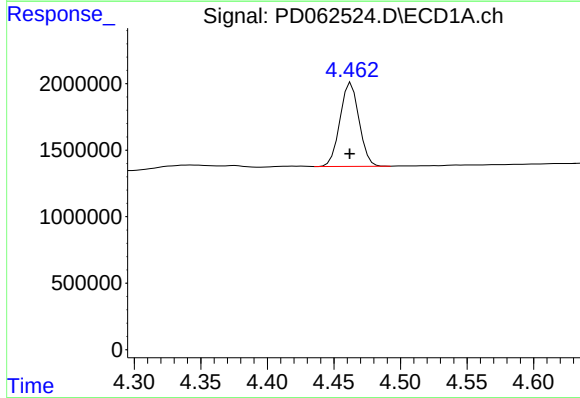


#4 Heptachlor

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 6256383
Conc: 4.86 ng/ml

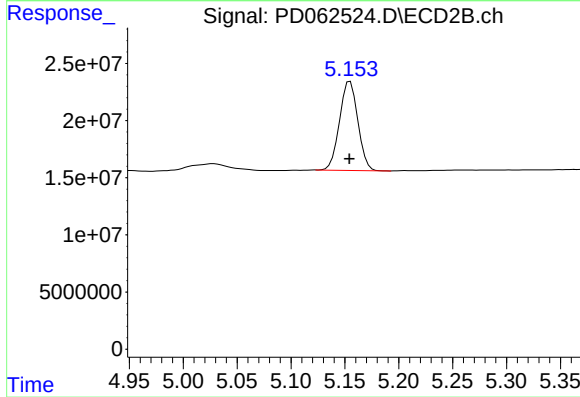

#4 Heptachlor


R.T.: 5.155 min
Delta R.T.: 0.000 min
Response: 92147790
Conc: 5.20 ng/ml

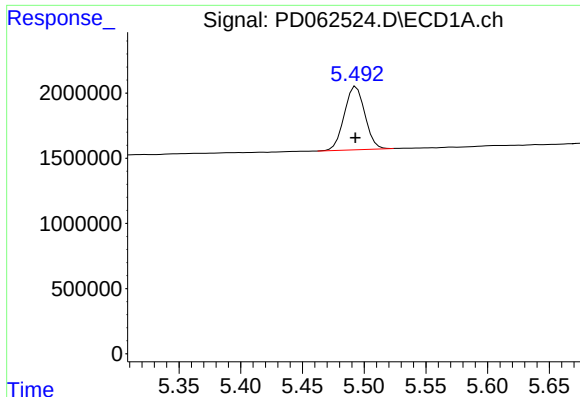

#9 Endosulfan I


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 5629582
Conc: 5.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

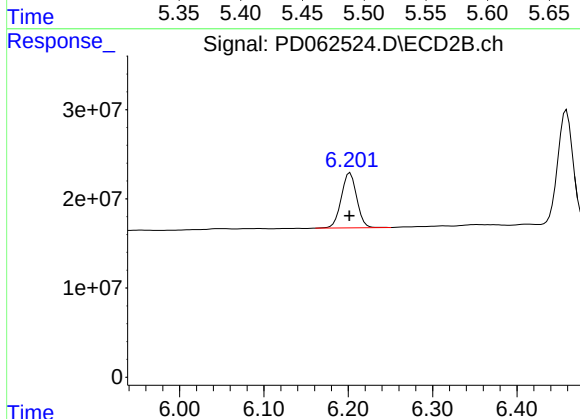


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 78556133
Conc: 5.29 ng/ml

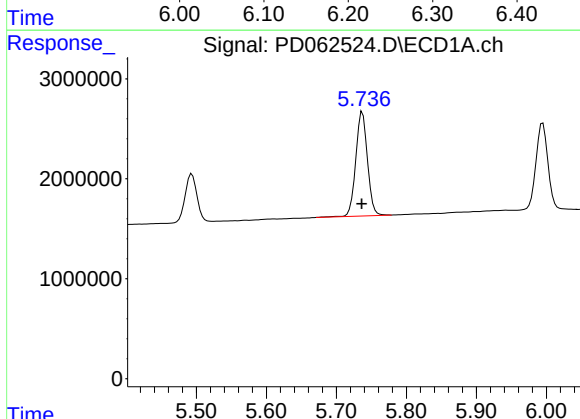


#13 Dieldrin

R.T.: 5.737 min
Delta R.T.: 0.000 min
Response: 12124662
Conc: 9.57 ng/ml

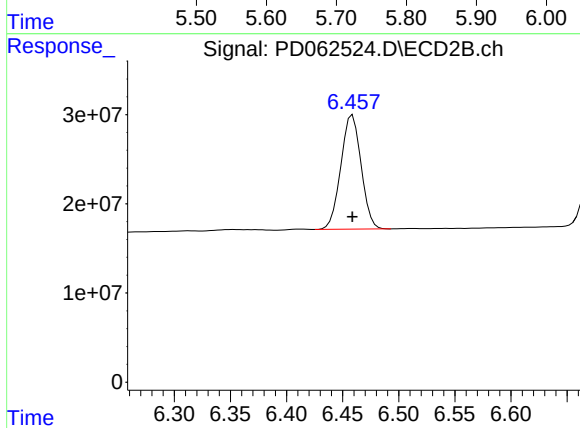

#13 Dieldrin


R.T.: 6.459 min
Delta R.T.: 0.000 min
Response: 161285361
Conc: 10.19 ng/ml

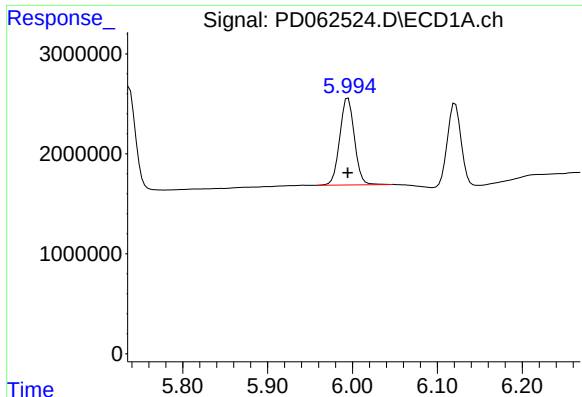

#14 Endrin


R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 10420959
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

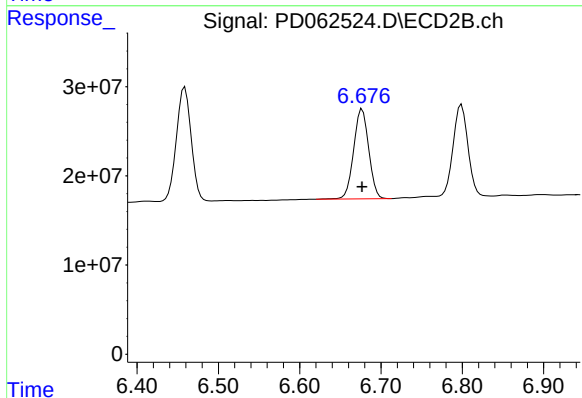


#14 Endrin

R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 129642852
Conc: 10.22 ng/ml

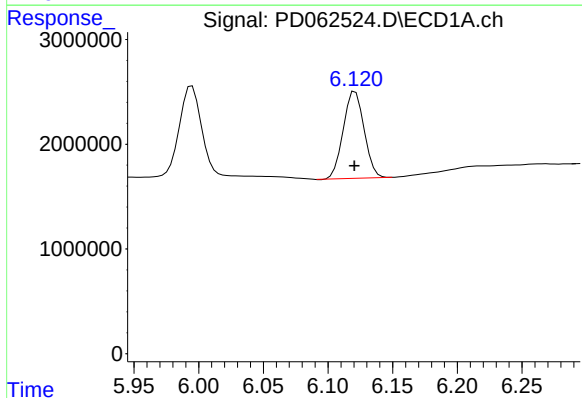


#16 4,4'-DDD

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 9295599
Conc: 9.20 ng/ml

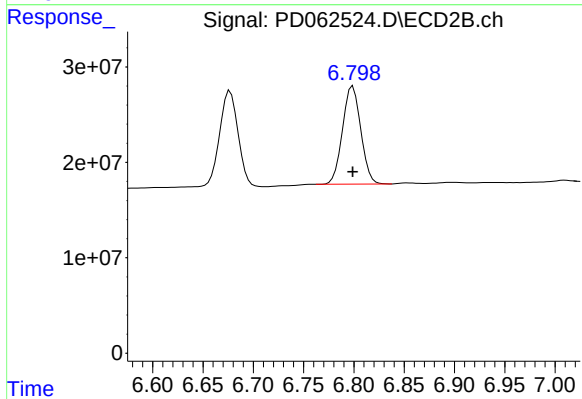

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 129555215
Conc: 10.27 ng/ml

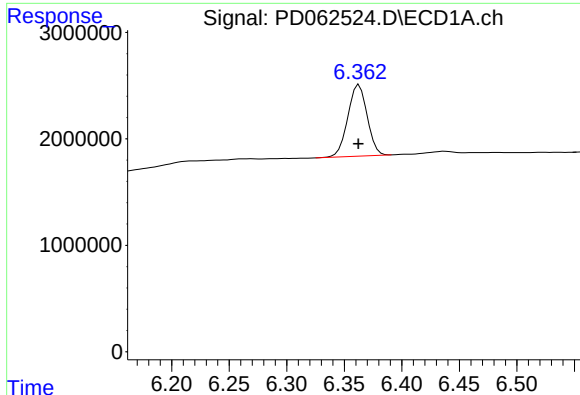

#17 4,4'-DDT


R.T.: 6.363 min
Delta R.T.: 0.000 min
Response: 7895809
Conc: 8.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

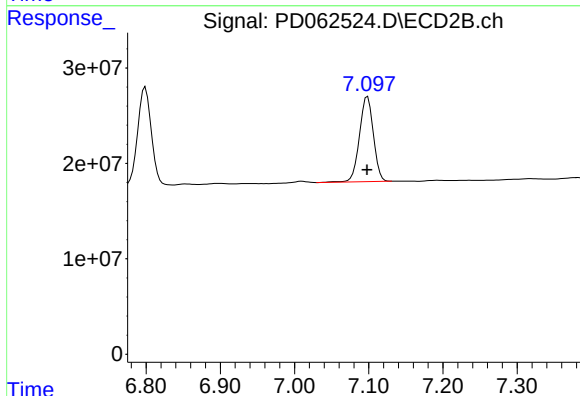


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: 0.000 min
Response: 116603803
Conc: 9.56 ng/ml

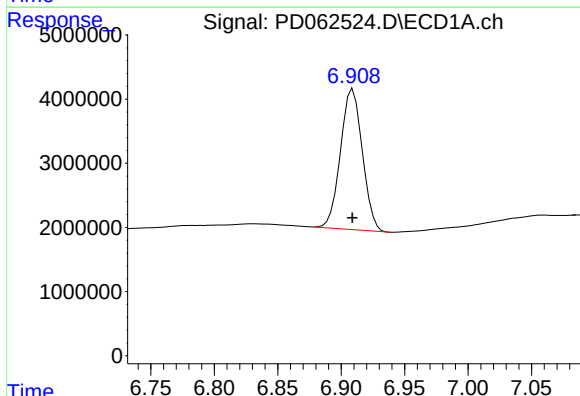


#20 Methoxychlor

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 26127700
Conc: 47.40 ng/ml

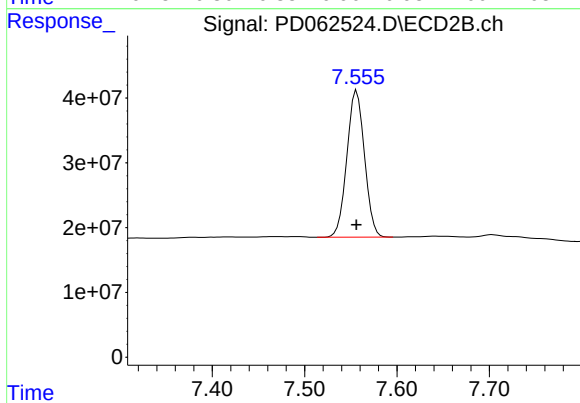

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 300096934
Conc: 51.35 ng/ml

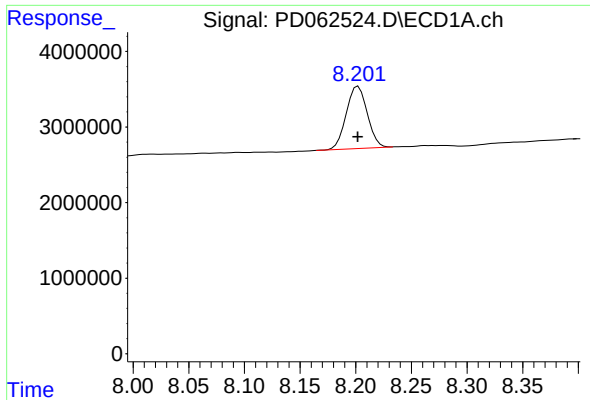

#27 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 10805827
Conc: 9.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

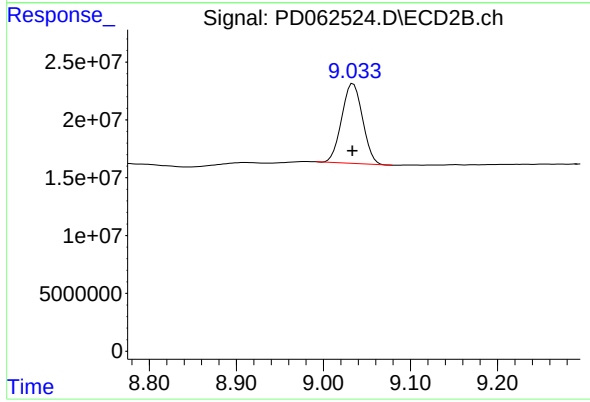

#27 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: 0.001 min
Response: 114252690
Conc: 10.26 ng/ml