

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 11:08
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 12:31:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 29 12:30:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.973	9843287	128.8E6	10.272	10.472
27)	SA Decachlor...	8.202	9.033	22266606	234.8E6	20.320	21.097
Target Compounds							
2)	A alpha-BHC	3.878	4.361	13505676	196.9E6	9.655	10.292
3)	MA gamma-BHC...	4.161	4.646	13179229	180.7E6	9.936	10.329
4)	MA Heptachlor	4.463	5.154	12750508	183.1E6	9.909	10.341
9)	A Endosulfan I	5.493	6.201	11266343	154.4E6	10.066	10.401
13)	MA Dieldrin	5.737	6.458	24773026	324.3E6	19.553	20.494
14)	MA Endrin	5.994	6.676	20841471	260.1E6	19.621	20.493
16)	A 4,4'-DDD	6.120	6.799	19501371	259.3E6	19.293	20.549
17)	MA 4,4'-DDT	6.362	7.097	17437856	241.9E6	18.233	19.835
20)	A Methoxychlor	6.909	7.556	54211695	605.8E6	98.342	103.661


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 11:08
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 12:31:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 29 12:30:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

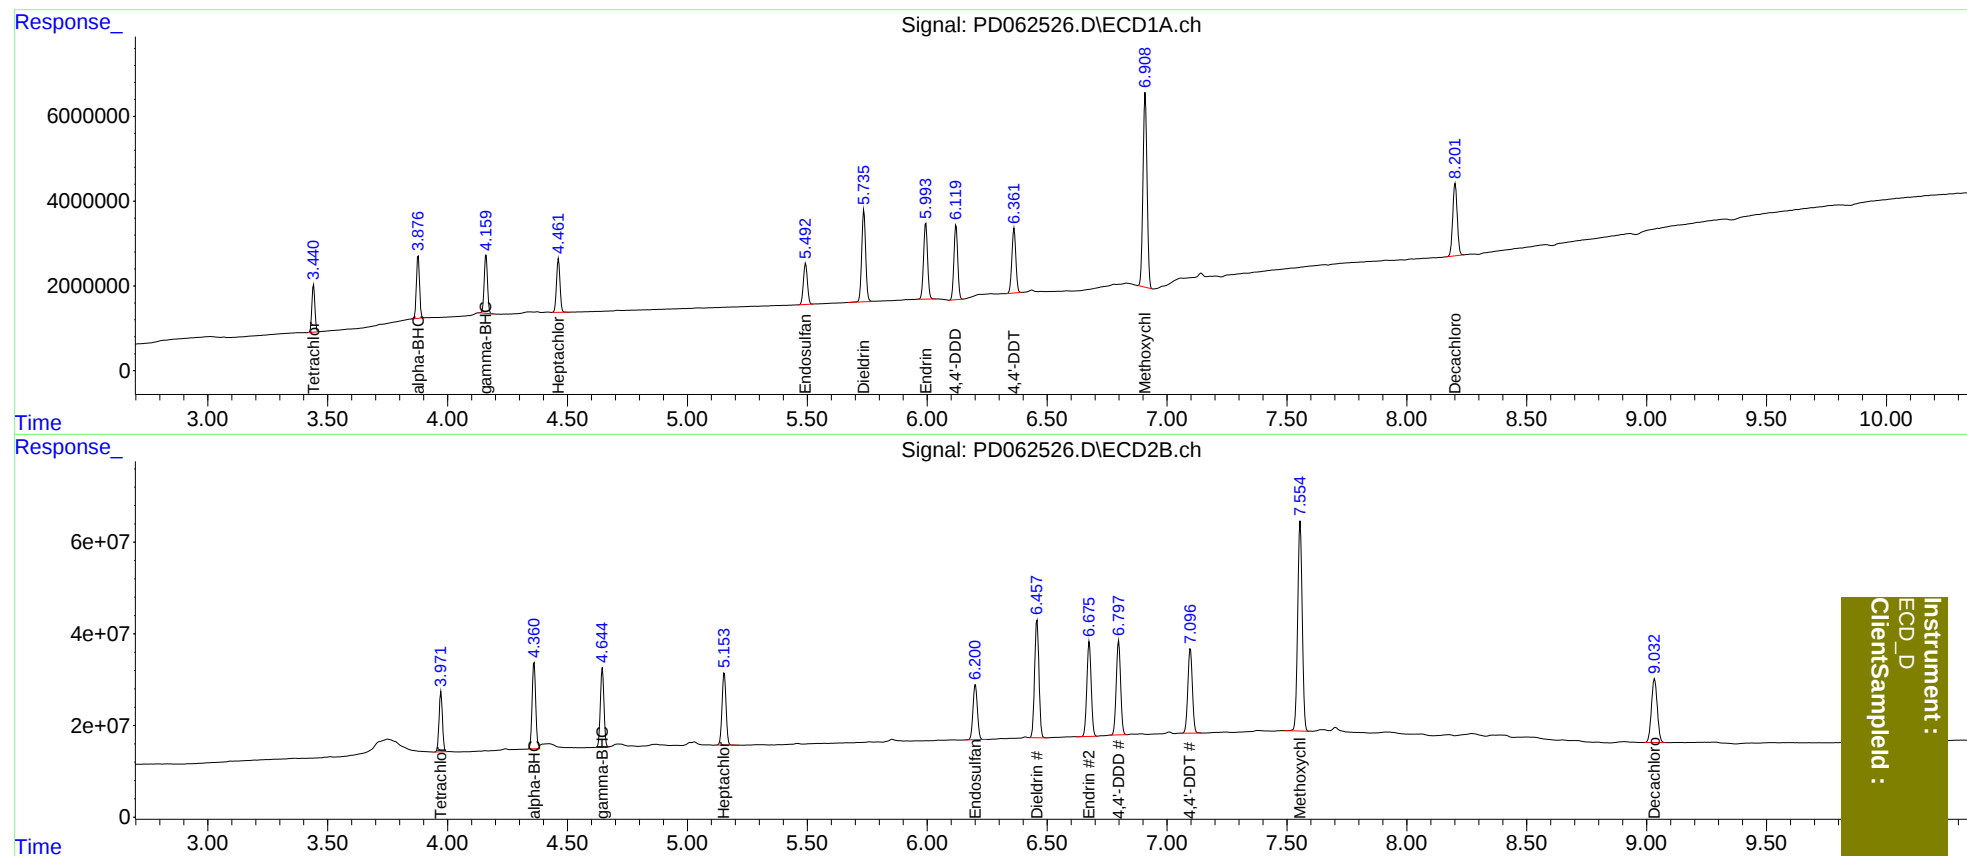


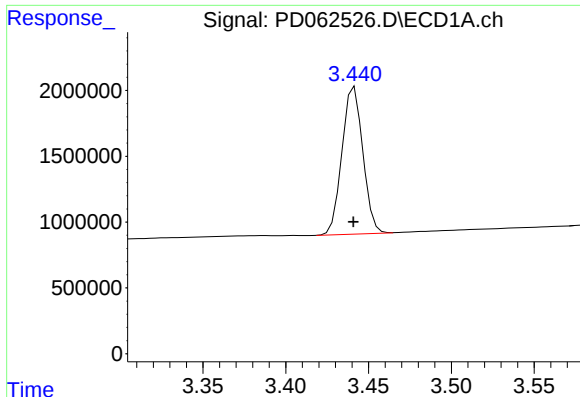

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 9843287
Conc: 10.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

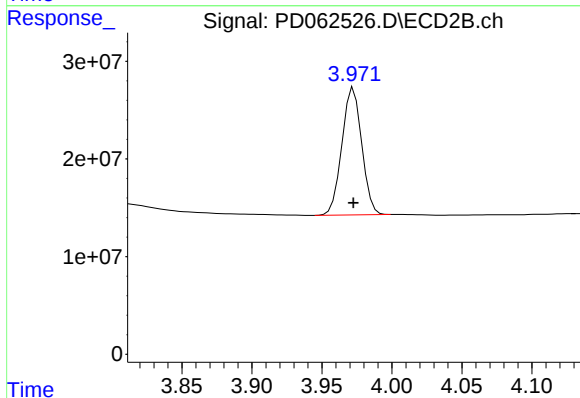


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 128776899
Conc: 10.47 ng/ml

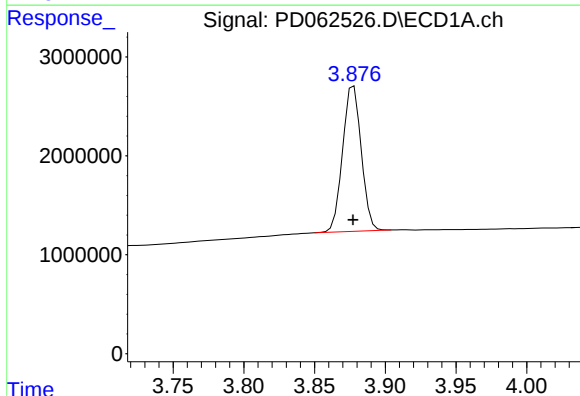


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 13505676
Conc: 9.65 ng/ml

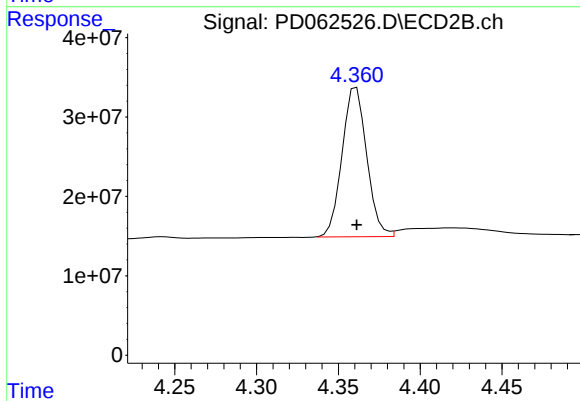

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 196912734
Conc: 10.29 ng/ml

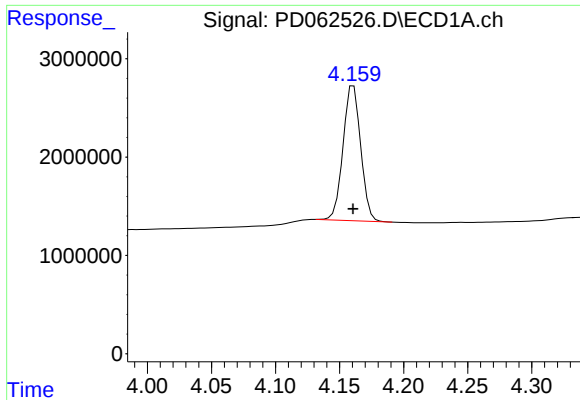

#3 gamma-BHC (Lindane)


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 13179229
Conc: 9.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

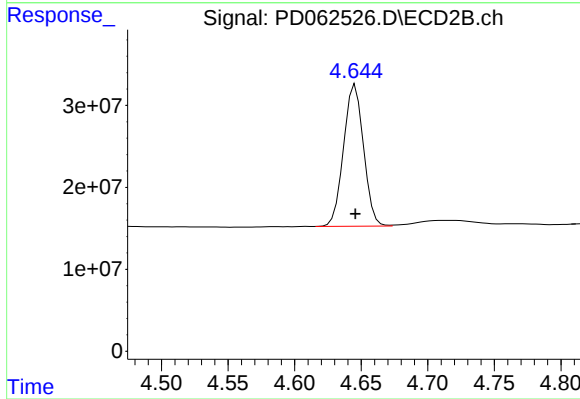


#3 gamma-BHC (Lindane)

R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 180672789
Conc: 10.33 ng/ml

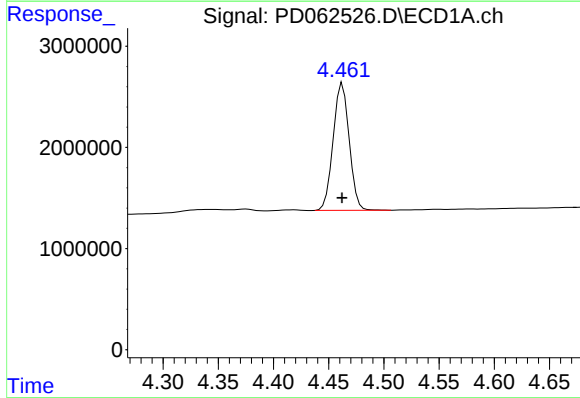


#4 Heptachlor

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 12750508
Conc: 9.91 ng/ml

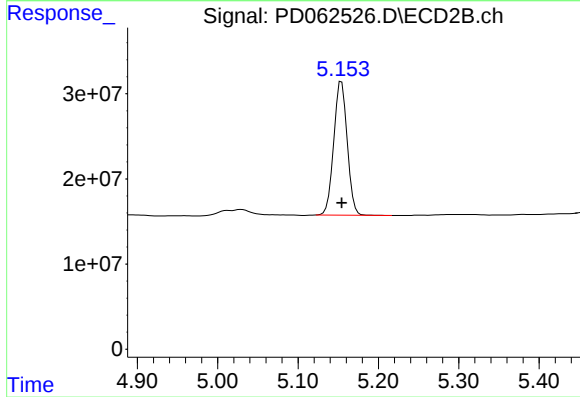

#4 Heptachlor


R.T.: 5.154 min
Delta R.T.: 0.000 min
Response: 183083885
Conc: 10.34 ng/ml

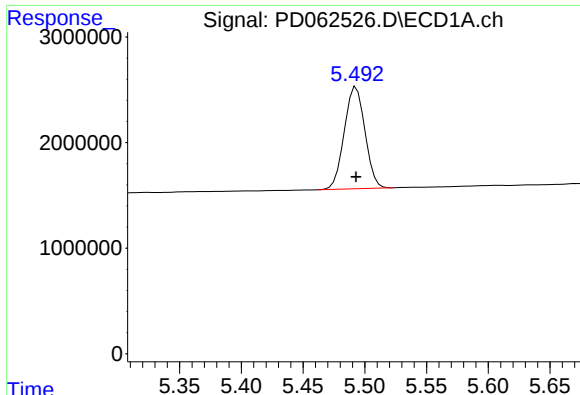

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 11266343
Conc: 10.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

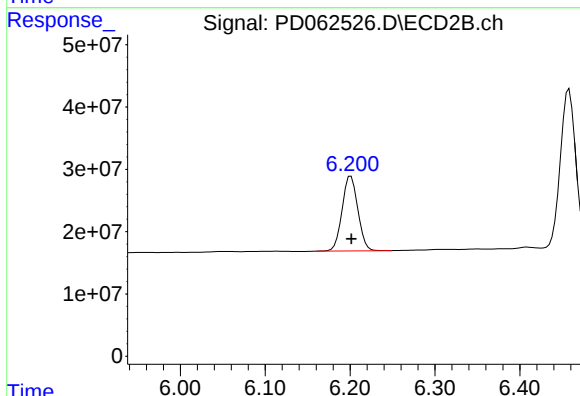


#9 Endosulfan I

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 154444499
Conc: 10.40 ng/ml

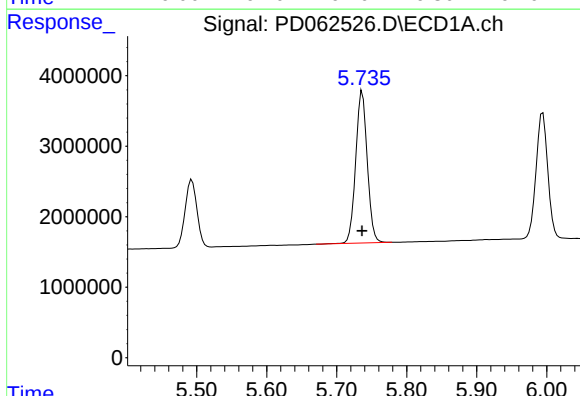


#13 Dieldrin

R.T.: 5.737 min
Delta R.T.: 0.000 min
Response: 24773026
Conc: 19.55 ng/ml

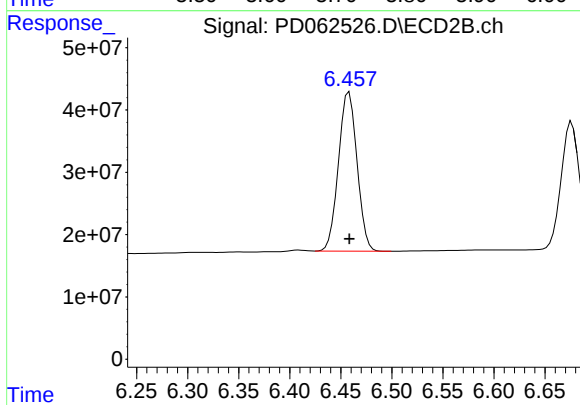

#13 Dieldrin


R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 324343045
Conc: 20.49 ng/ml

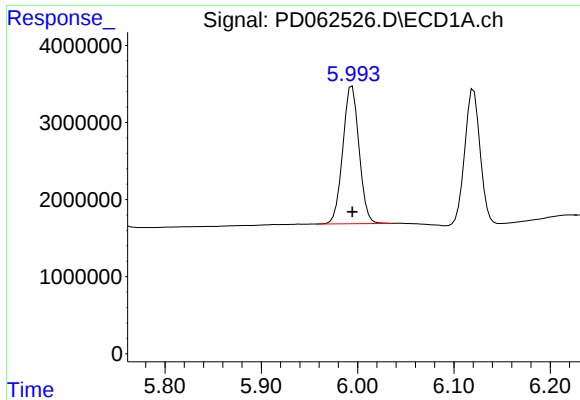

#14 Endrin


R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 20841471
Conc: 19.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

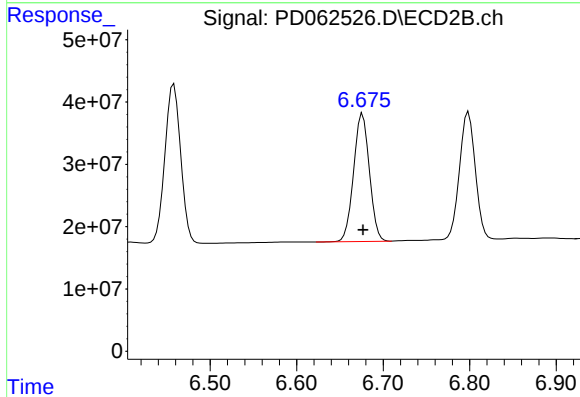


#14 Endrin

R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 260073164
Conc: 20.49 ng/ml

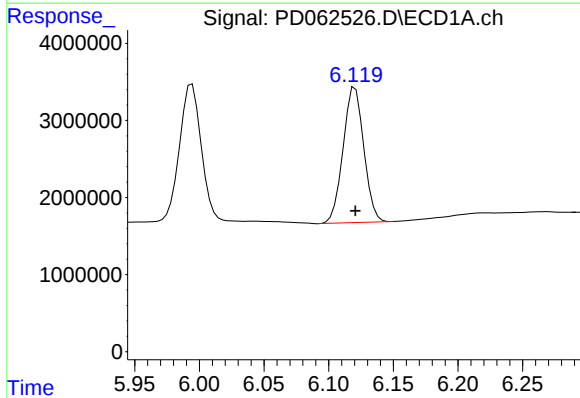


#16 4,4'-DDD

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 19501371
Conc: 19.29 ng/ml

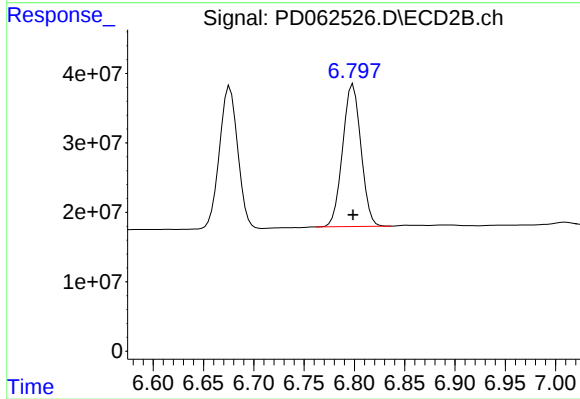

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 259309988
Conc: 20.55 ng/ml

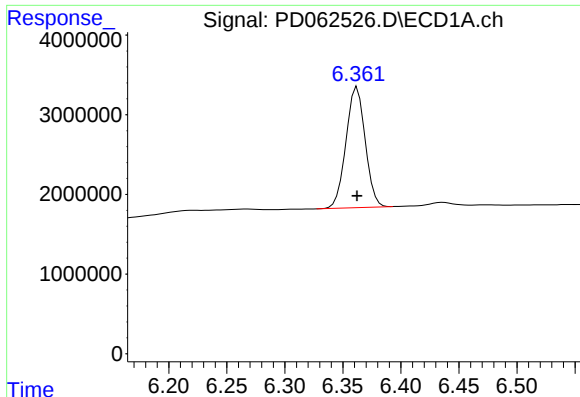

#17 4,4'-DDT


R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 17437856
Conc: 18.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

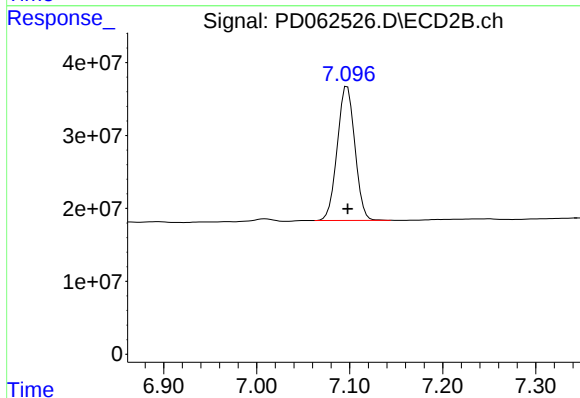


#17 4,4'-DDT

R.T.: 7.097 min
Delta R.T.: 0.000 min
Response: 241934852
Conc: 19.83 ng/ml

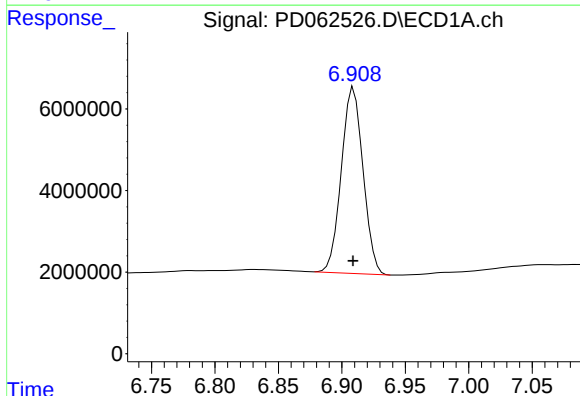


#20 Methoxychlor

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 54211695
Conc: 98.34 ng/ml

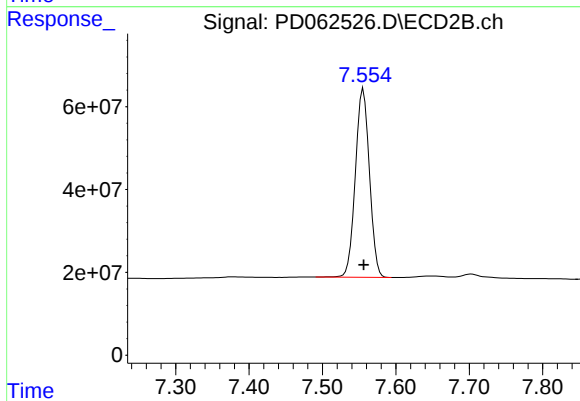

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 605792248
Conc: 103.66 ng/ml

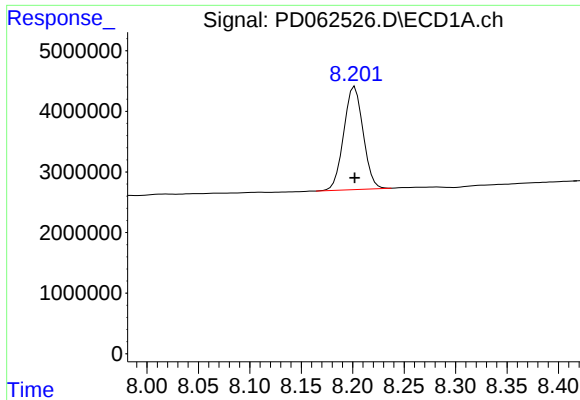

#27 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 22266606
Conc: 20.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

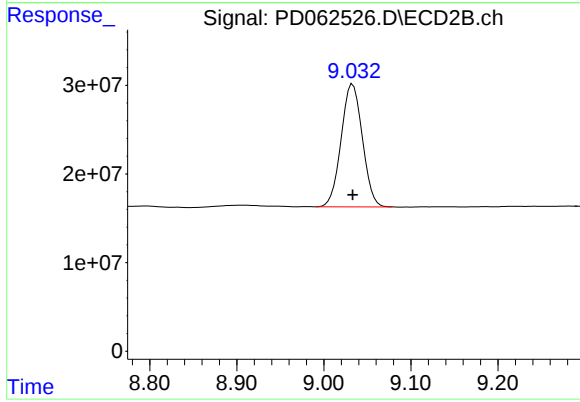

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 234822366
Conc: 21.10 ng/ml