

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 11:36
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 12:31:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 29 12:30:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.972	19165924	245.9E6	20.000	20.000
27)	SA Decachlor...	8.202	9.033	43831222	445.2E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.877	4.361	27976581	382.7E6	20.000	20.000
3)	MA gamma-BHC...	4.161	4.646	26528357	349.8E6	20.000	20.000
4)	MA Heptachlor	4.462	5.154	25735066	354.1E6	20.000	20.000
9)	A Endosulfan I	5.493	6.202	22384671	297.0E6	20.000	20.000
13)	MA Dieldrin	5.736	6.459	50678058	633.0E6	40.000	40.000
14)	MA Endrin	5.994	6.677	42487171	507.6E6	40.000	40.000
16)	A 4,4'-DDD	6.121	6.799	40432501	504.8E6	40.000	40.000
17)	MA 4,4'-DDT	6.362	7.098	38255386	487.9E6	40.000	40.000
20)	A Methoxychlor	6.909	7.556	110.3E6	1168.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 11:36
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 12:31:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 29 12:30:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

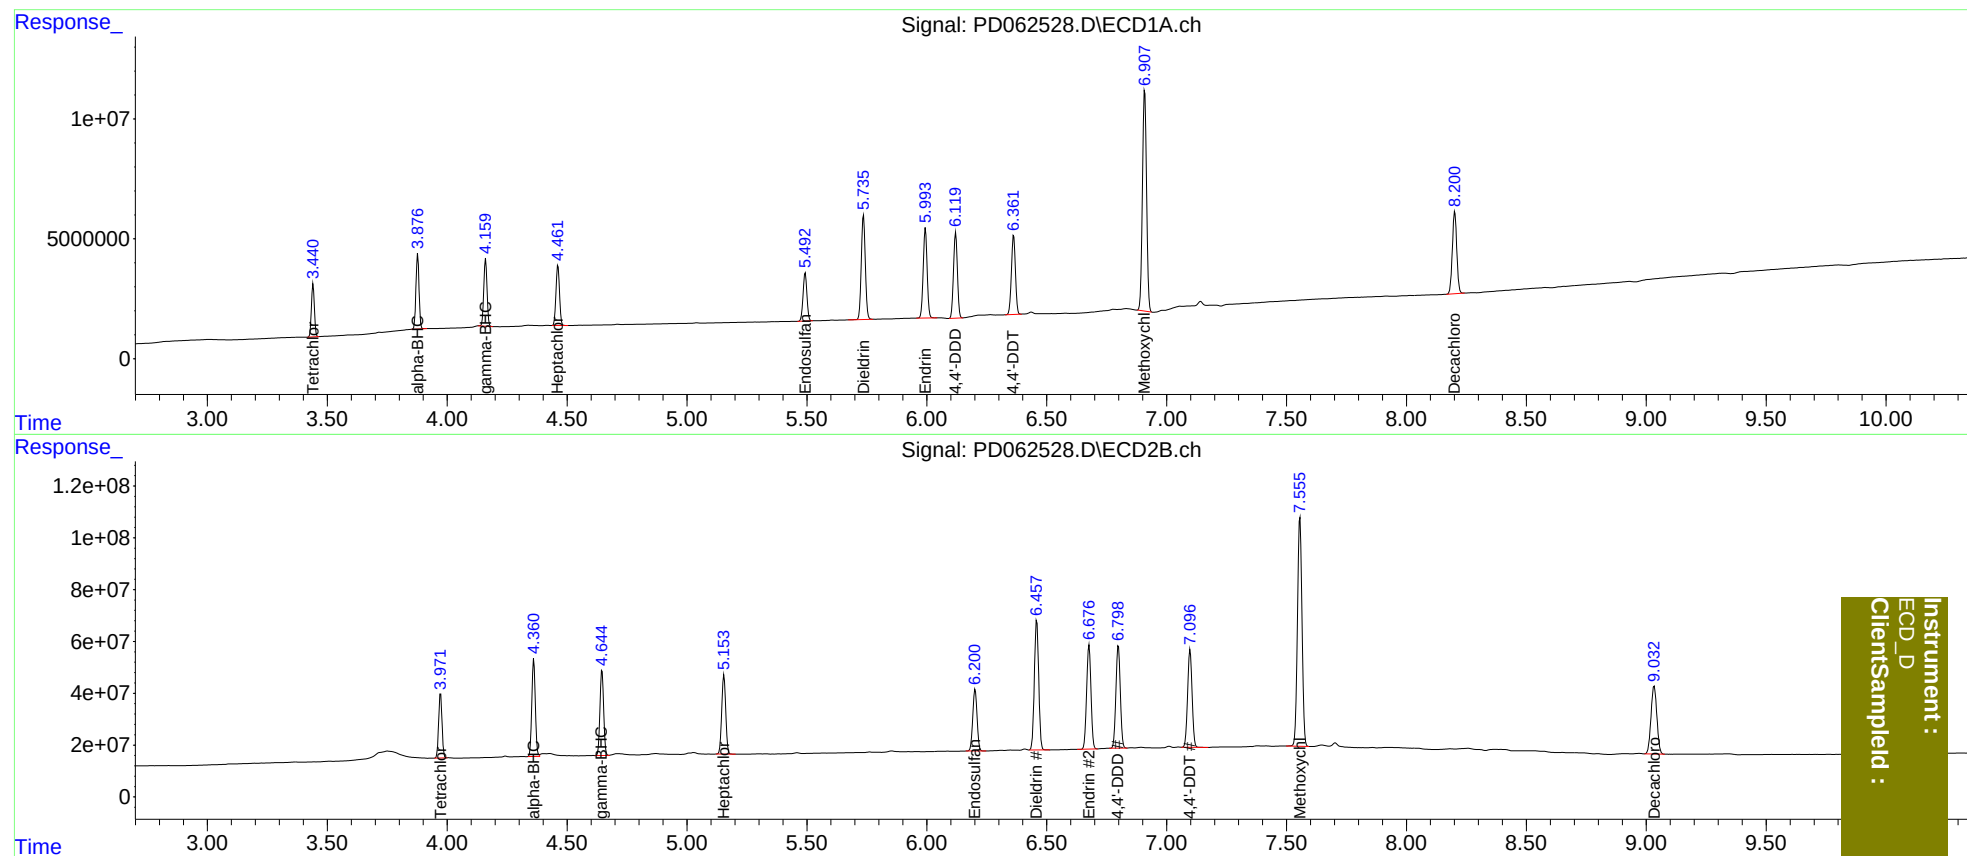


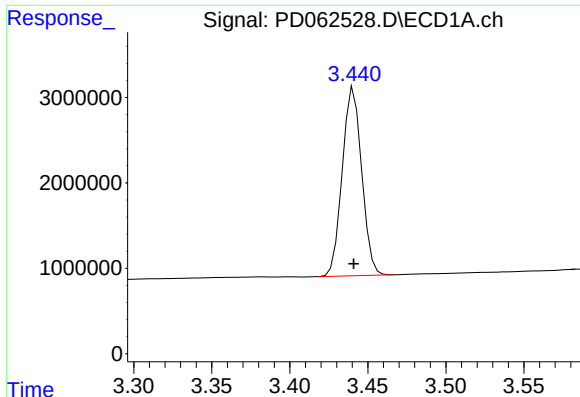

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 19165924
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

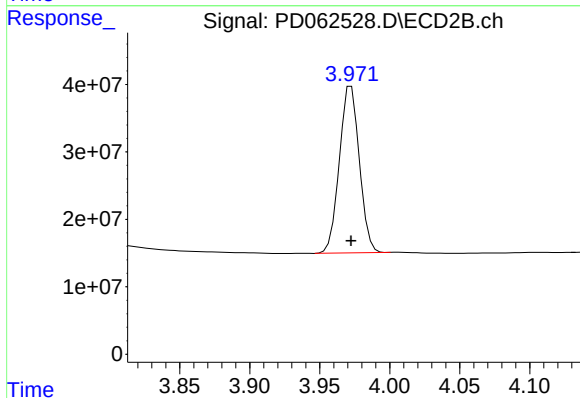


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 245938166
Conc: 20.00 ng/ml

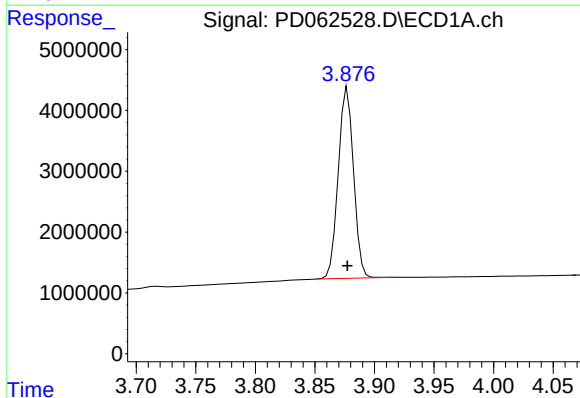


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 27976581
Conc: 20.00 ng/ml

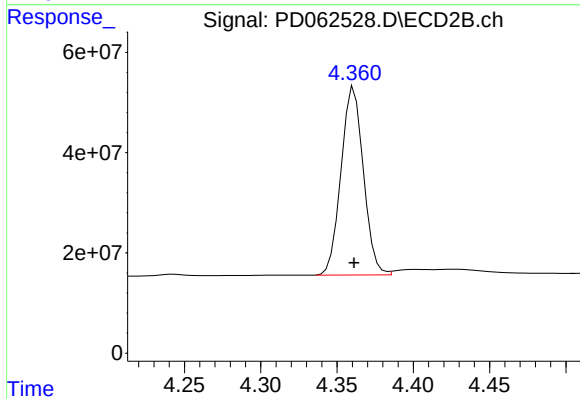

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 382650307
Conc: 20.00 ng/ml

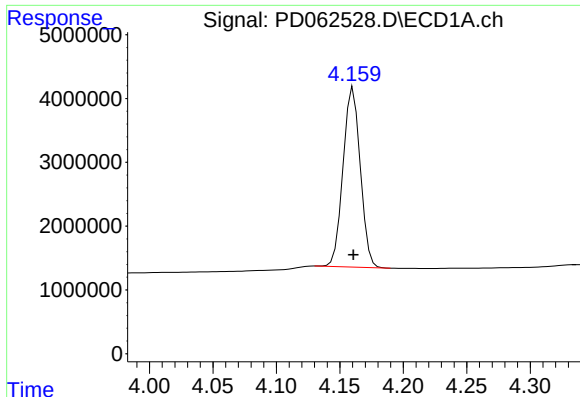

#3 gamma-BHC (Lindane)


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 26528357
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

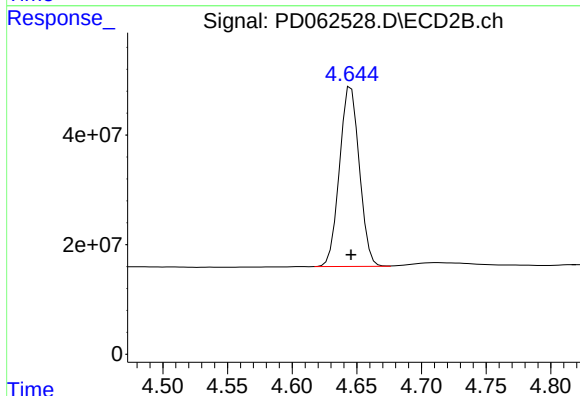


#3 gamma-BHC (Lindane)

R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 349840575
Conc: 20.00 ng/ml

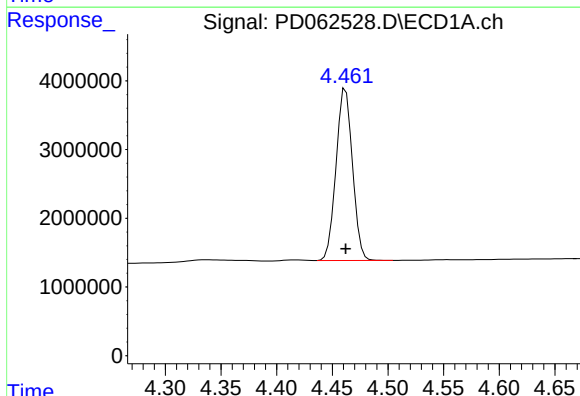


#4 Heptachlor

R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 25735066
Conc: 20.00 ng/ml

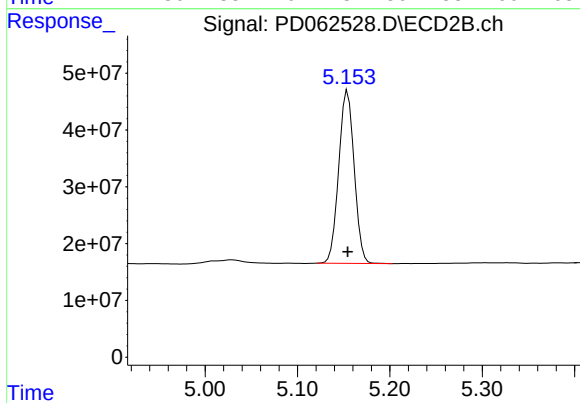

#4 Heptachlor


R.T.: 5.154 min
Delta R.T.: 0.000 min
Response: 354083984
Conc: 20.00 ng/ml

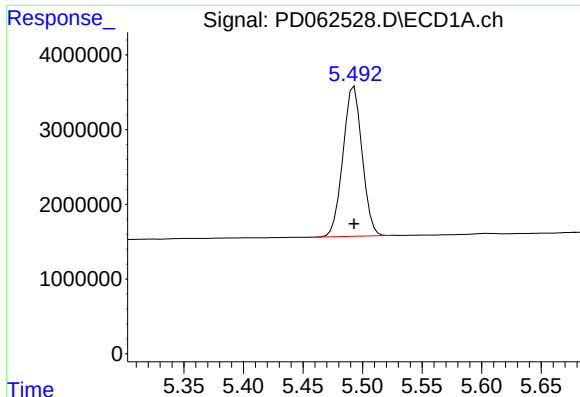

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 22384671
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

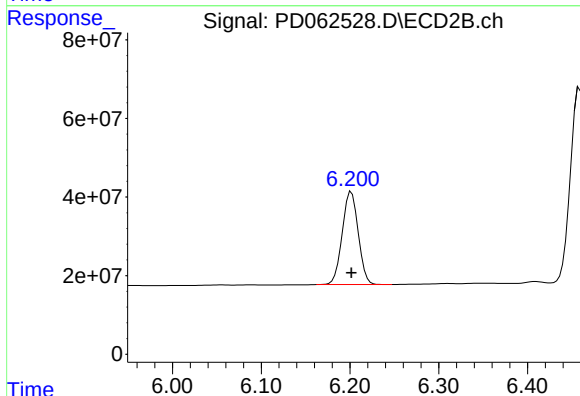


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 296991034
Conc: 20.00 ng/ml

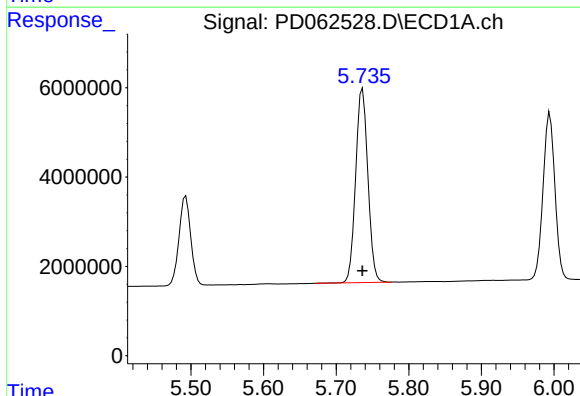


#13 Dieldrin

R.T.: 5.736 min
Delta R.T.: 0.000 min
Response: 50678058
Conc: 40.00 ng/ml

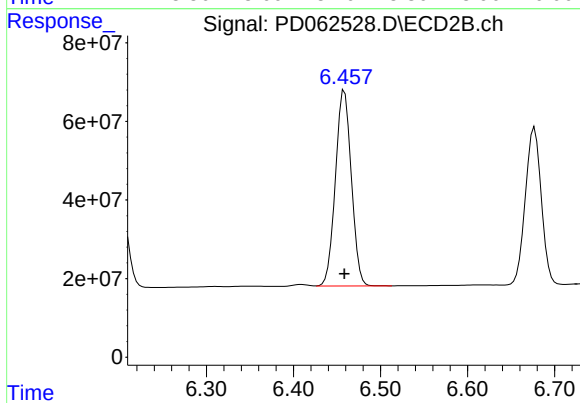

#13 Dieldrin


R.T.: 6.459 min
Delta R.T.: 0.000 min
Response: 633049106
Conc: 40.00 ng/ml

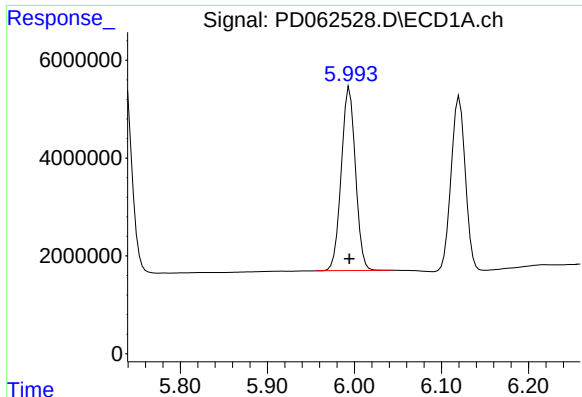

#14 Endrin


R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 42487171
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

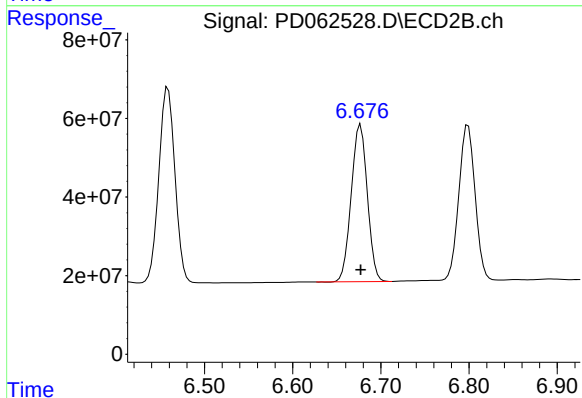


#14 Endrin

R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 507642734
Conc: 40.00 ng/ml

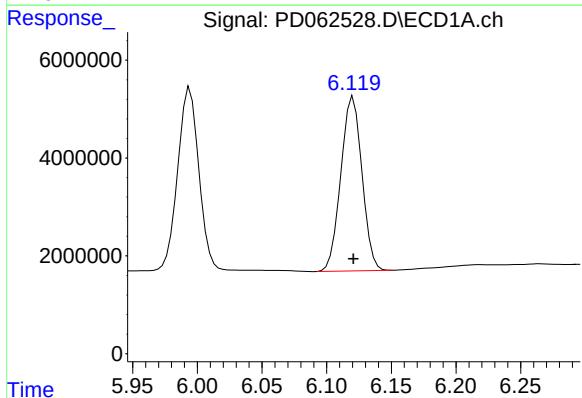


#16 4,4'-DDD

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 40432501
Conc: 40.00 ng/ml

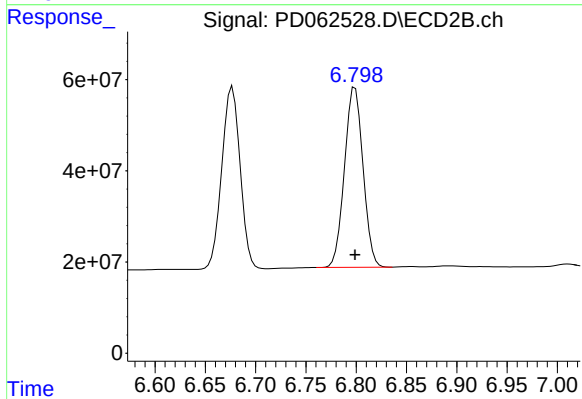

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 504766508
Conc: 40.00 ng/ml

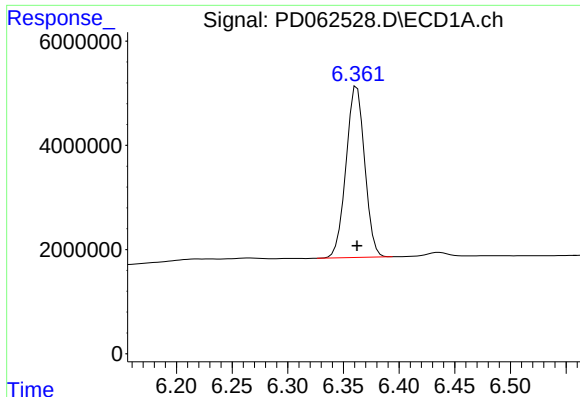

#17 4,4'-DDT


R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 38255386
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

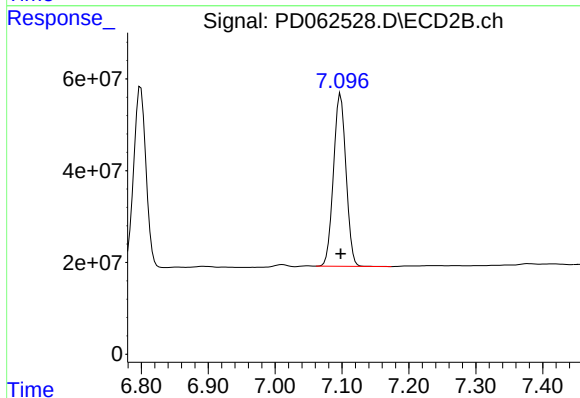


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: 0.000 min
Response: 487905844
Conc: 40.00 ng/ml

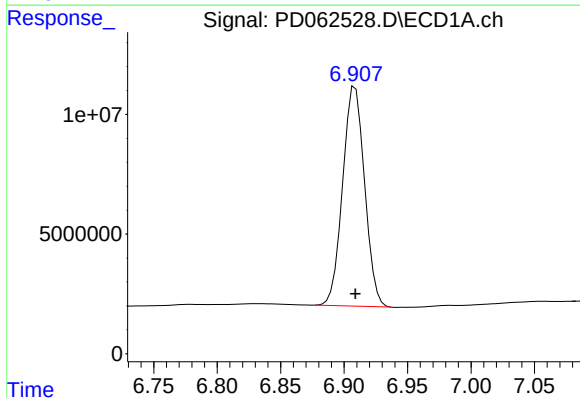


#20 Methoxychlor

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 110250923
Conc: 200.00 ng/ml

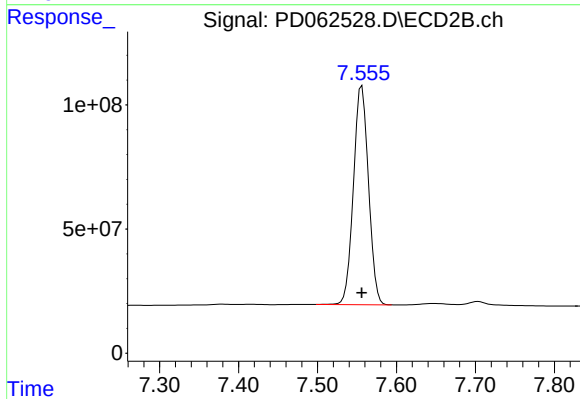

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 1168792559
Conc: 200.00 ng/ml

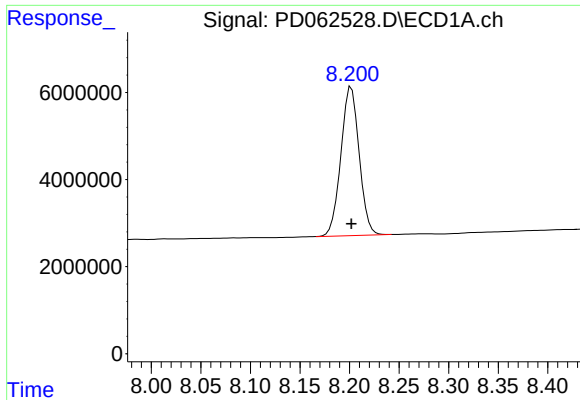

#27 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 43831222
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

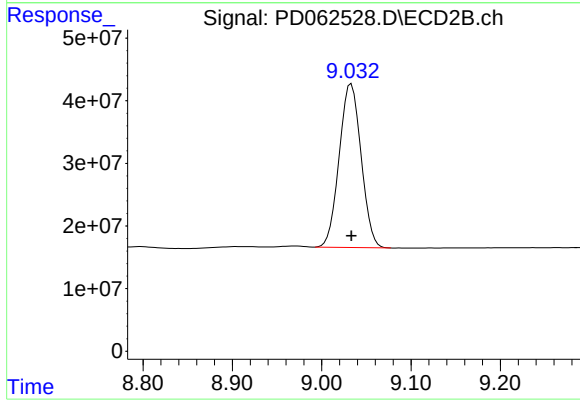

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 445221621
Conc: 40.00 ng/ml