

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 12:04
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 12:31:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 29 12:30:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.973	37626801	463.9E6	39.264	37.726
27)	SA Decachlor...	8.202	9.033	84709412	836.0E6	77.305	75.104
Target Compounds							
2)	A alpha-BHC	3.878	4.361	57640459	728.4E6	41.206	38.069
3)	MA gamma-BHC...	4.161	4.646	53786282	667.2E6	40.550	38.144
4)	MA Heptachlor	4.463	5.154	51956405	663.7E6	40.378	37.486
9)	A Endosulfan I	5.493	6.202	44474155	561.5E6	39.736	37.811
13)	MA Dieldrin	5.736	6.459	103.1E6	1205.3E6	81.369	76.158
14)	MA Endrin	5.994	6.677	85229154	967.4E6	80.240	76.228
16)	A 4,4'-DDD	6.121	6.799	82221414	965.7E6	81.342	76.527
17)	MA 4,4'-DDT	6.362	7.098	80860667	948.7E6	84.548	77.774
20)	A Methoxychlor	6.909	7.556	215.0E6	2171.9E6	389.954	371.642


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 12:04
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 12:31:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 29 12:30:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

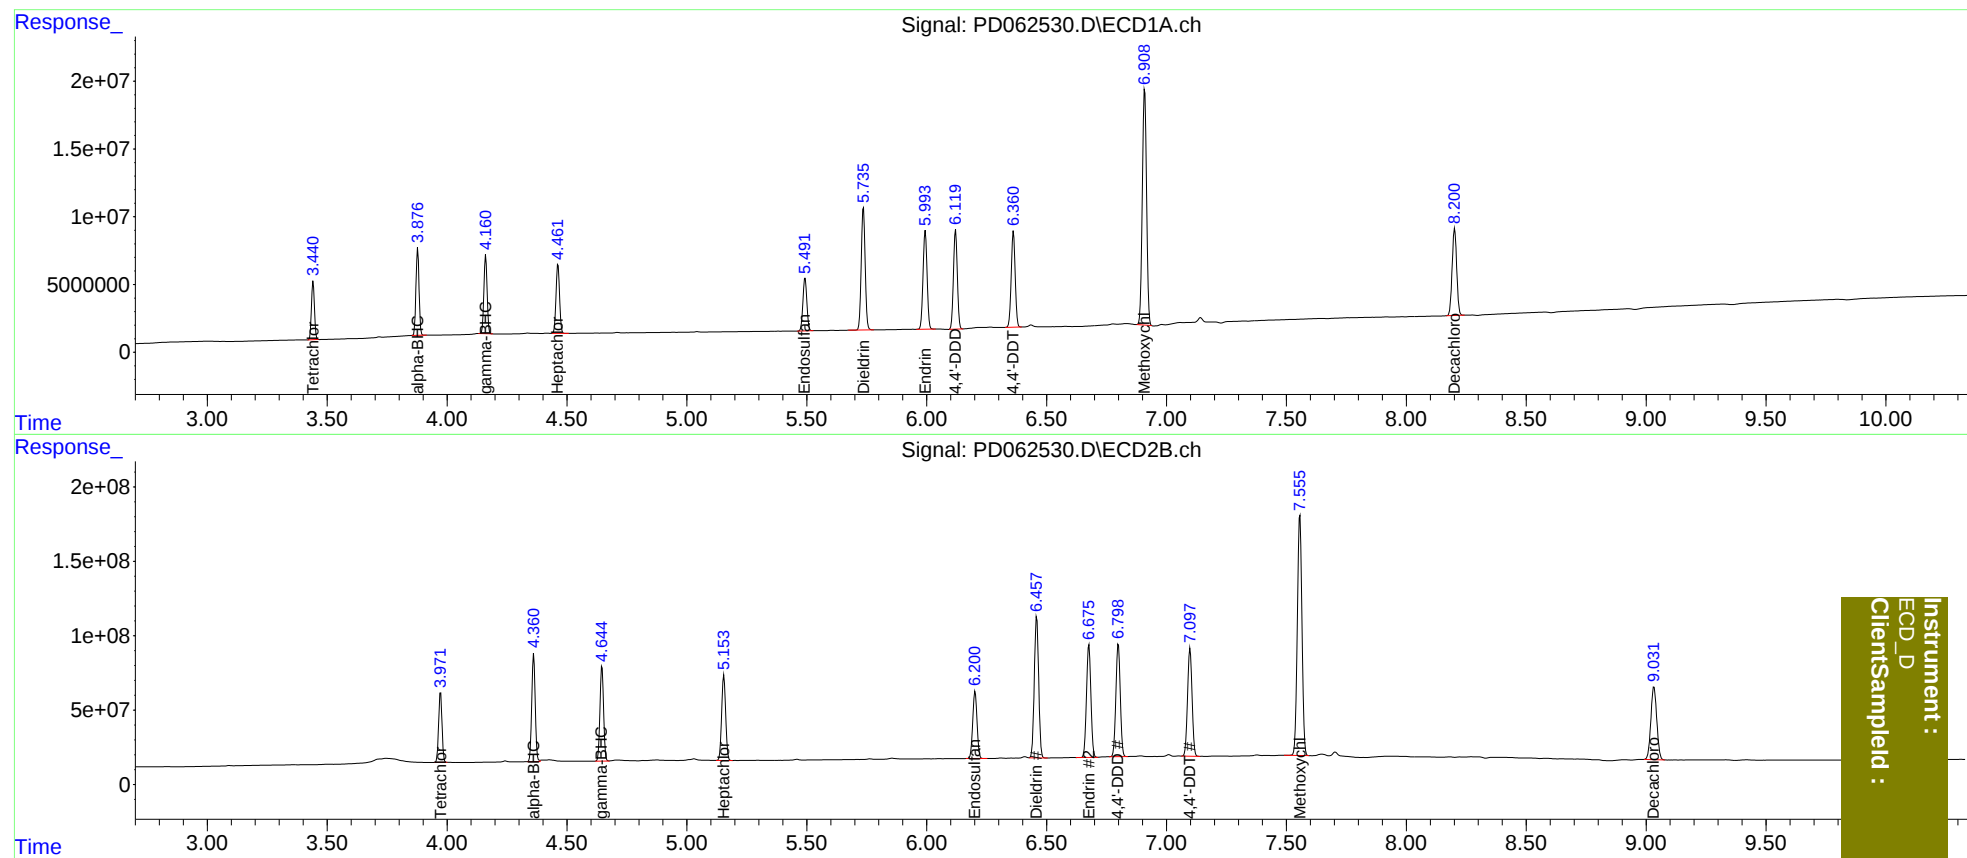


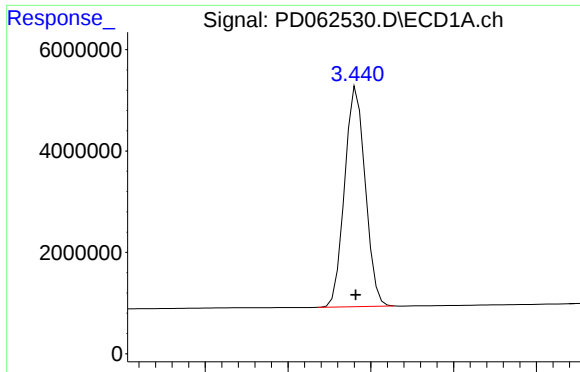

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 37626801
Conc: 39.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

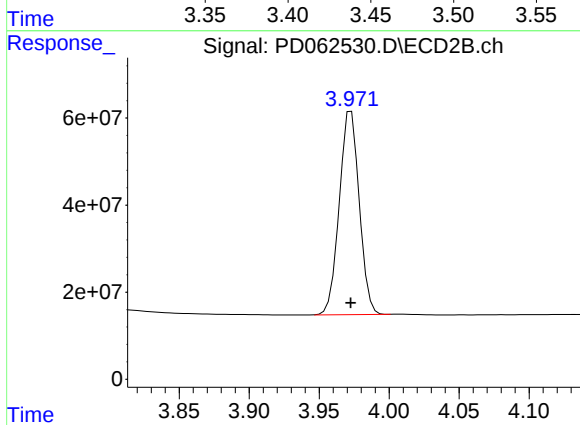


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 463918742
Conc: 37.73 ng/ml

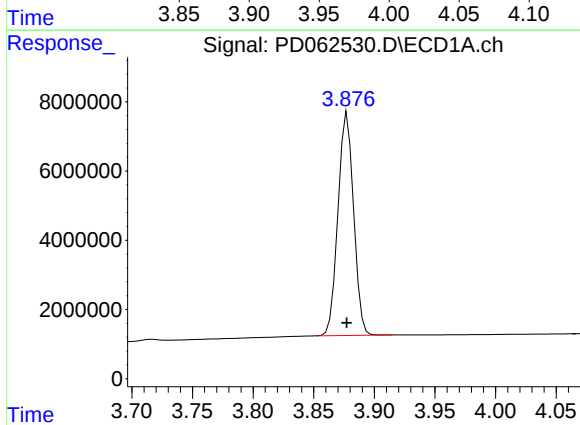


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 57640459
Conc: 41.21 ng/ml

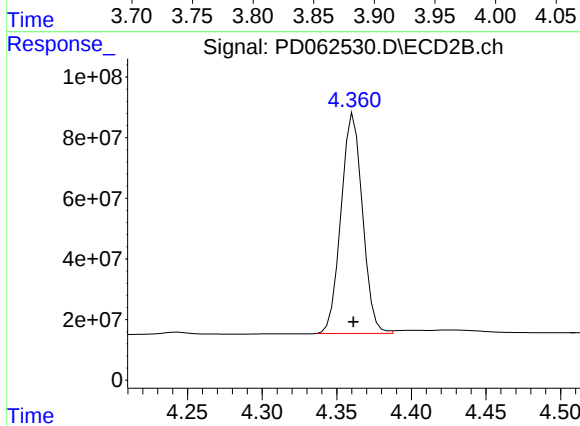

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 728364470
Conc: 38.07 ng/ml

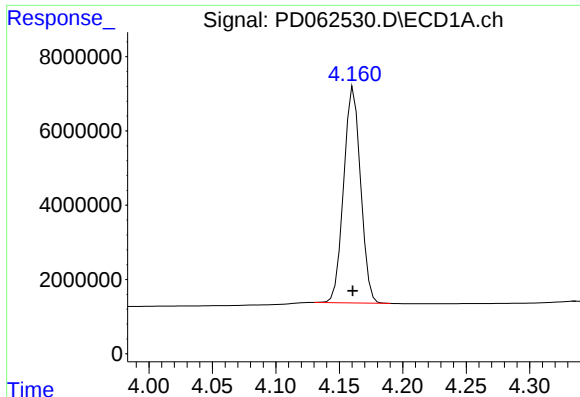

#3 gamma-BHC (Lindane)


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 53786282
Conc: 40.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

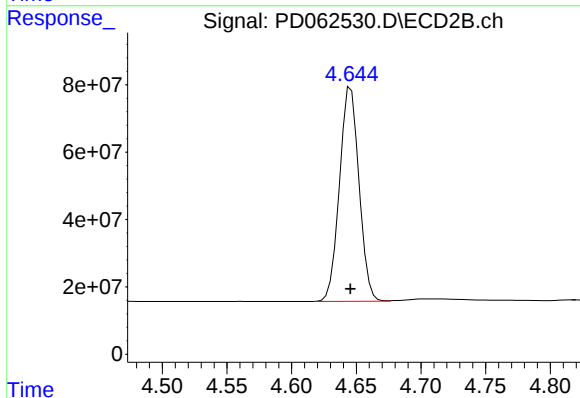


#3 gamma-BHC (Lindane)

R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 667208790
Conc: 38.14 ng/ml

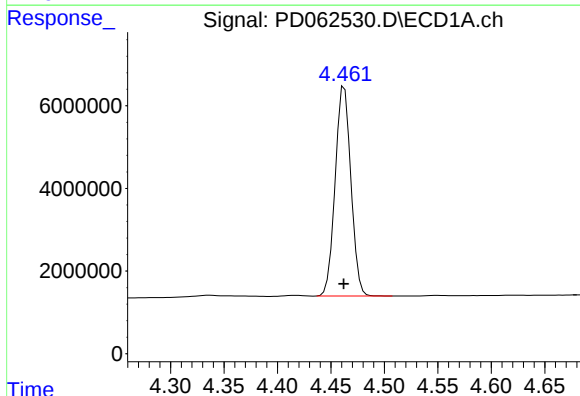


#4 Heptachlor

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 51956405
Conc: 40.38 ng/ml

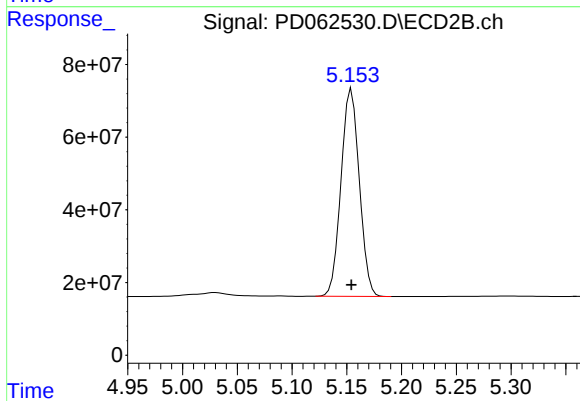

#4 Heptachlor


R.T.: 5.154 min
Delta R.T.: 0.000 min
Response: 663663518
Conc: 37.49 ng/ml

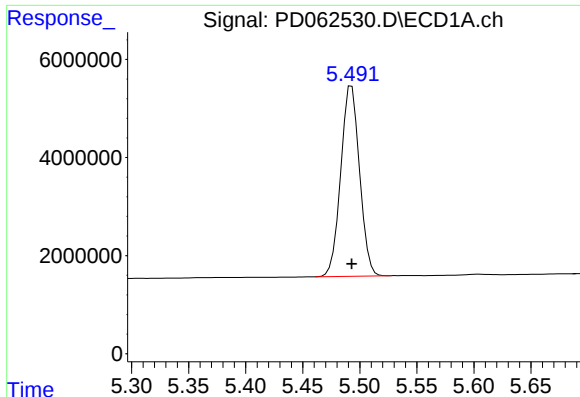

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 44474155
Conc: 39.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

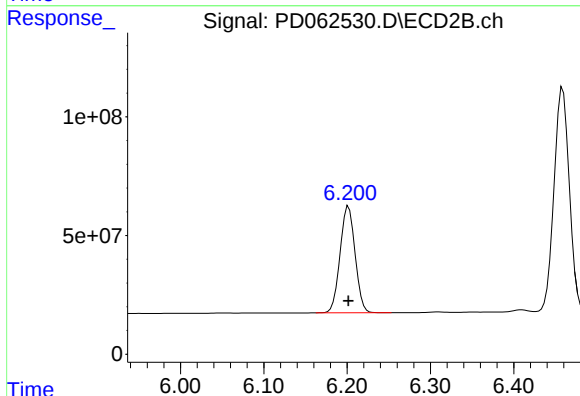


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 561479843
Conc: 37.81 ng/ml

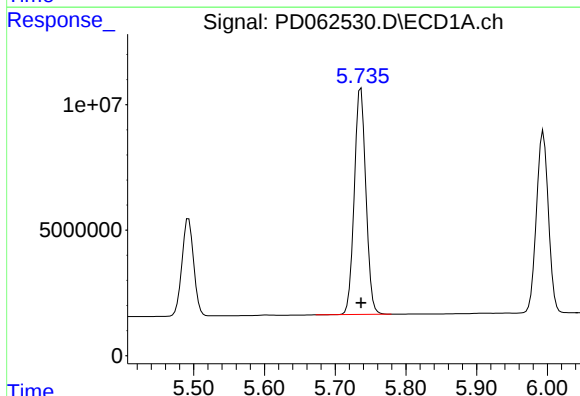


#13 Dieldrin

R.T.: 5.736 min
Delta R.T.: 0.000 min
Response: 103090365
Conc: 81.37 ng/ml

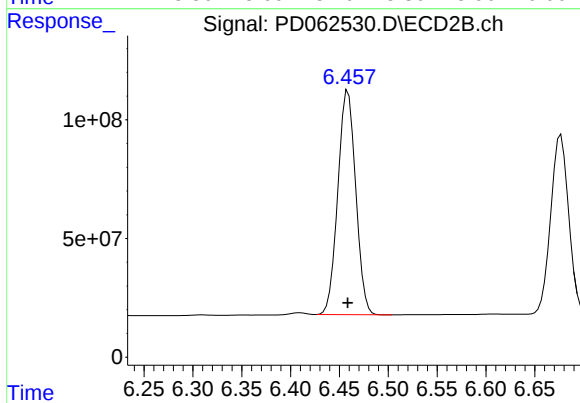

#13 Dieldrin


R.T.: 6.459 min
Delta R.T.: 0.000 min
Response: 1205295128
Conc: 76.16 ng/ml

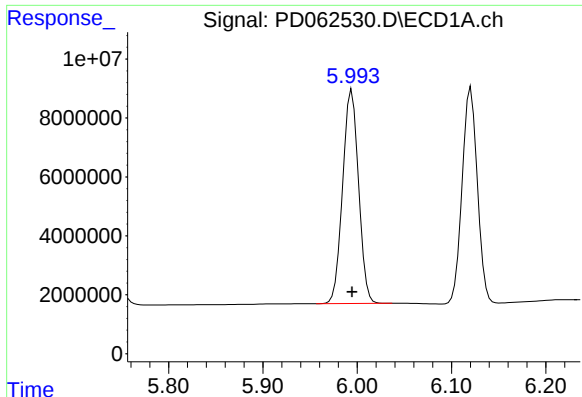

#14 Endrin


R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 85229154
Conc: 80.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

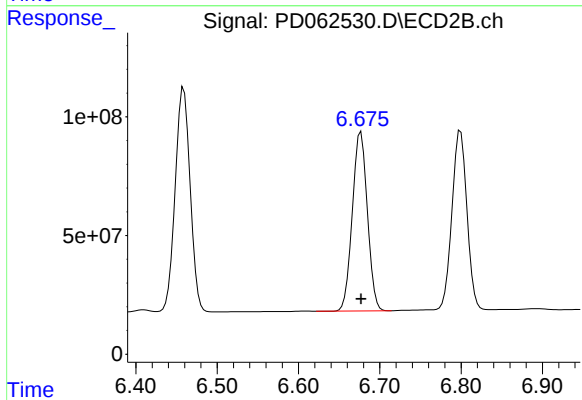


#14 Endrin

R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 967408939
Conc: 76.23 ng/ml

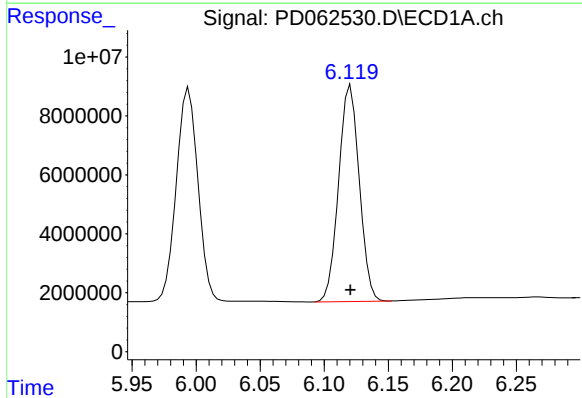


#16 4,4'-DDD

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 82221414
Conc: 81.34 ng/ml

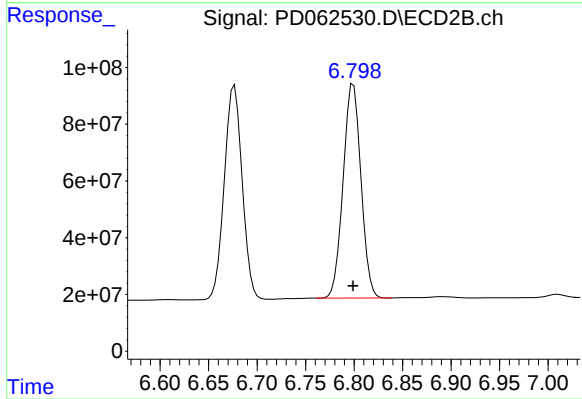

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 965708822
Conc: 76.53 ng/ml

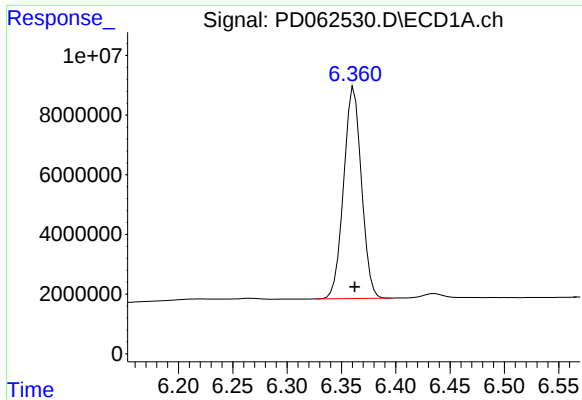

#17 4,4'-DDT


R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 80860667
Conc: 84.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

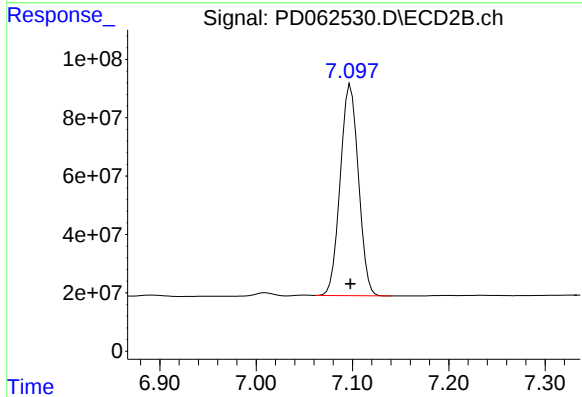


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: 0.000 min
Response: 948656946
Conc: 77.77 ng/ml

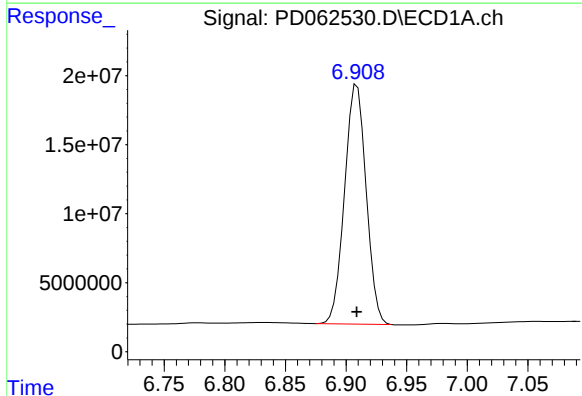


#20 Methoxychlor

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 214963764
Conc: 389.95 ng/ml

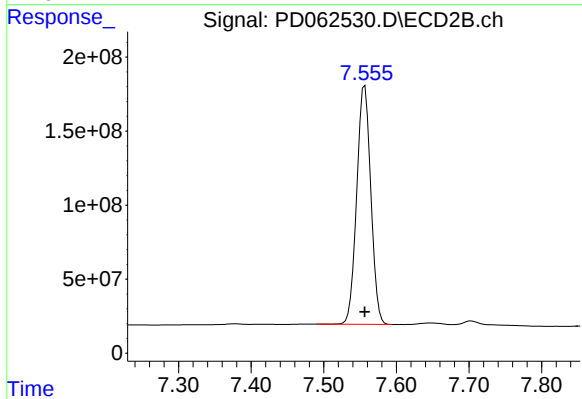

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 2171860272
Conc: 371.64 ng/ml

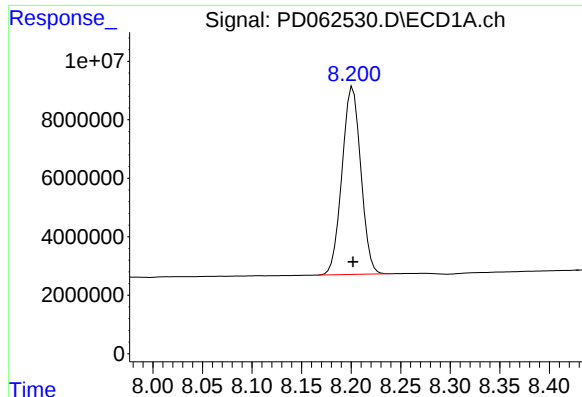

#27 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 84709412
Conc: 77.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

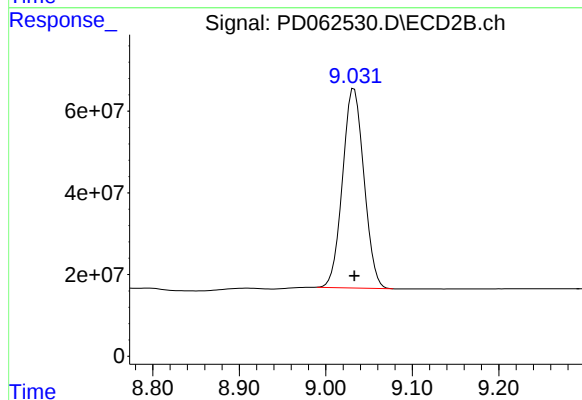

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 835950126
Conc: 75.10 ng/ml