

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 12:32
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 12:44:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 29 12:30:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.973	74053405	884.5E6	77.276	71.928
27)	SA Decachlor...	8.201	9.034	162.9E6	1572.7E6	148.698	141.296
Target Compounds							
2)	A alpha-BHC	3.878	4.361	118.1E6	1406.8E6	84.405	73.530
3)	MA gamma-BHC...	4.161	4.646	109.1E6	1287.1E6	82.248	73.581
4)	MA Heptachlor	4.462	5.154	104.7E6	1279.2E6	81.330	72.256
9)	A Endosulfan I	5.493	6.202	88582123	1063.4E6	79.145	71.609
13)	MA Dieldrin	5.736	6.459	207.3E6	2286.9E6	163.658	144.503
14)	MA Endrin	5.994	6.676	172.6E6	1856.9E6	162.492	146.315
16)	A 4,4'-DDD	6.121	6.799	165.7E6	1845.2E6	163.929	146.220
17)	MA 4,4'-DDT	6.362	7.098	168.7E6	1848.6E6	176.430	151.552
20)	A Methoxychlor	6.909	7.557	411.6E6	4005.9E6	746.623	685.480


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 12:32
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 12:44:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 29 12:30:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

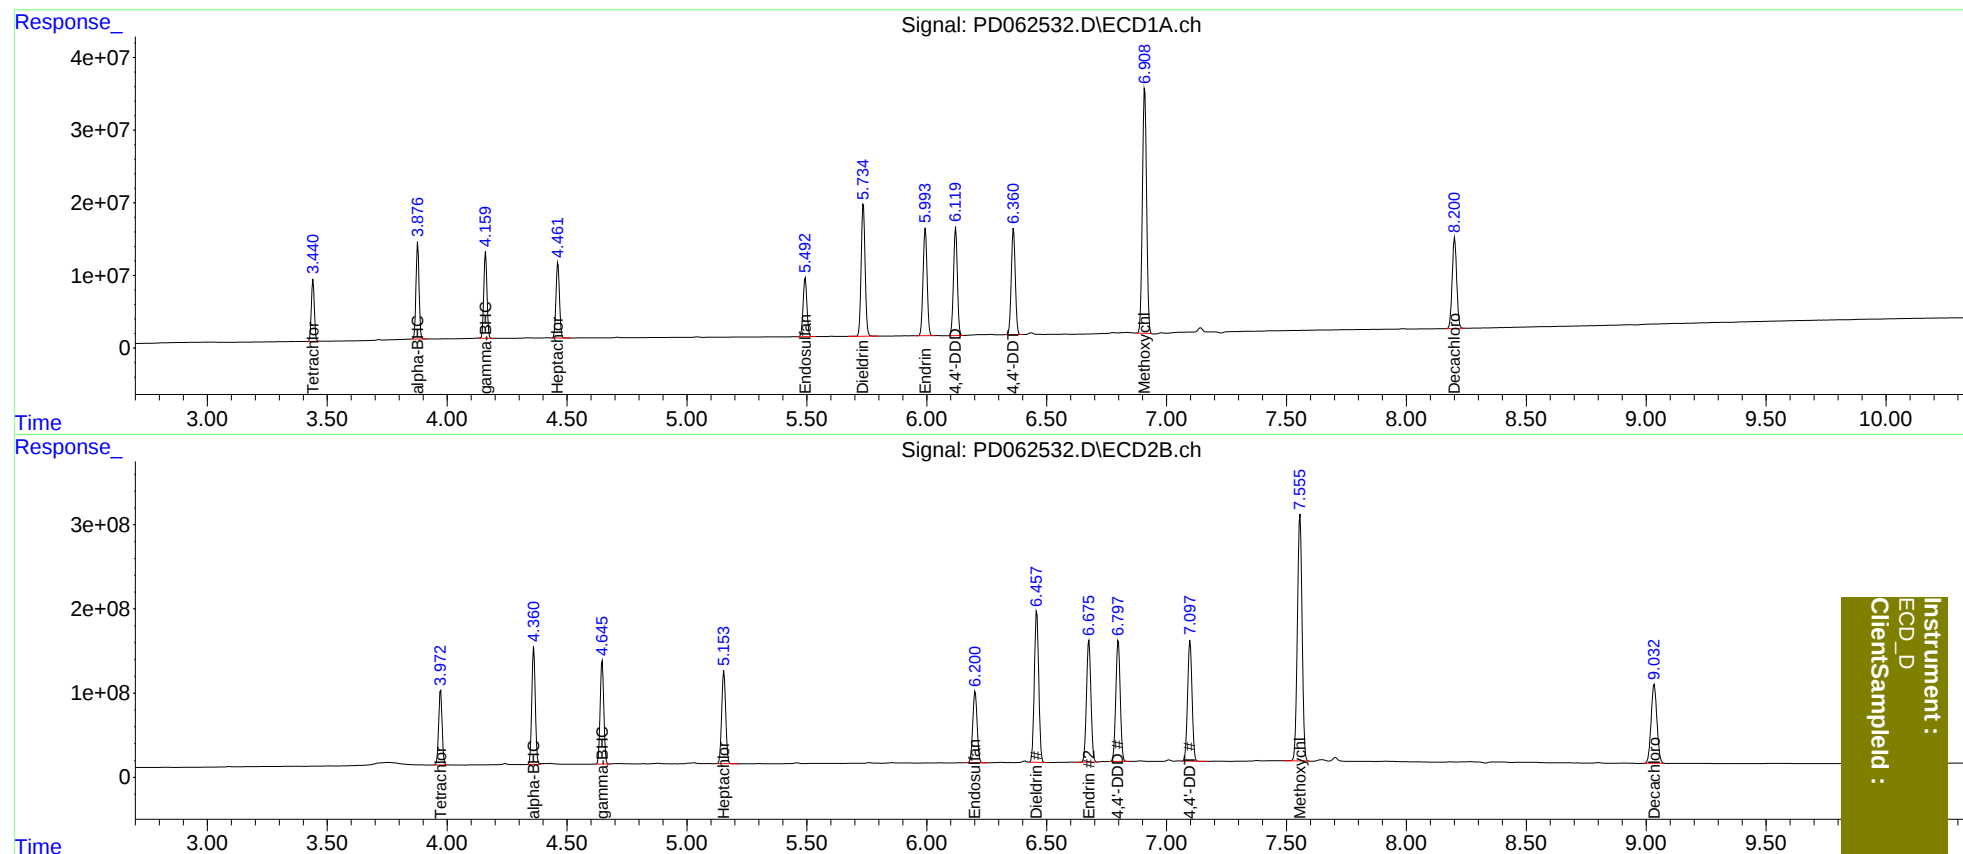


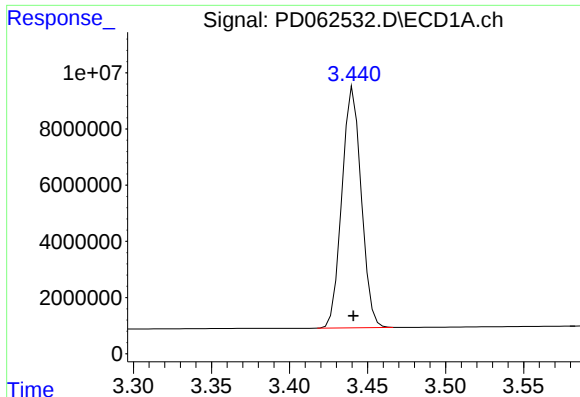

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 74053405
Conc: 77.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

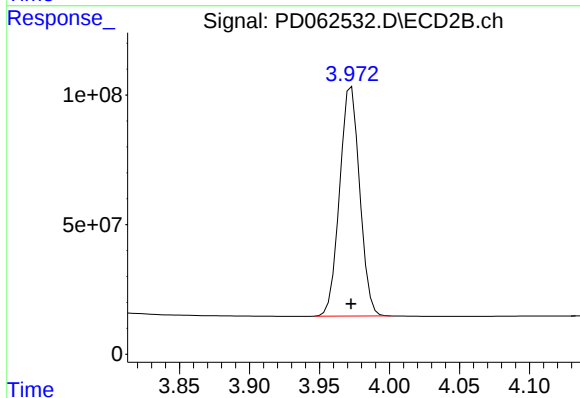


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 884492221
Conc: 71.93 ng/ml

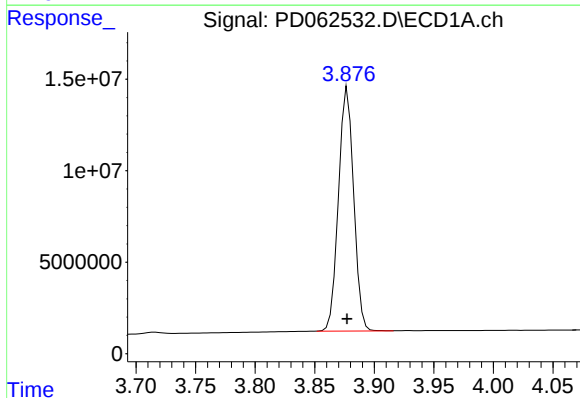


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 118068646
Conc: 84.41 ng/ml

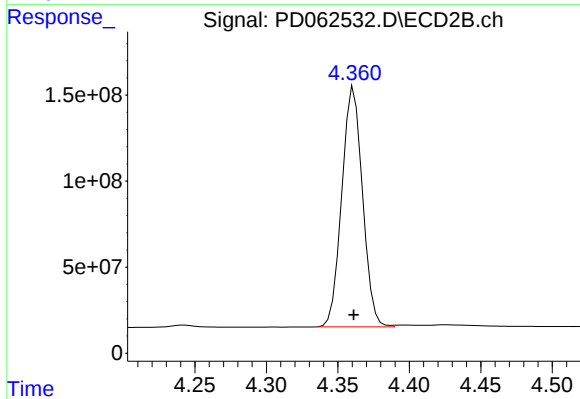

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 1406811095
Conc: 73.53 ng/ml

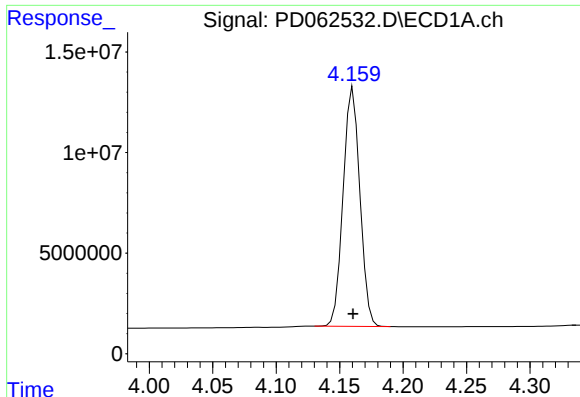

#3 gamma-BHC (Lindane)


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 109095082
Conc: 82.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

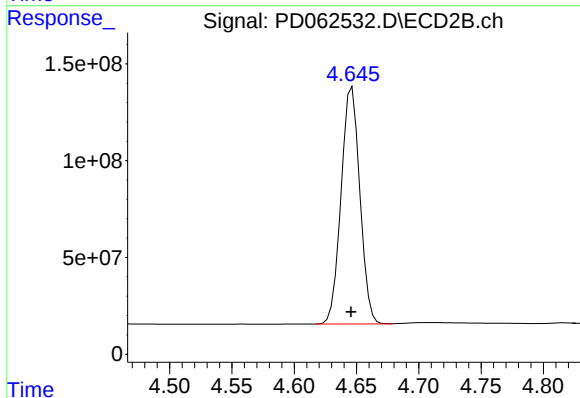


#3 gamma-BHC (Lindane)

R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 1287081570
Conc: 73.58 ng/ml

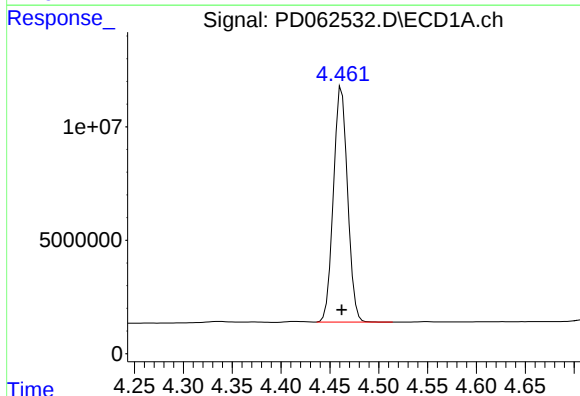


#4 Heptachlor

R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 104651281
Conc: 81.33 ng/ml

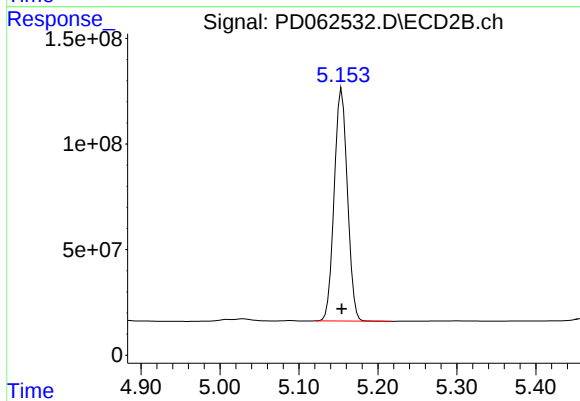

#4 Heptachlor


R.T.: 5.154 min
Delta R.T.: 0.000 min
Response: 1279227155
Conc: 72.26 ng/ml

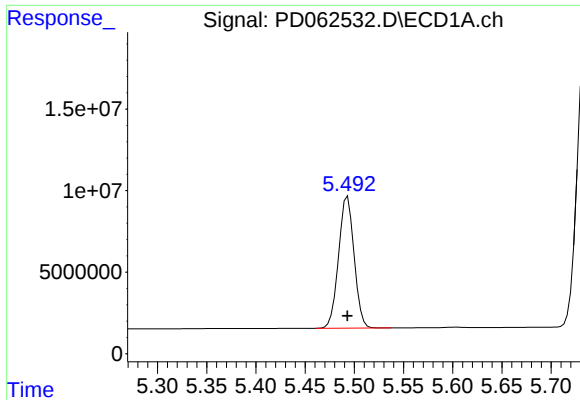

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 88582123
Conc: 79.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

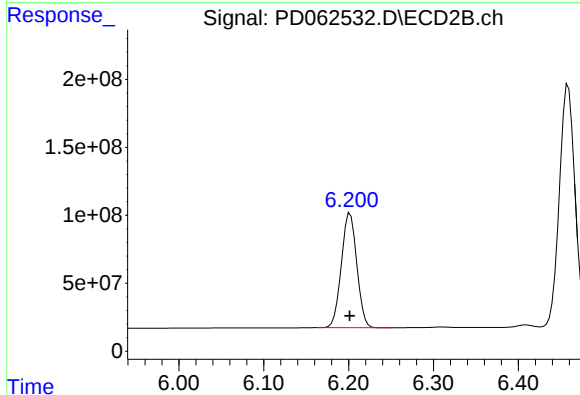


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 1063365835
Conc: 71.61 ng/ml

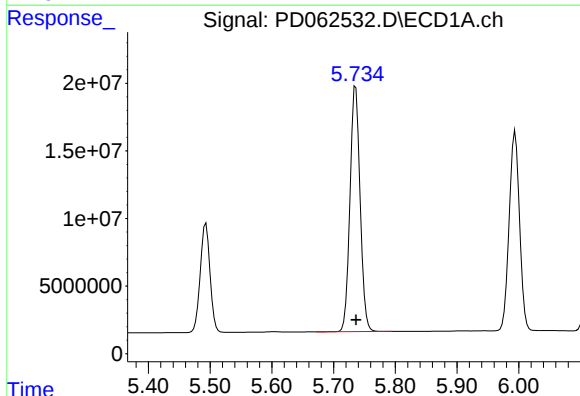


#13 Dieldrin

R.T.: 5.736 min
Delta R.T.: 0.000 min
Response: 207346282
Conc: 163.66 ng/ml

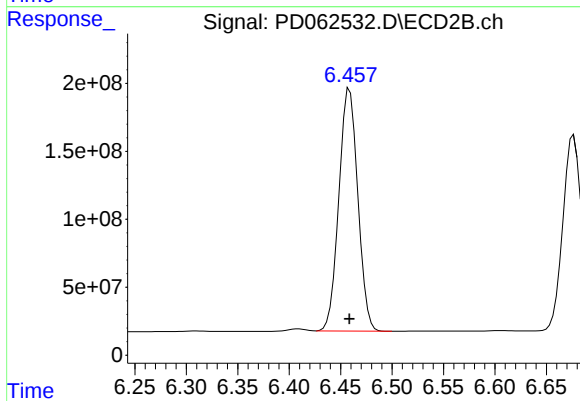

#13 Dieldrin


R.T.: 6.459 min
Delta R.T.: 0.000 min
Response: 2286932198
Conc: 144.50 ng/ml

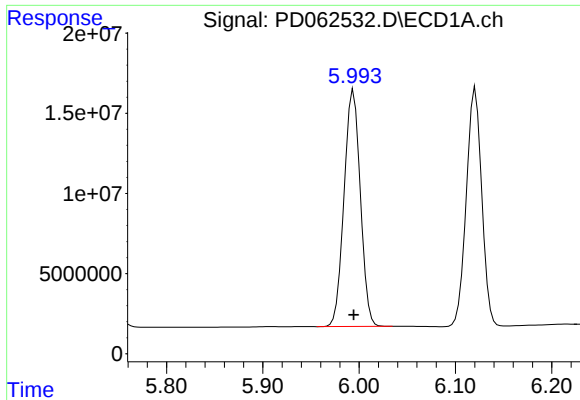

#14 Endrin


R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 172595832
Conc: 162.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

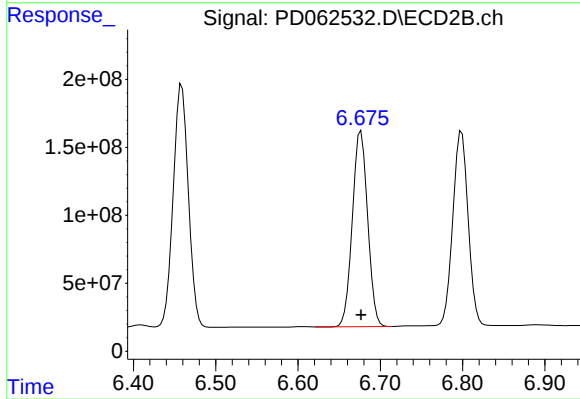


#14 Endrin

R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 1856893226
Conc: 146.31 ng/ml

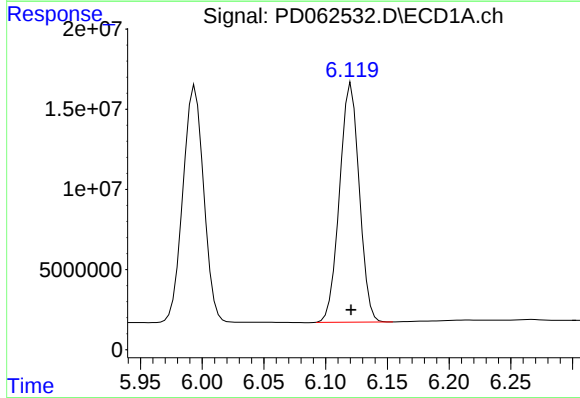


#16 4,4'-DDD

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 165701427
Conc: 163.93 ng/ml

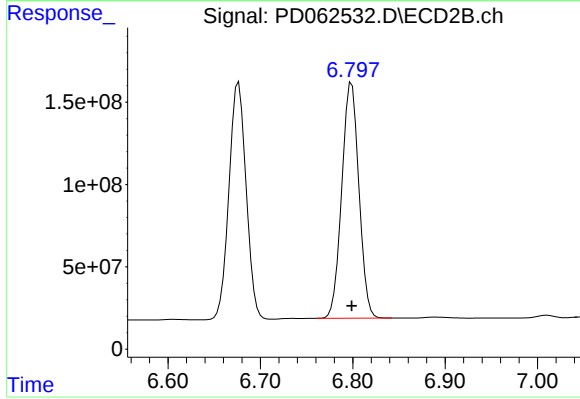

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 1845168403
Conc: 146.22 ng/ml

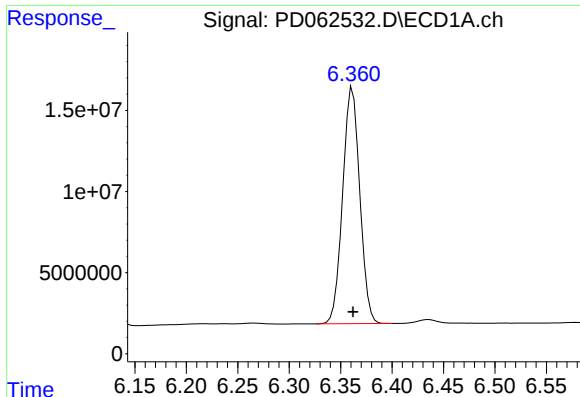

#17 4,4'-DDT


R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 168735127
Conc: 176.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

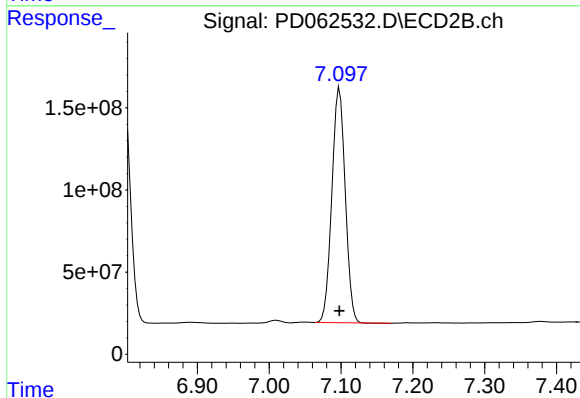


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: 0.000 min
Response: 1848579326
Conc: 151.55 ng/ml

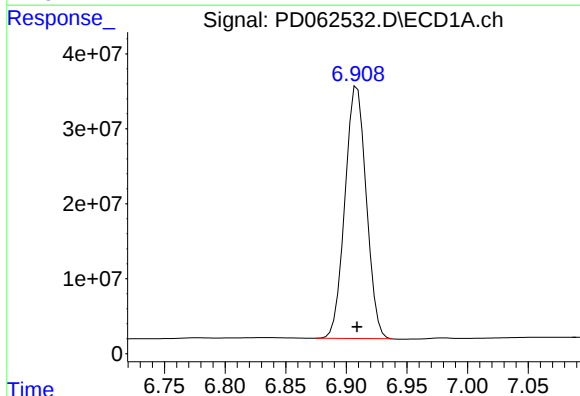


#20 Methoxychlor

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 411579208
Conc: 746.62 ng/ml

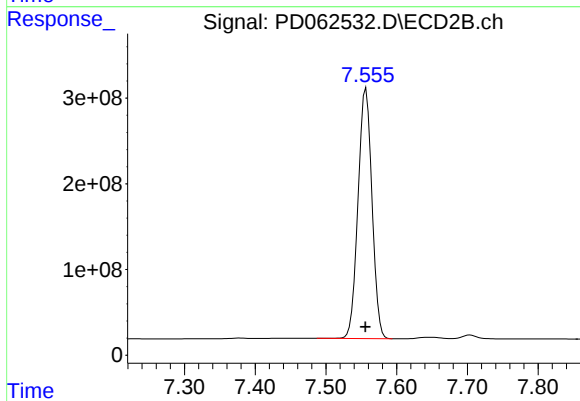

#20 Methoxychlor

R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 4005918875
Conc: 685.48 ng/ml

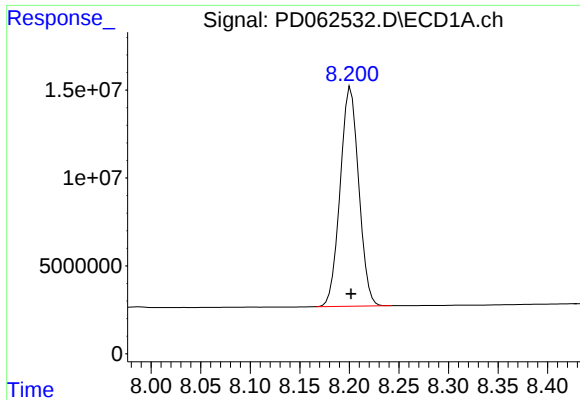

#27 Decachlorobiphenyl


R.T.: 8.201 min

Delta R.T.: 0.000 min

Response: 162939908

Conc: 148.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

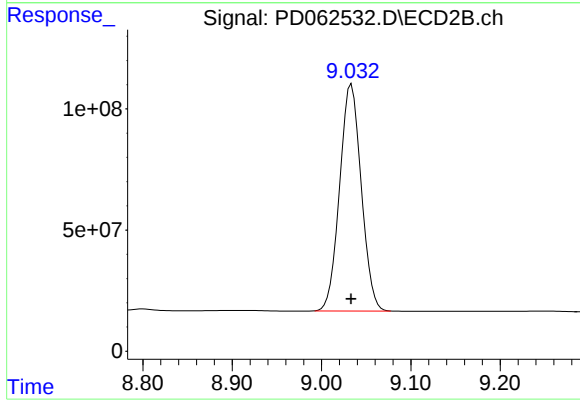

#27 Decachlorobiphenyl

R.T.: 9.034 min

Delta R.T.: 0.000 min

Response: 1572703168

Conc: 141.30 ng/ml