

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 12:04
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 12:31:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 29 12:30:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.973	37626801	463.9E6	39.264	37.726
27)	SA Decachlor...	8.202	9.033	84709412	836.0E6	77.305	75.104
Target Compounds							
2)	A alpha-BHC	3.878	4.361	57640459	728.4E6	41.206	38.069
3)	MA gamma-BHC...	4.161	4.646	53786282	667.2E6	40.550	38.144
4)	MA Heptachlor	4.463	5.154	51956405	663.7E6	40.378	37.486
9)	A Endosulfan I	5.493	6.202	44474155	561.5E6	39.736	37.811
13)	MA Dieldrin	5.736	6.459	103.1E6	1205.3E6	81.369	76.158
14)	MA Endrin	5.994	6.677	85229154	967.4E6	80.240	76.228
16)	A 4,4'-DDD	6.121	6.799	82221414	965.7E6	81.342	76.527
17)	MA 4,4'-DDT	6.362	7.098	80860667	948.7E6	84.548	77.774
20)	A Methoxychlor	6.909	7.556	215.0E6	2171.9E6	389.954	371.642

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 12:04
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 12:31:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 29 12:30:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

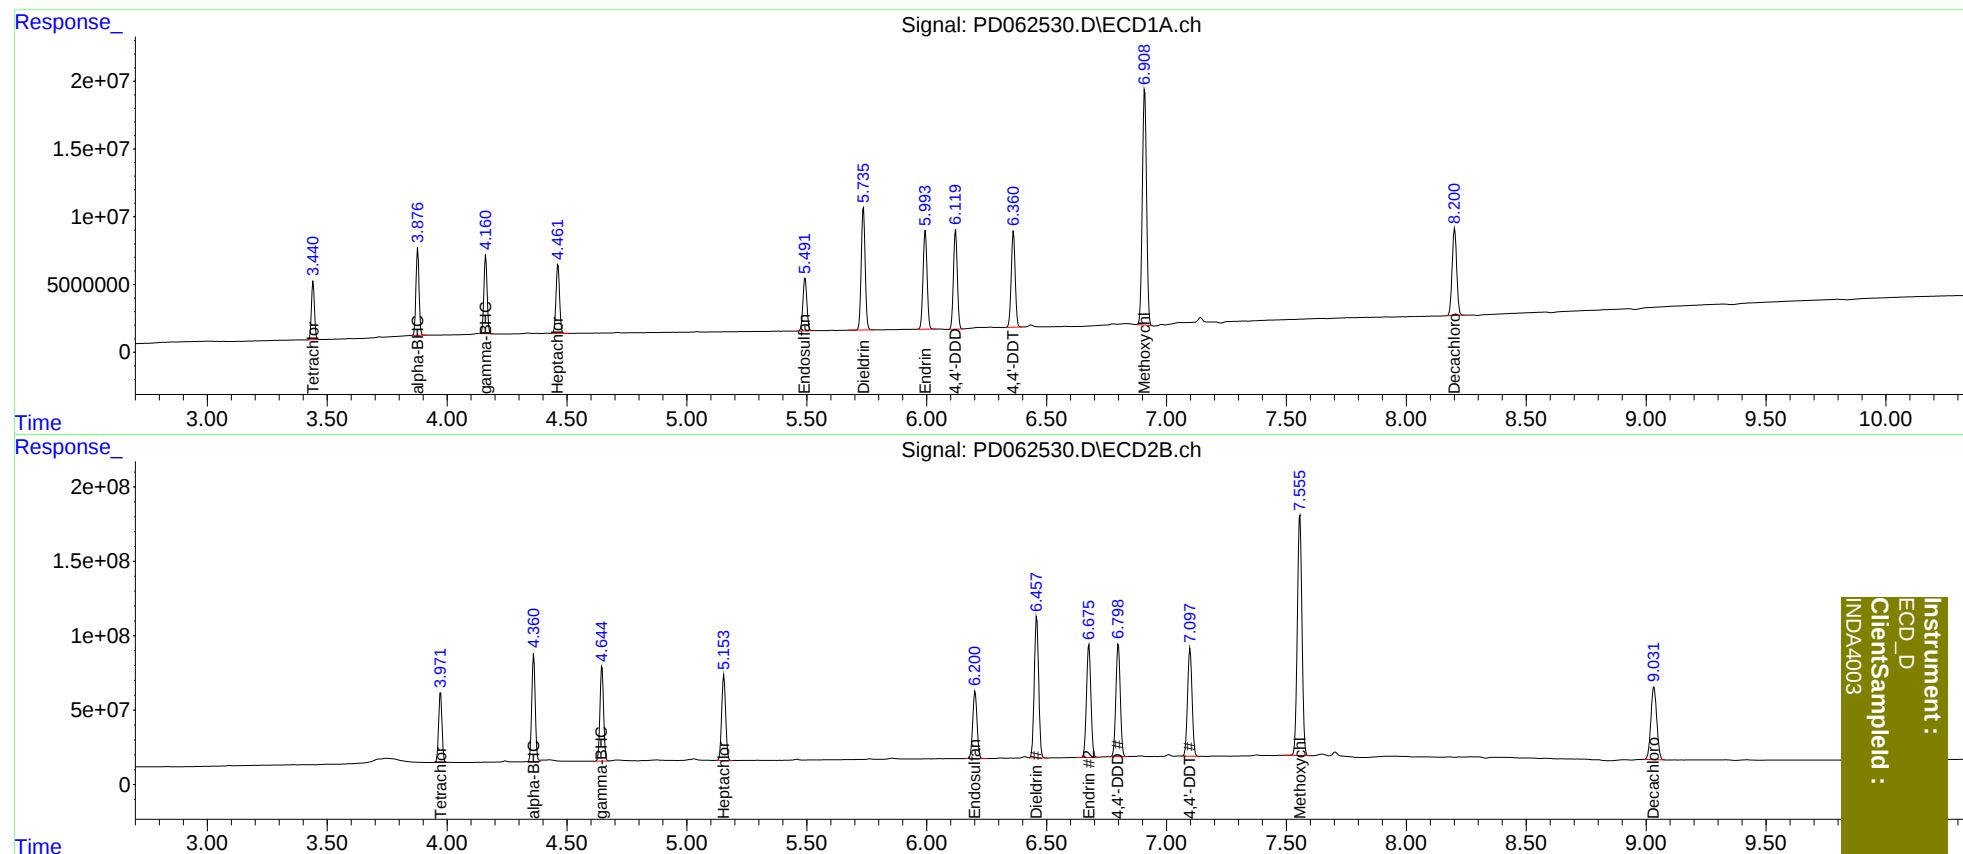

Instrument :
ECD_D
ClientSample :
INDA4003