

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 17:12
 Operator : AR\AJ
 Sample : M2161-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ2

Manual Integrations
 APPROVED

Ankita
 5/3/2021 2:57:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 08:29:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.974	15736788	195.3E6	16.437	16.083
27)	SA Decachlor...	8.202	9.036	32217779	323.4E6	30.015	29.628
Target Compounds							
8)	B Heptachlo...	5.153	5.845	3391282	82577637	2.767m	5.149 #
10)	B trans-Chl...	5.380	6.079	3459111	53388891	2.759m	3.260m
11)	B cis-Chlor...	5.440	6.154	4526407	73212386	3.686	4.717 #
13)	MA Dieldrin	5.737	6.460	19242185	251.5E6	15.265	16.220
21)	B Endrin ke...	7.143	7.704	842749	18547187	0.719	1.507 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 17:12
Operator : AR\AJ
Sample : M2161-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 08:29:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

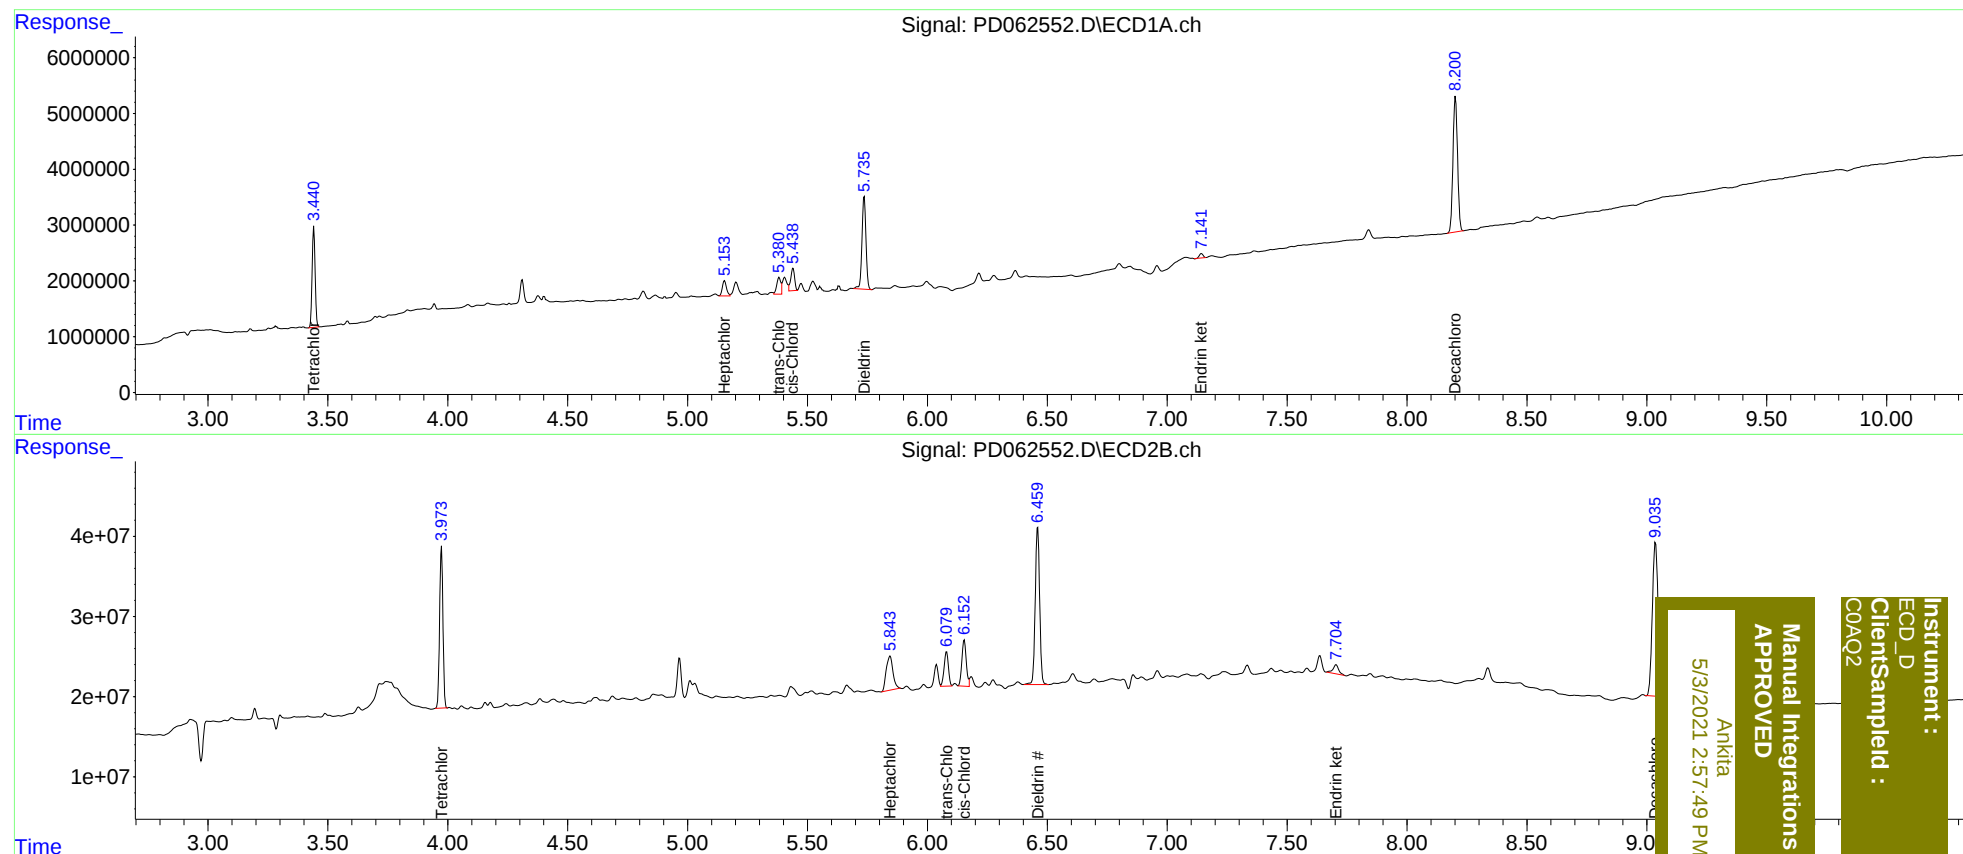

5/3/2021 2:57:49 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C0A02