

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 19:31
 Operator : AR\AJ
 Sample : INDA331
 Misc :
 ALS Vial : 43 Sample Multiplier: 1


Instrument :
 ECD_D
 LabSampleId :
 INDA331

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:31:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 03:01:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

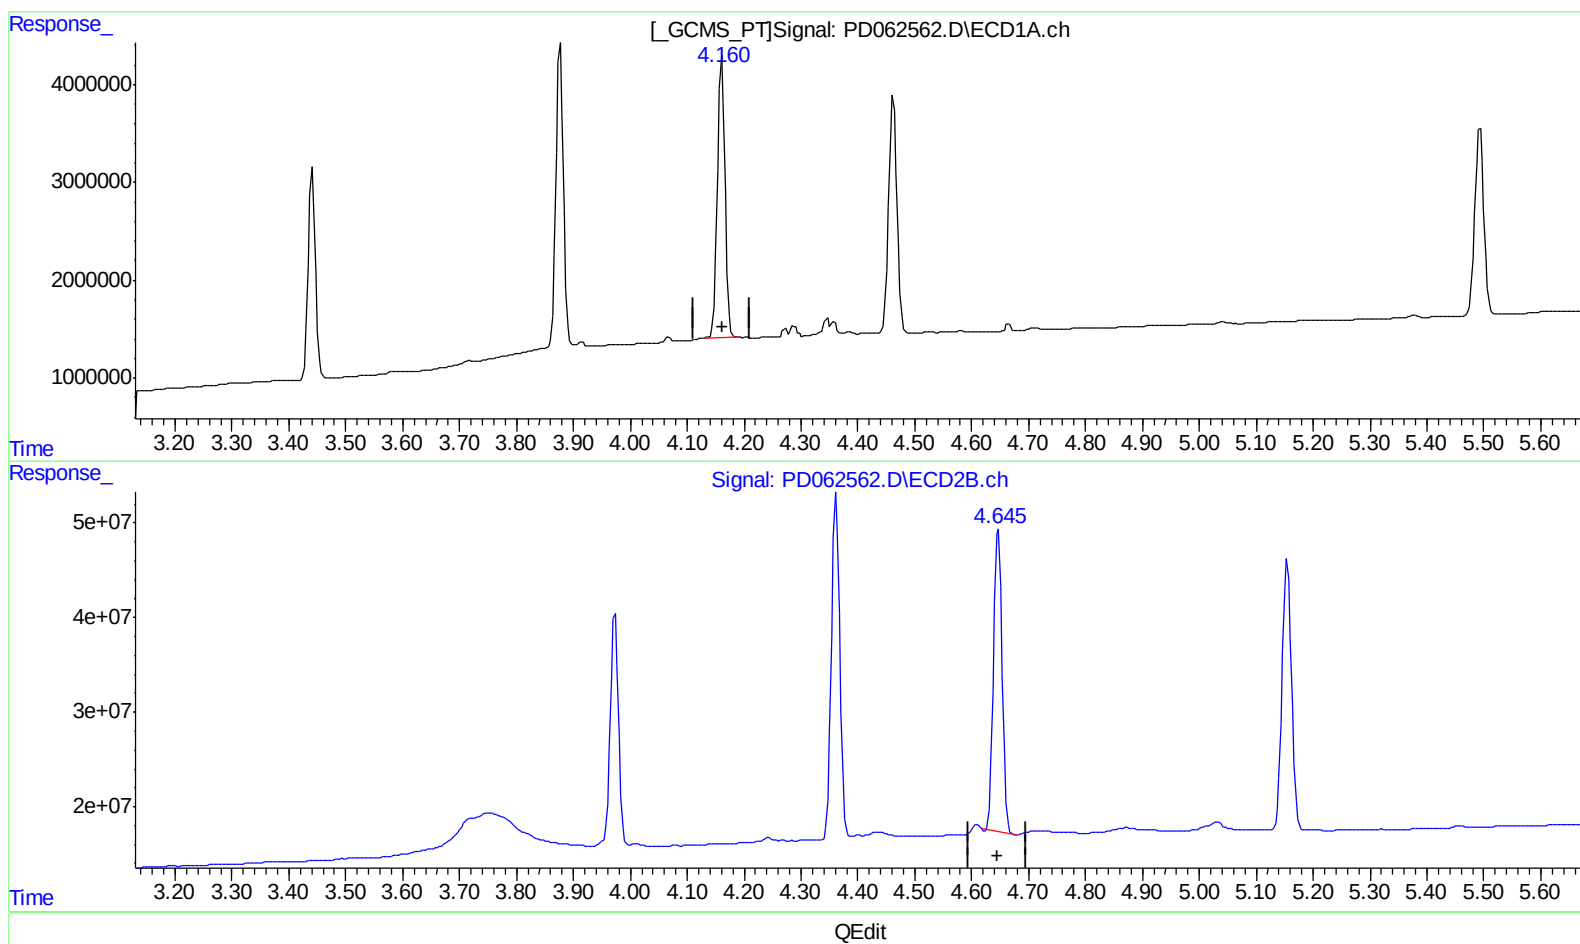

(3) gamma-BHC (Lindane) (MA)

4.161min 19.814 ng/ml

response 26468130

(3) gamma-BHC (Lindane) #2 (MA)

4.647min 19.136 ng/ml

response 330573038

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 19:31
Operator : AR\AJ
Sample : INDA331
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA331

Manual Integrations
APPROVED

Ankita
4/30/2021 2:31:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 03:01:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

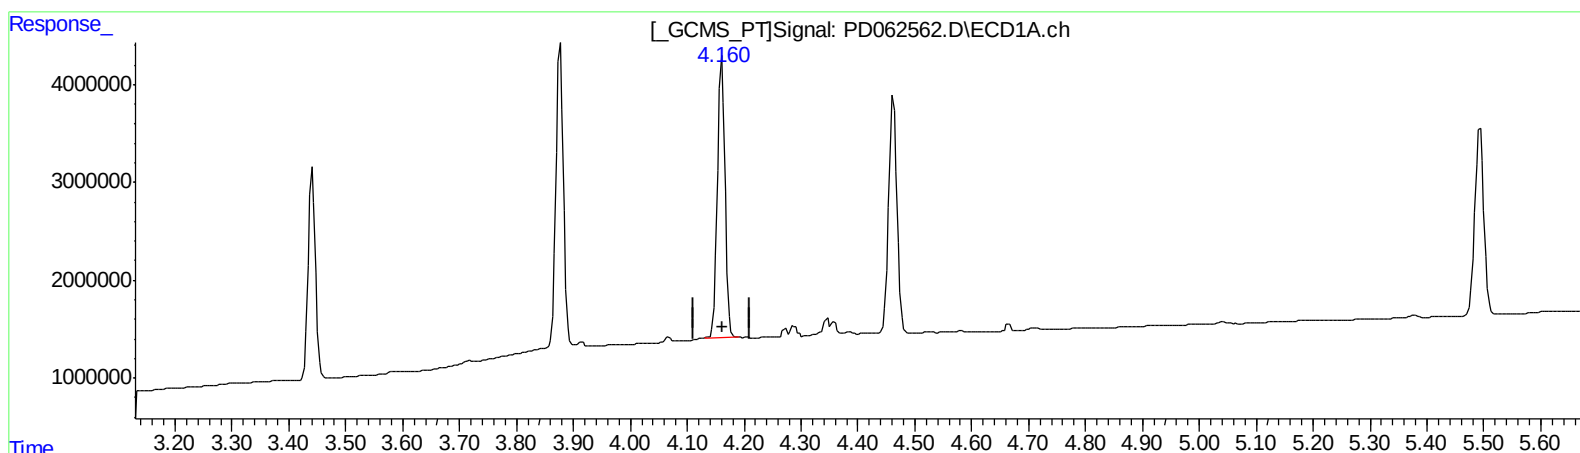

(3) gamma-BHC (Lindane) (MA)

4.161min 19.814 ng/ml

response 26468130

(3) gamma-BHC (Lindane) #2 (MA)

4.645min 19.765 ng/ml m

response 341442602

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 19:31
 Operator : AR\AJ
 Sample : INDA331
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA331

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:31:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 03:01:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.441	3.973	19037255	238.6E6	19.884	19.650
27) SA Decachlor...	8.202	9.036	43463535	451.9E6	40.492	41.397
Target Compounds						
2) A alpha-BHC	3.877	4.362	28166426	374.2E6	20.118	19.787
3) MA gamma-BHC...	4.161	4.645	26468130	341.4E6	19.814	19.765m
4) MA Heptachlor	4.462	5.155	24485187	330.4E6	19.069	18.982
9) A Endosulfan I	5.493	6.203	21469876	292.9E6	19.201	19.967
13) MA Dieldrin	5.737	6.460	50258953	624.8E6	39.872	40.296
14) MA Endrin	5.994	6.678	41453098	488.6E6	39.177	39.180
16) A 4,4'-DDD	6.121	6.800	40063070	499.7E6	40.233	40.203
17) MA 4,4'-DDT	6.362	7.099	35969457	452.5E6	38.403	38.115
20) A Methoxychlor	6.909	7.557	102.4E6	1073.6E6	191.951	189.402

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 05/25/21