

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 15:20
 Operator : AR\AJ
 Sample : M2127-12MS
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AB4MS

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:31:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:56:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.973	12766000	154.8E6	13.334	12.751
27)	SA Decachlor...	8.200	9.035	30002242	280.7E6	27.951m	25.713
Target Compounds							
2)	A alpha-BHC	3.877	4.361	36369145	412.5E6	25.976	21.813
3)	MA gamma-BHC...	4.161	4.646	33658423	400.5E6	25.197	23.185
4)	MA Heptachlor	4.462	5.155	35808403	403.8E6	27.888	23.198
5)	MB Aldrin	4.710	5.460	32059559	428.3E6	24.612	24.760
6)	B beta-BHC	4.411	4.816	14645833	133.8E6	23.590	17.524m#
7)	B delta-BHC	4.616	5.034	14602012	171.4E6	10.731	9.237
8)	B Heptachlo...	5.154	5.845	32819013	364.6E6	26.781	22.731
9)	A Endosulfan I	5.493	6.202	28252565	365.3E6	25.266	24.904
10)	B trans-Chl...	5.381	6.080	31049245	363.5E6	24.767	22.195
11)	B cis-Chlor...	5.440	6.152	28717592	369.6E6	23.387	23.813
12)	B 4,4'-DDE	5.604	6.310	62078707	732.8E6	50.162	46.764
13)	MA Dieldrin	5.737	6.459	67253425	836.7E6	53.354	53.962
14)	MA Endrin	5.994	6.677	61495667	640.4E6	58.120	51.346
15)	B Endosulfa...	6.267	6.886	53110621	588.1E6	51.210	46.989
16)	A 4,4'-DDD	6.121	6.800	53355455	618.4E6	53.582	49.753
17)	MA 4,4'-DDT	6.362	7.098	52883542	604.8E6	56.461	50.941
18)	B Endrin al...	6.436	7.011	47026972	544.8E6	52.706	49.933
19)	B Endosulfa...	6.650	7.237	40768124	829.5E6	40.784	65.003 #
20)	A Methoxychlor	6.907	7.557	150.3E6	1491.4E6	281.684m	263.117
21)	B Endrin ke...	7.142	7.704	65017579	651.0E6	55.480	52.897

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 15:20
Operator : AR\AJ
Sample : M2127-12MS
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:56:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

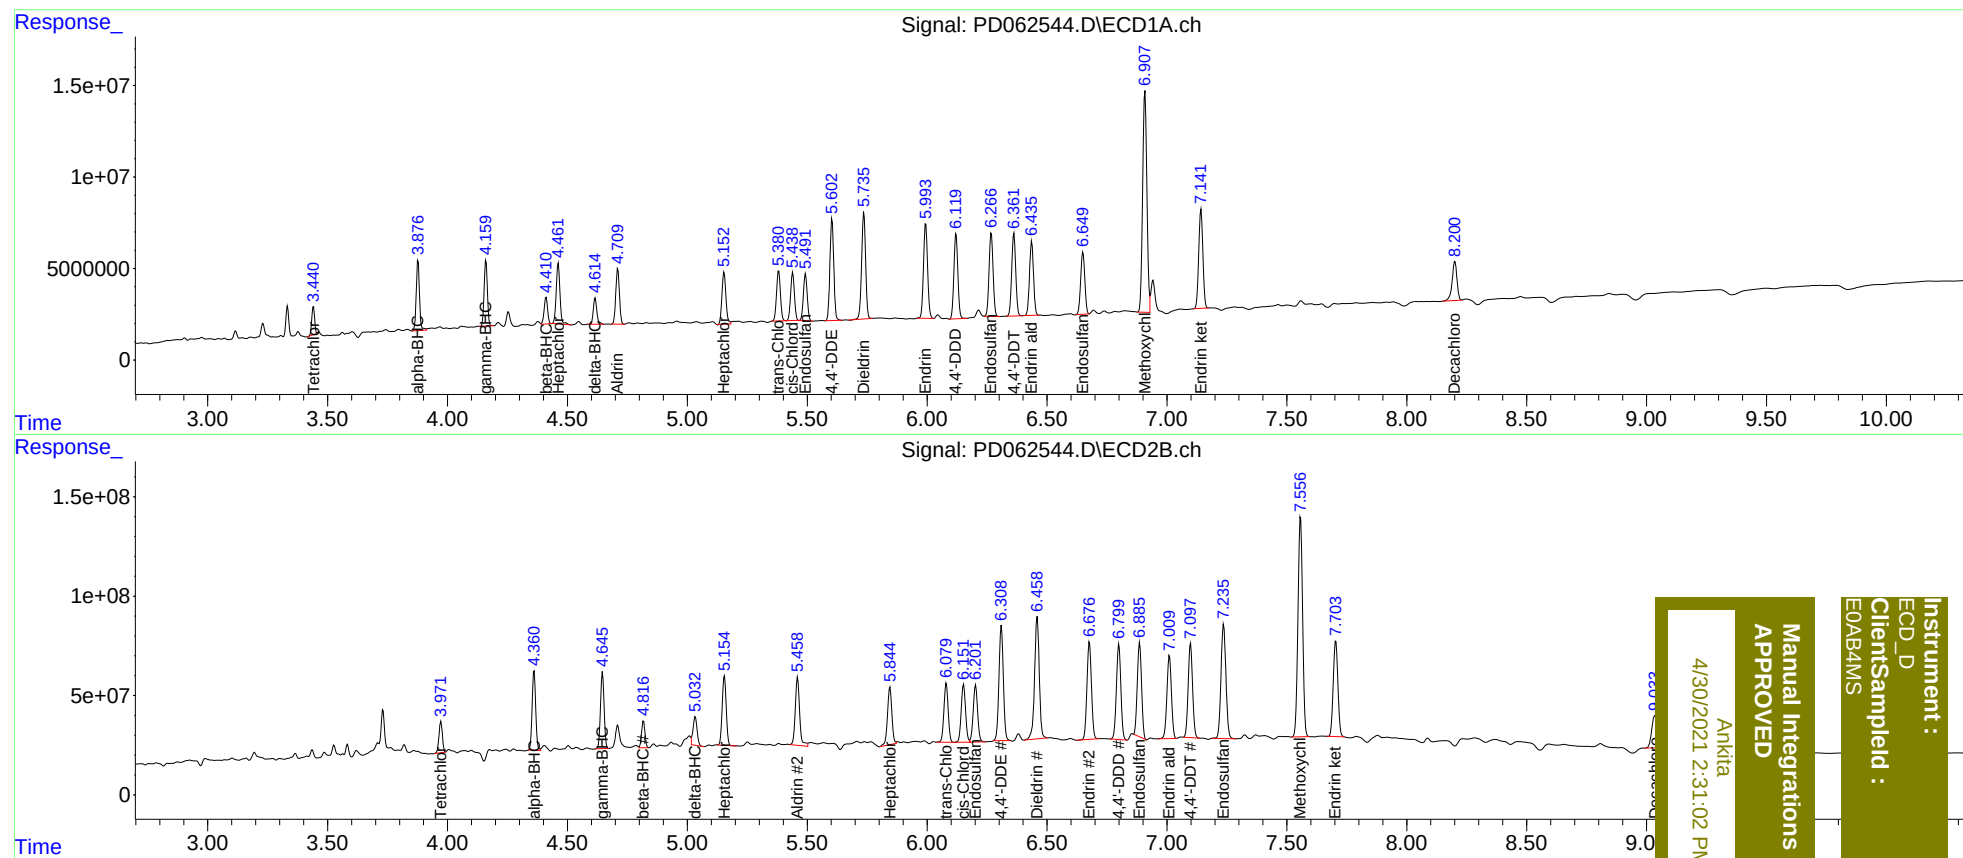

4/30/2021 2:31:02 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
E0AB4M5