

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
 Data File : PD062560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 19:03
 Operator : AR\AJ
 Sample : PB135896BS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS896

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:31:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 03:01:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.972	18102771	217.5E6	18.908m	17.913m
27)	SA Decachlor...	8.202	9.036	38678457	402.0E6	36.034	36.833
Target Compounds							
2)	A alpha-BHC	3.877	4.362	5341612	77111082	3.815	4.078
3)	MA gamma-BHC...	4.160	4.645	5237389	73091179	3.921	4.231m
4)	MA Heptachlor	4.462	5.155	4729655	68173835	3.683	3.917
5)	MB Aldrin	4.710	5.460	4856239	69673997	3.728	4.028
6)	B beta-BHC	4.412	4.817	2493809	28731847	4.017	3.764
7)	B delta-BHC	4.616	5.033	4941151	77751519	3.631	4.191
8)	B Heptachlo...	5.153	5.846	4628044	71582778	3.777	4.463
9)	A Endosulfan I	5.493	6.202	4213194	57325727	3.768	3.909
10)	B trans-Chl...	5.380	6.080	5081359	61955556	4.053	3.783
11)	B cis-Chlor...	5.440	6.153	4529202	60425987	3.688	3.893
12)	B 4,4'-DDE	5.604	6.310	8800832	121.7E6	7.111	7.767
13)	MA Dieldrin	5.736	6.460	9326232	126.6E6	7.399	8.166
14)	MA Endrin	5.994	6.677	8591856	102.2E6	8.120	8.195
15)	B Endosulfa...	6.268	6.887	8100144	115.4E6	7.810	9.223
16)	A 4,4'-DDD	6.120	6.800	7347500	109.9E6	7.379	8.846
17)	MA 4,4'-DDT	6.362	7.098	5968453	86377103	6.372	7.275
18)	B Endrin al...	6.437	7.011	7246055	91964841	8.121	8.429
19)	B Endosulfa...	6.650	7.233	7349241	102.3E6	7.352	8.014
20)	A Methoxychlor	6.910	7.558	19840645	225.5E6	37.185	39.783
21)	B Endrin ke...	7.143	7.705	8958639	103.0E6	7.644	8.368

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042921\
Data File : PD062560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 19:03
Operator : AR\AJ
Sample : PB135896BS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 03:01:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

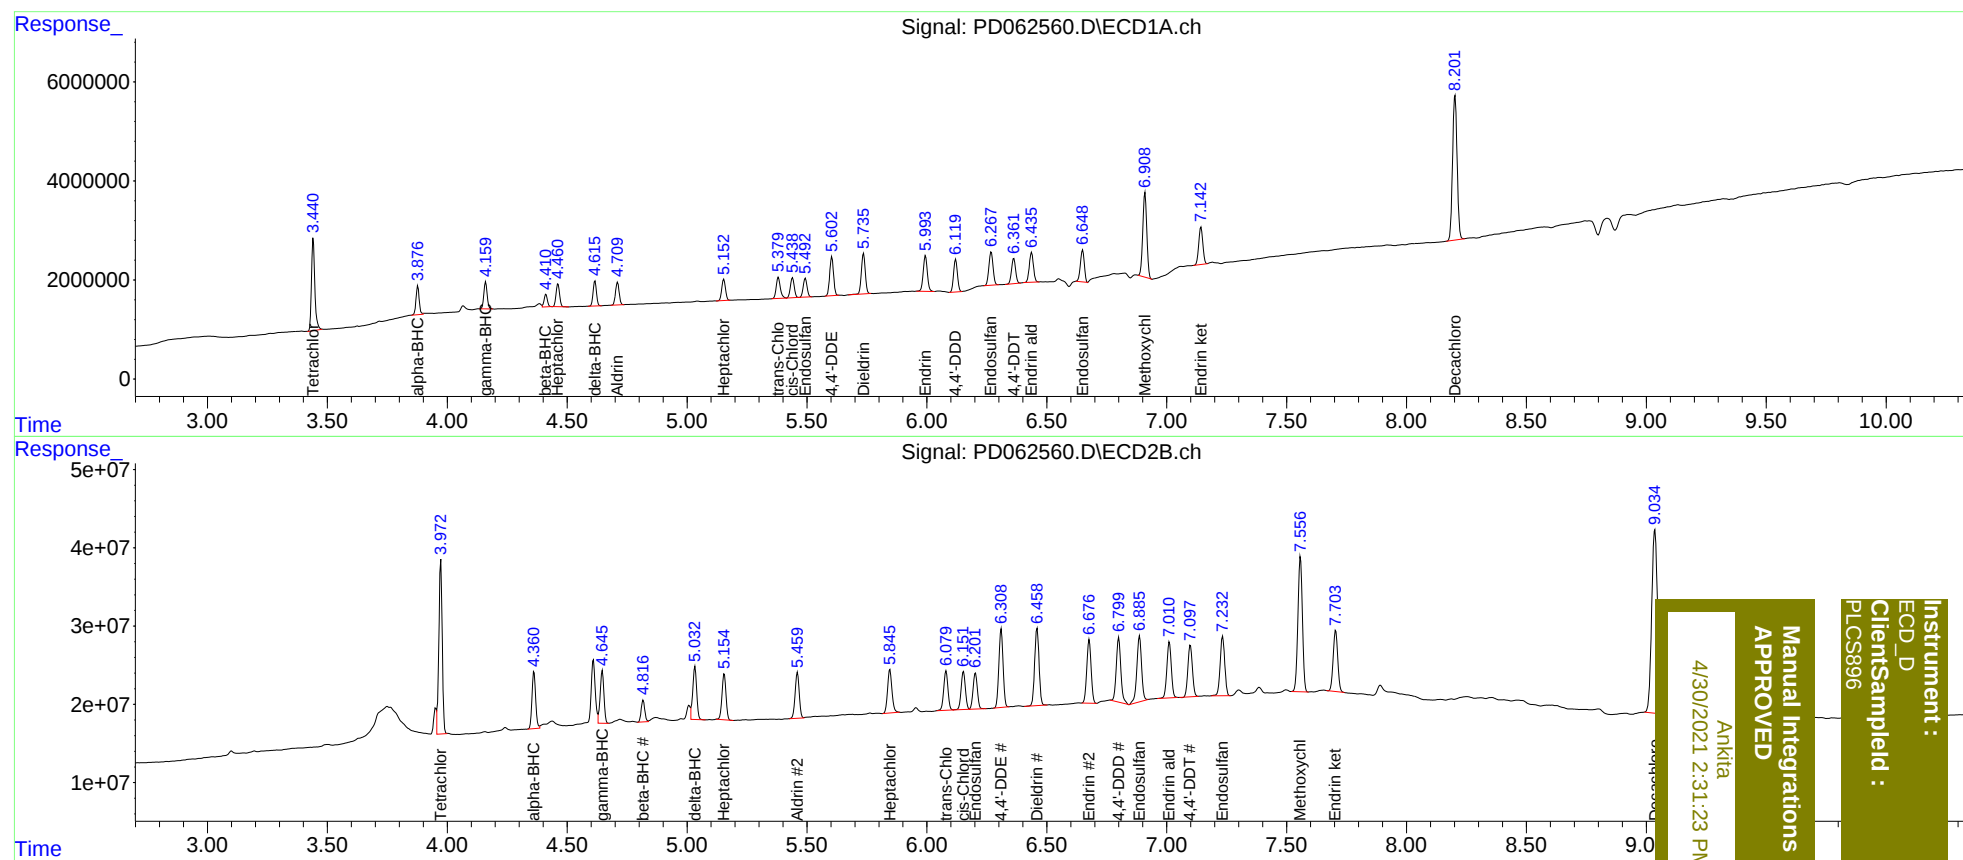

Manual Integrations
APPROVED

Ankita
4/30/2021 2:31:23 PM

Instrument :
ECD_D
ClientSampled :
PLCS896