

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042922\
 Data File : PD069314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2022 20:12
 Operator : AR\AJ
 Sample : N2616-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 01:02:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:40:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	12119487	112.4E6	10.918	10.484
28)	SA Decachlor...	8.199	9.368	11767498	65148507	9.424	9.955
Target Compounds							
3)	MA gamma-BHC...	4.170	0.000	2431484	0	1.421	N.D. #
10)	B gamma-Chl...	0.000	6.317	0	1548920	N.D.	0.133 #
12)	B 4,4'-DDE	0.000	6.548	0	447439	N.D.	0.041 #
14)	MA Endrin	0.000	6.949f	0	2545047	N.D.	0.281 #
17)	MA 4,4'-DDT	0.000	7.350	0	316008	N.D.	0.036 #
21)	B Endrin ke...	0.000	7.968	0	2498966	N.D.	0.276 #
22)	Mirex	0.000	8.419	0	287666	N.D.	0.045 #
23)	Chlordane-1	0.000	5.169f	0	1857003	N.D.	3.866 #
25)	Chlordane-3	0.000	6.317	0	1548920	N.D.	0.951 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042922\
Data File : PD069314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2022 20:12
Operator : AR\AJ
Sample : N2616-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 01:02:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:40:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

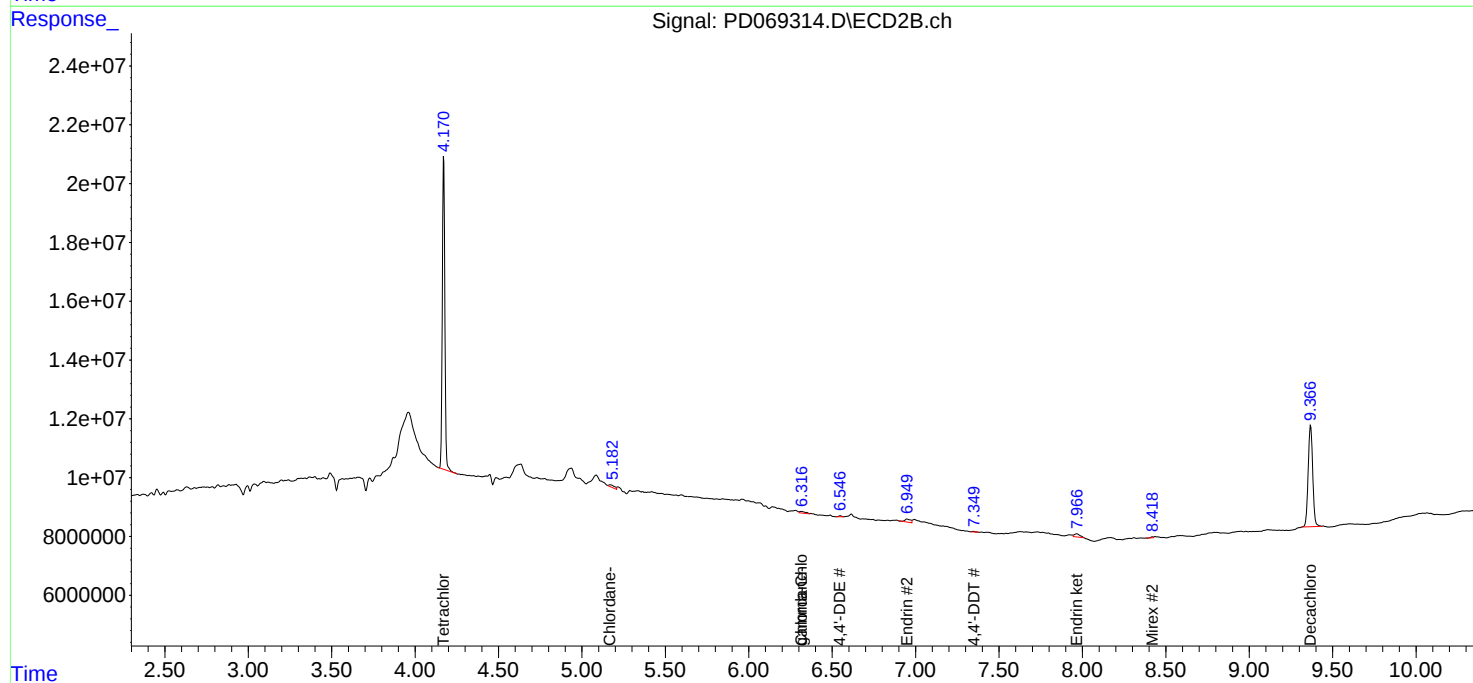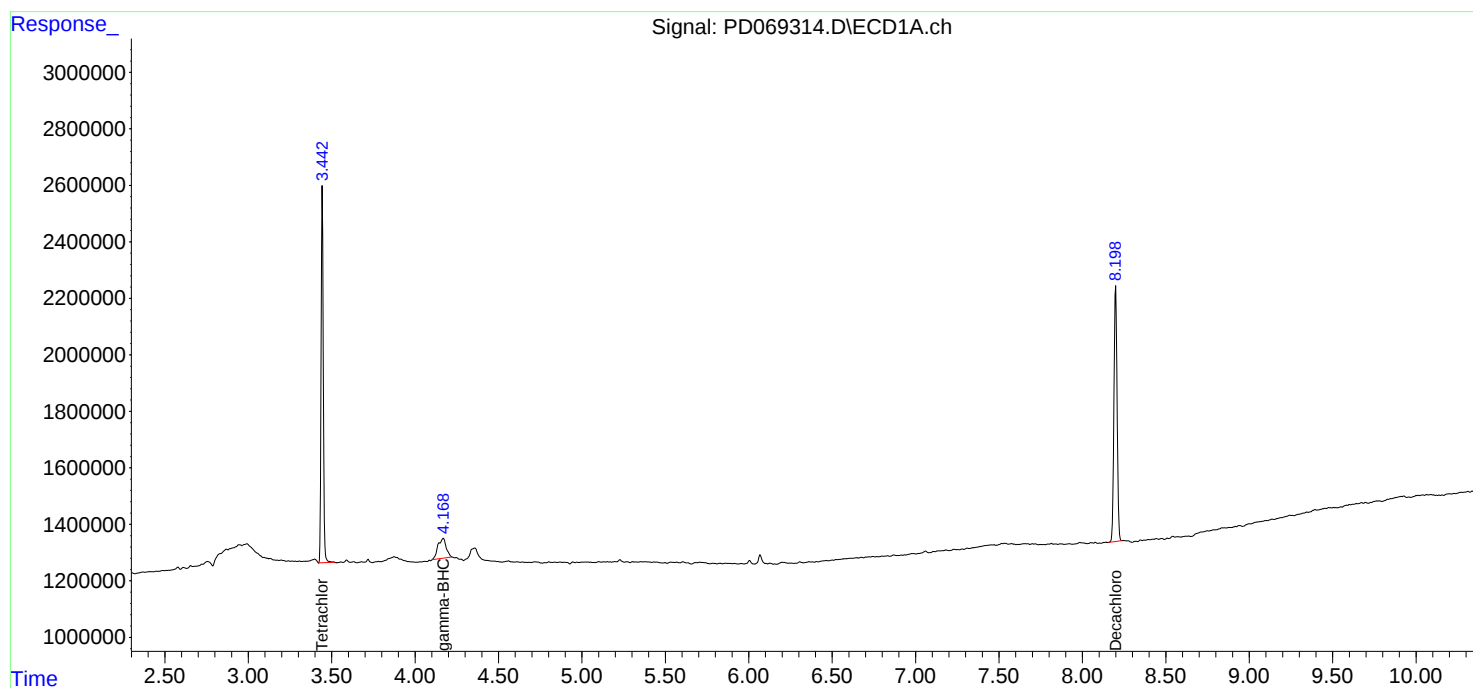


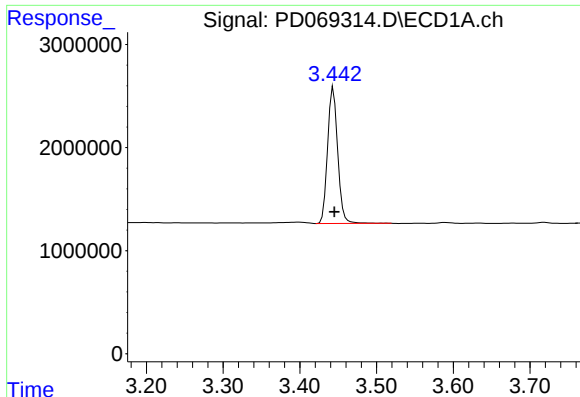

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 12119487
Conc: 10.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

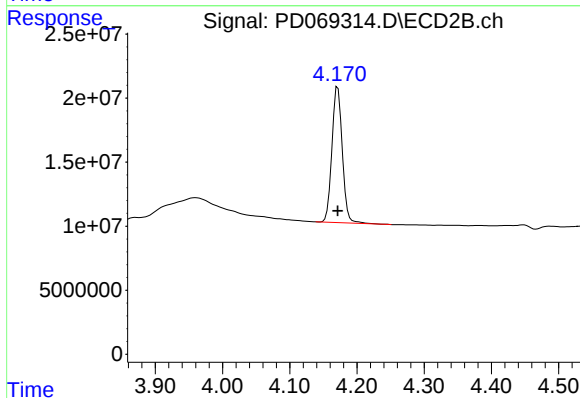


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 112410807
Conc: 10.48 ng/ml

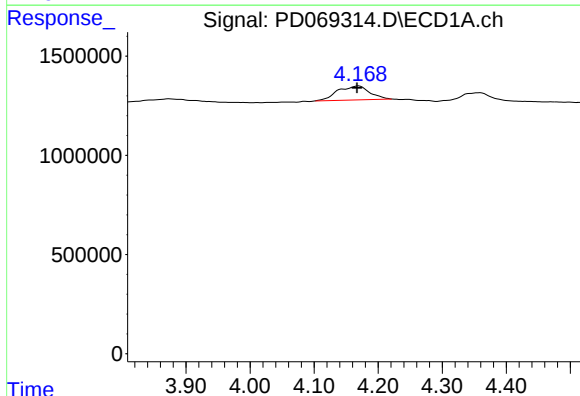


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: 0.003 min
Response: 2431484
Conc: 1.42 ng/ml

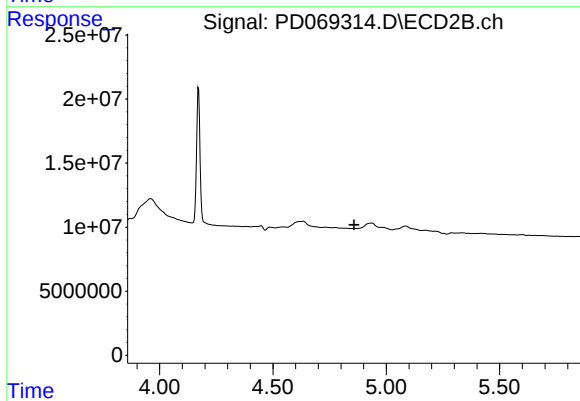

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.858 min
Response: 0
Conc: N.D.

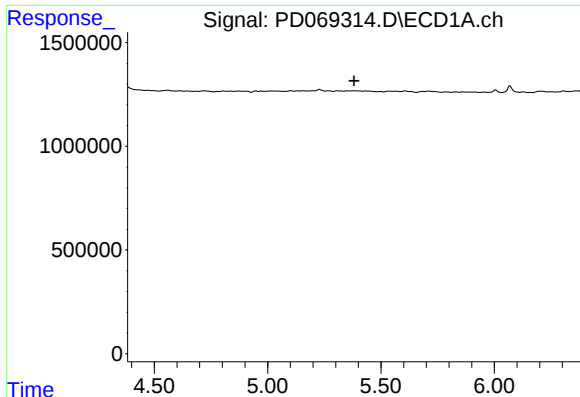

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.381 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

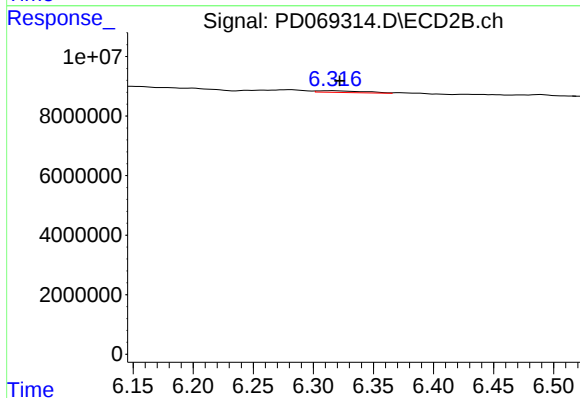


#10 gamma-Chlordane

R.T.: 6.317 min
Delta R.T.: -0.005 min
Response: 1548920
Conc: 0.13 ng/ml

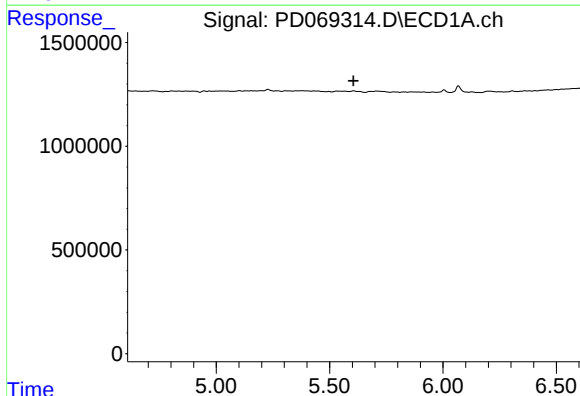


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.606 min
Response: 0
Conc: N.D.

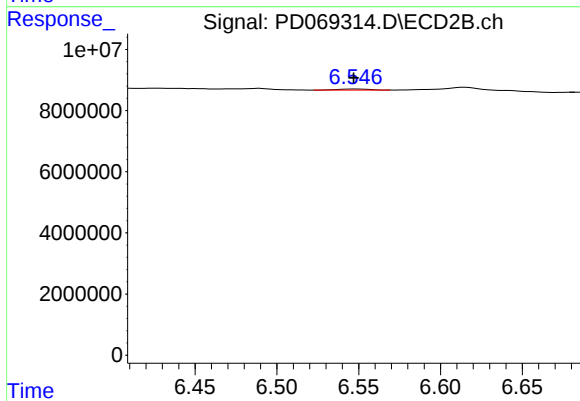

#12 4,4'-DDE


R.T.: 6.548 min
Delta R.T.: 0.001 min
Response: 447439
Conc: 0.04 ng/ml

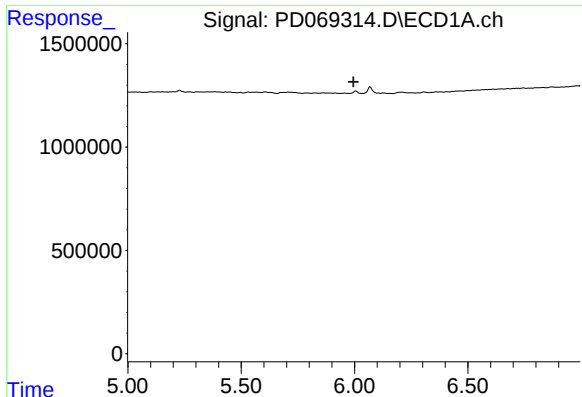

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

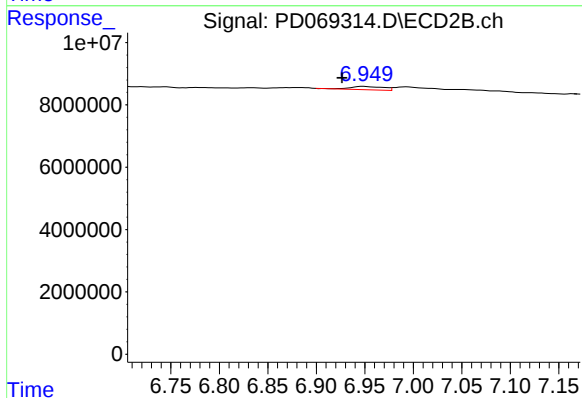


#14 Endrin

R.T.: 6.949 min
Delta R.T.: 0.022 min
Response: 2545047
Conc: 0.28 ng/ml

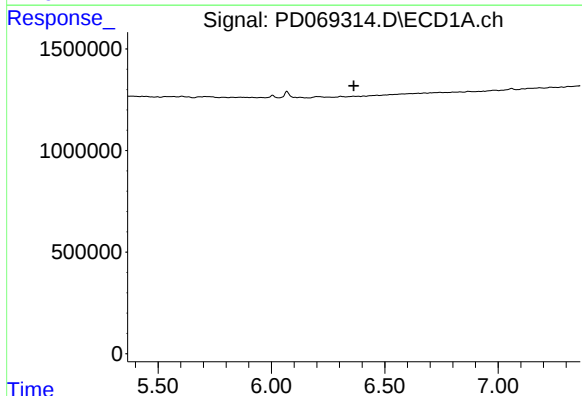


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

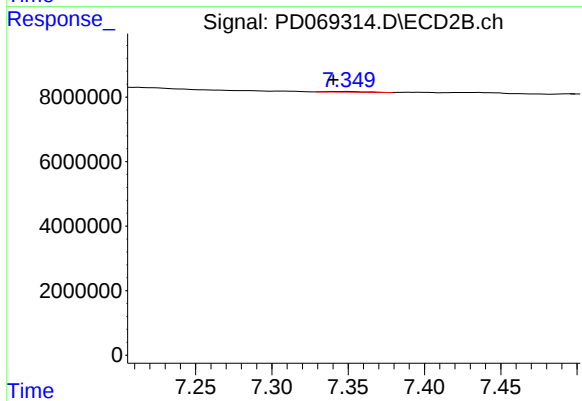

#17 4,4'-DDT


R.T.: 7.350 min
Delta R.T.: 0.010 min
Response: 316008
Conc: 0.04 ng/ml

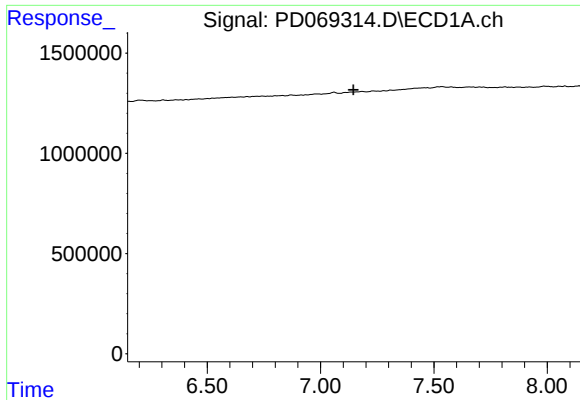

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

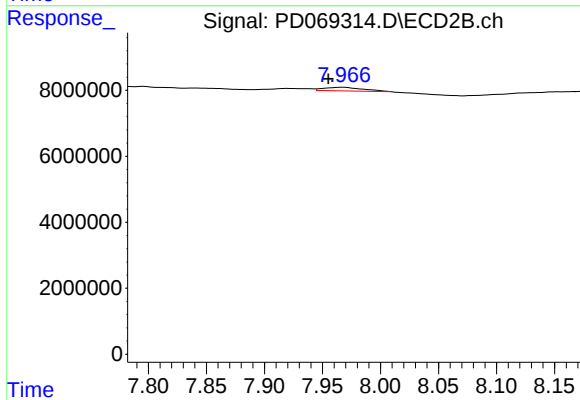


#21 Endrin ketone

R.T.: 7.968 min
Delta R.T.: 0.013 min
Response: 2498966
Conc: 0.28 ng/ml

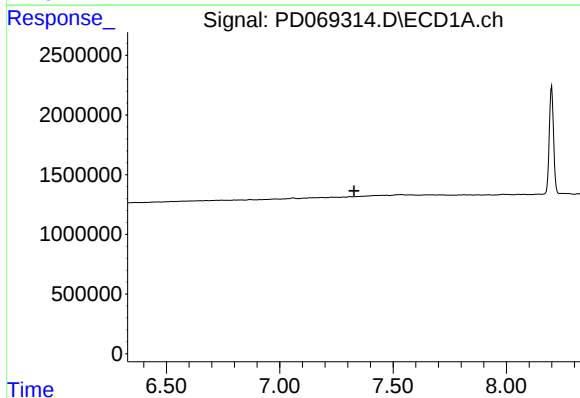


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.328 min
Response: 0
Conc: N.D.

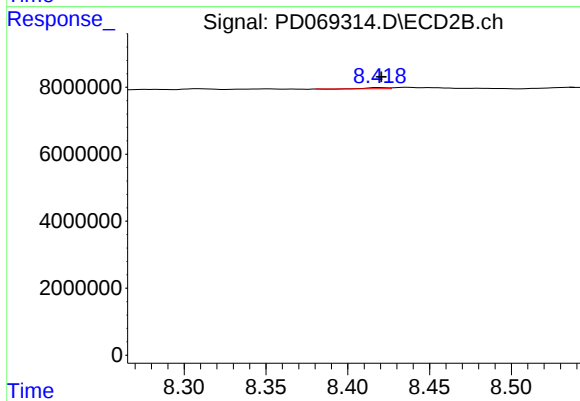

#22 Mirex


R.T.: 8.419 min
Delta R.T.: -0.001 min
Response: 287666
Conc: 0.04 ng/ml

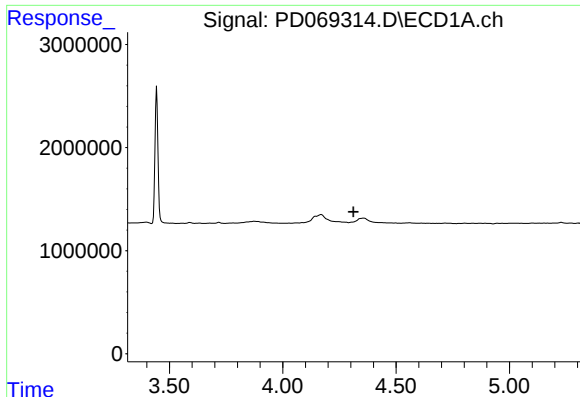

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.312 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

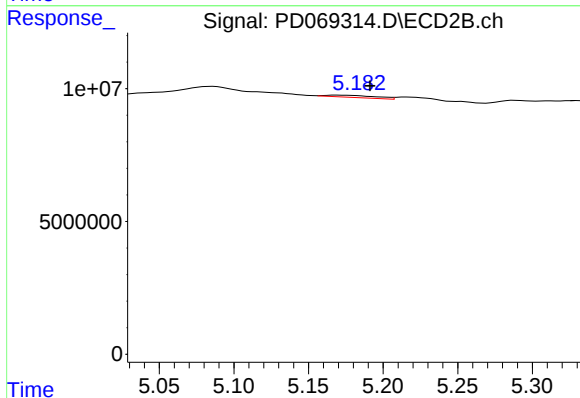


#23 Chlordane-1

R.T.: 5.169 min
Delta R.T.: -0.022 min
Response: 1857003
Conc: 3.87 ng/ml

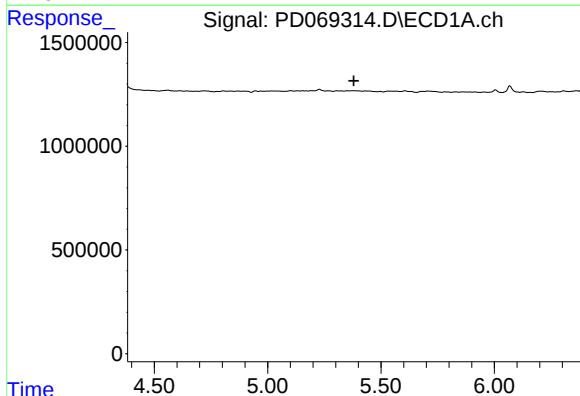


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.381 min
Response: 0
Conc: N.D.

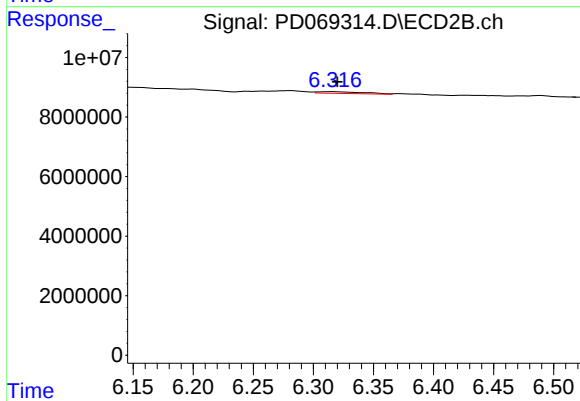

#25 Chlordane-3


R.T.: 6.317 min
Delta R.T.: -0.002 min
Response: 1548920
Conc: 0.95 ng/ml

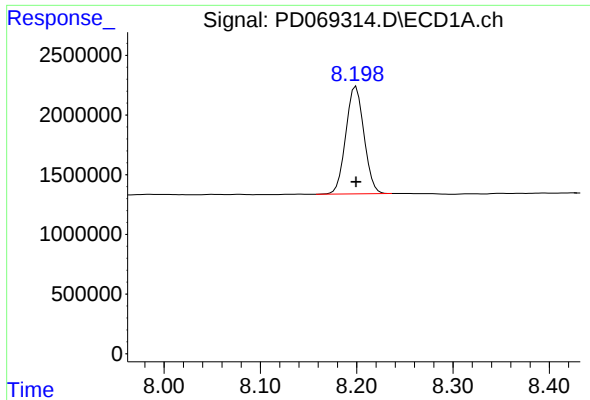

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 11767498
Conc: 9.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

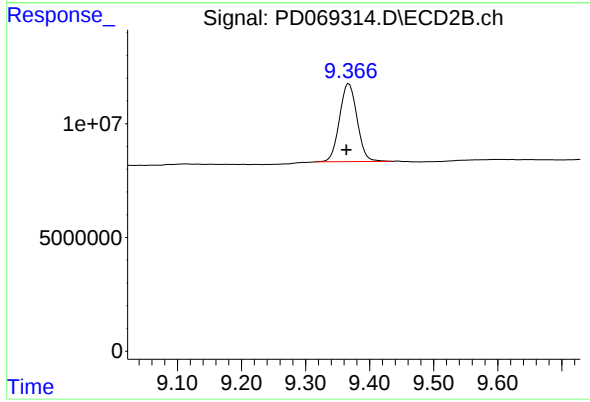

#28 Decachlorobiphenyl

R.T.: 9.368 min
Delta R.T.: 0.004 min
Response: 65148507
Conc: 9.96 ng/ml