

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042922\
 Data File : PD069304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2022 17:49
 Operator : AR\AJ
 Sample : N2605-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TR-04-042822

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 00:59:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:40:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	14787204	129.6E6	13.321	12.089
28)	SA Decachlor...	8.199	9.367	14541535	83580633	11.646	12.772
Target Compounds							
10)	B gamma-Chl...	5.384	6.321	1643639	35649183	1.182m	3.062m#
11)	B alpha-Chl...	5.439	6.399	4482806	103.2E6	3.260	9.024m#
12)	B 4,4'-DDE	5.605	6.549	663079	10546579	0.524	0.976 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042922\
Data File : PD069304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2022 17:49
Operator : AR\AJ
Sample : N2605-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TR-04-042822

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 00:59:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:40:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

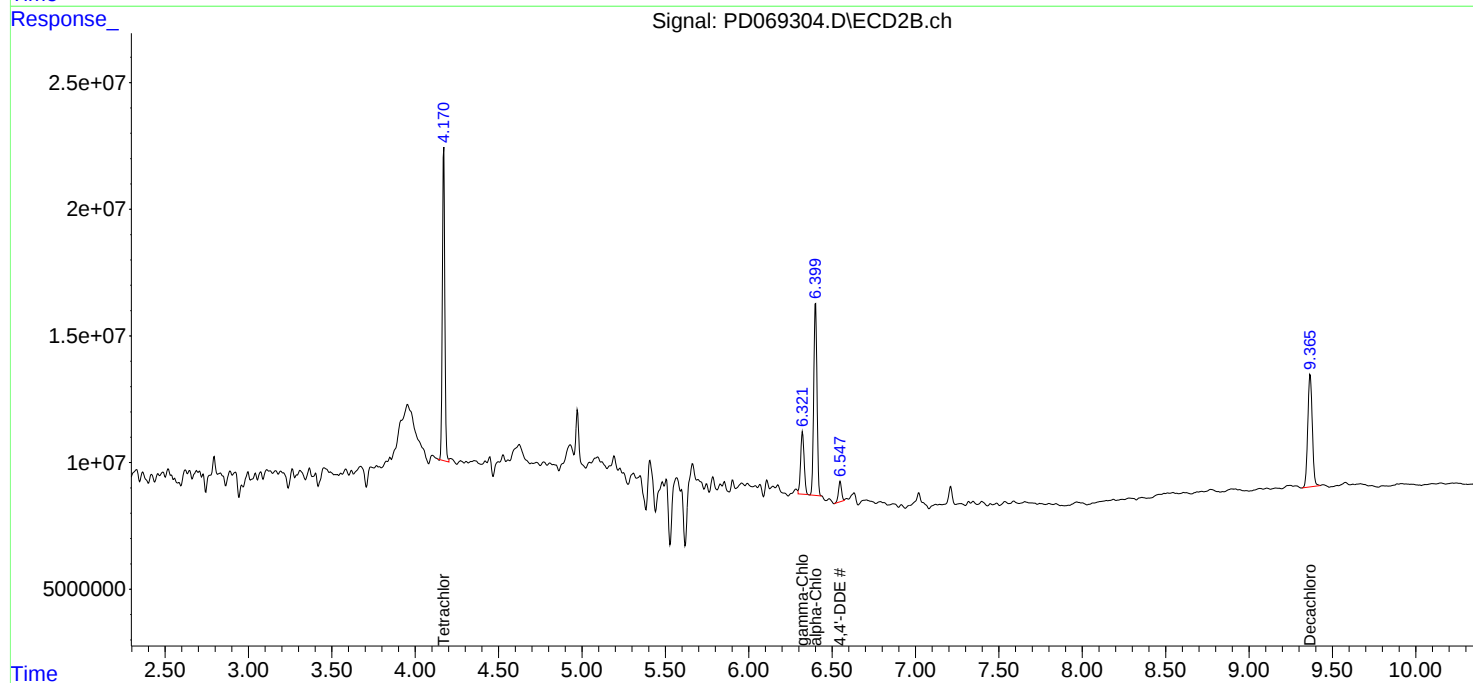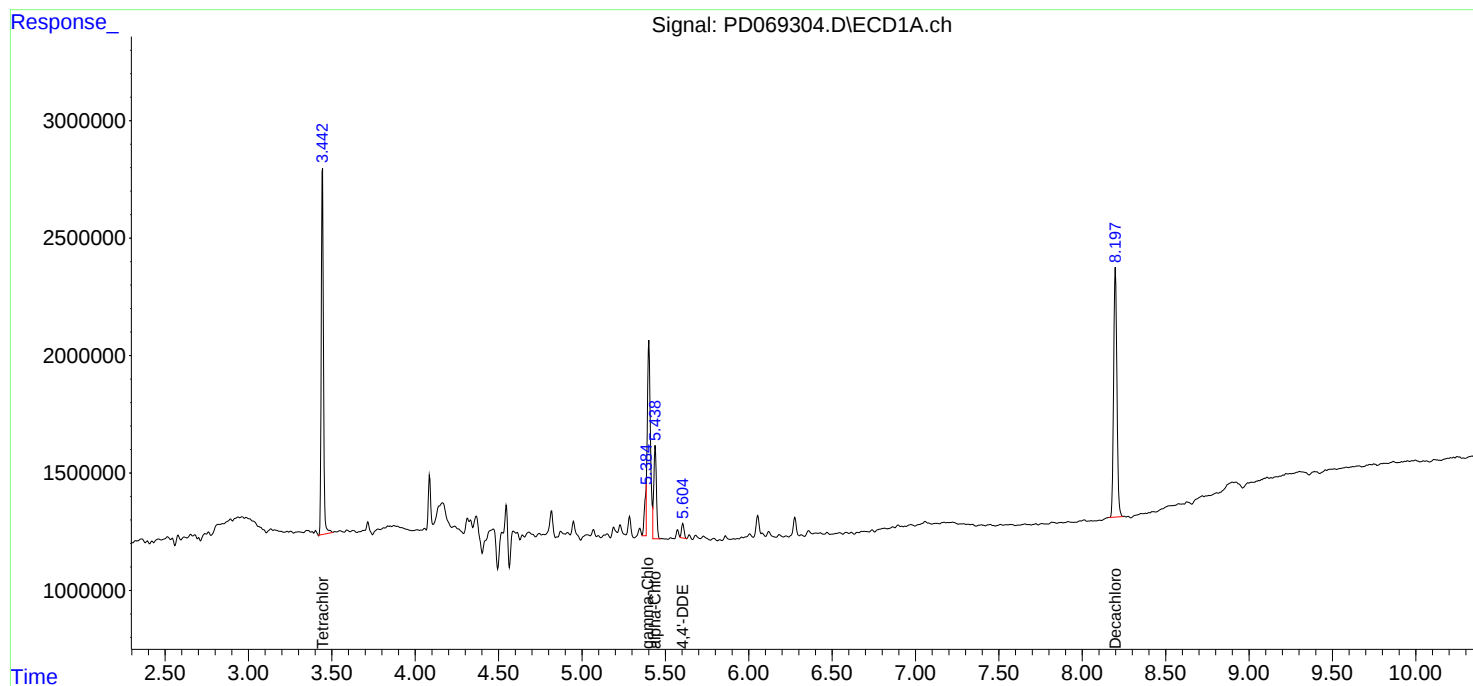


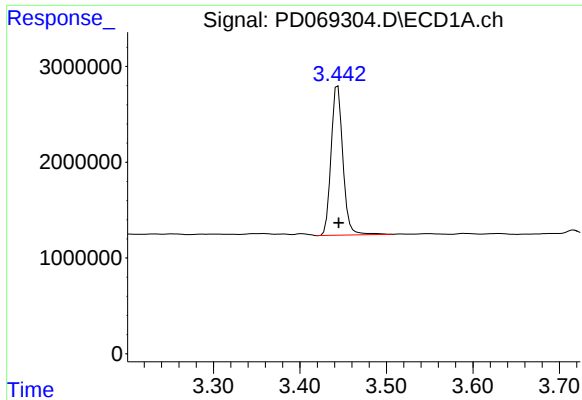

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 14787204
Conc: 13.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-04-042822

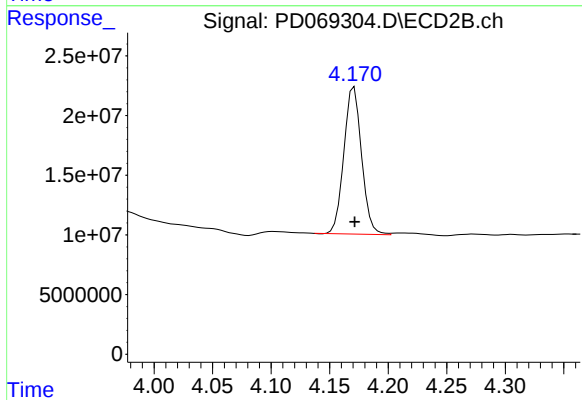


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 129615750
Conc: 12.09 ng/ml

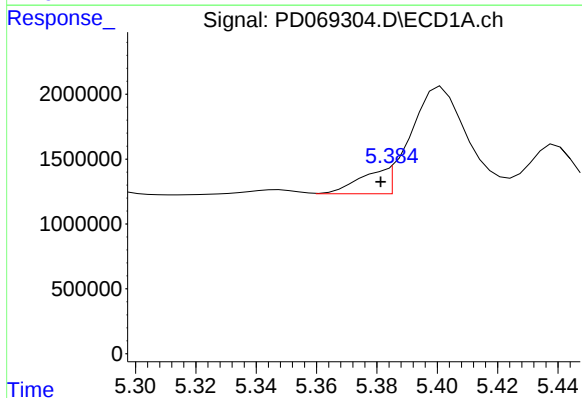


#10 gamma-Chlordane

R.T.: 5.384 min
Delta R.T.: 0.003 min
Response: 1643639
Conc: 1.18 ng/ml m

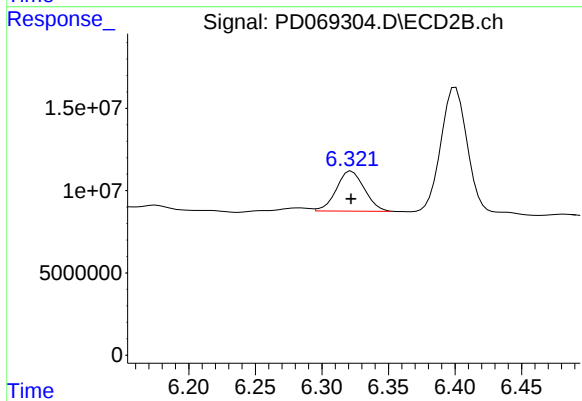

#10 gamma-Chlordane


R.T.: 6.321 min
Delta R.T.: -0.001 min
Response: 35649183
Conc: 3.06 ng/ml m

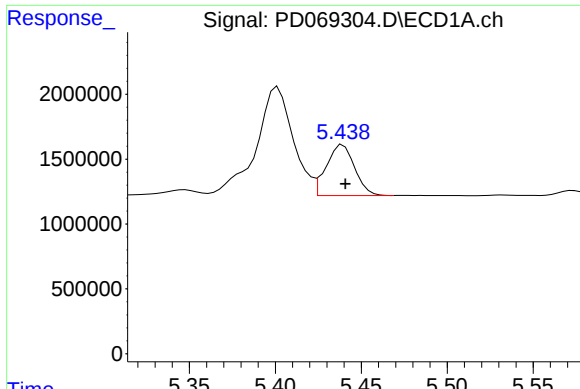

#11 alpha-Chlordane


R.T.: 5.439 min
Delta R.T.: -0.001 min
Response: 4482806
Conc: 3.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-04-042822

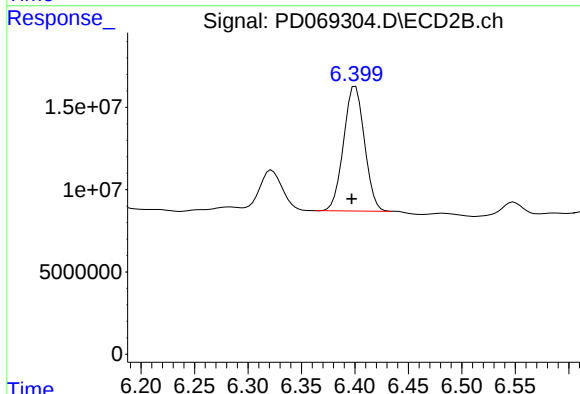


#11 alpha-Chlordane

R.T.: 6.399 min
Delta R.T.: 0.002 min
Response: 103209327
Conc: 9.02 ng/ml m

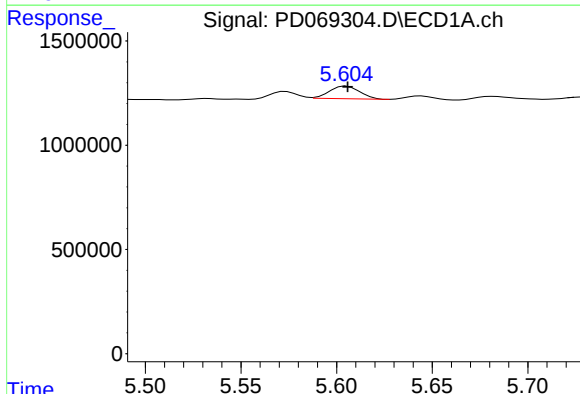


#12 4,4'-DDE

R.T.: 5.605 min
Delta R.T.: 0.000 min
Response: 663079
Conc: 0.52 ng/ml

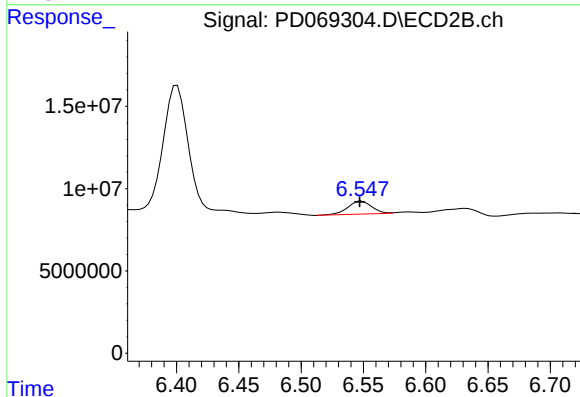

#12 4,4'-DDE


R.T.: 6.549 min
Delta R.T.: 0.002 min
Response: 10546579
Conc: 0.98 ng/ml

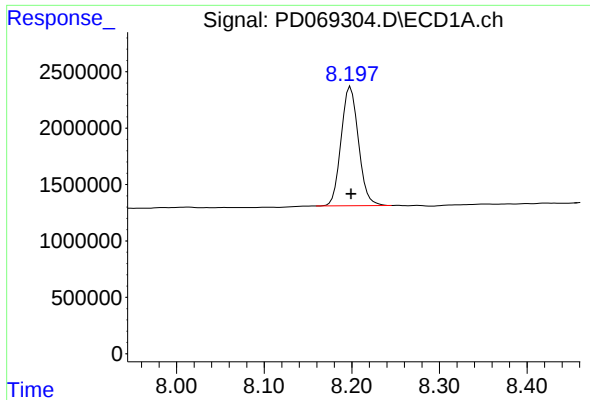

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 14541535
Conc: 11.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-04-042822

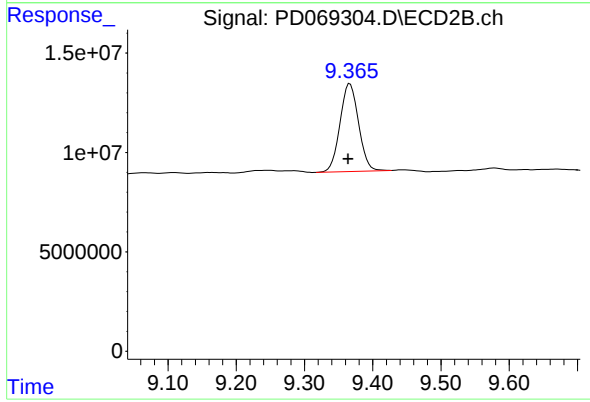

#28 Decachlorobiphenyl

R.T.: 9.367 min
Delta R.T.: 0.003 min
Response: 83580633
Conc: 12.77 ng/ml