

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
 Data File : PD082644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 11:11
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:46:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 29 14:45:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	29527156	71673142	19.396	18.771
28)	SA Decachlor...	9.121	7.907	37983251	72316420	19.450	18.921
Target Compounds							
9)	A Endosulfan I	6.108	5.094	18531857	37762372	8.720	8.328
10)	B gamma-Chl...	5.977	4.974	20459307	44390306	9.135	8.969
12)	B 4,4'-DDE	6.228	5.227	40024260	84460040	18.747	18.347
13)	MA Dieldrin	6.383	5.359	39558067	88408551	18.128	17.781
19)	B Endosulfa...	7.199	6.328	31006889	72387252	18.124	18.334
20)	A Methoxychlor	7.539	6.606	80757900	183.4E6	91.300	88.532
21)	B Endrin ke...	7.686	6.834	34259960	82056310	18.463	18.125



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
Data File : PD082644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 11:11
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:46:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 14:45:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

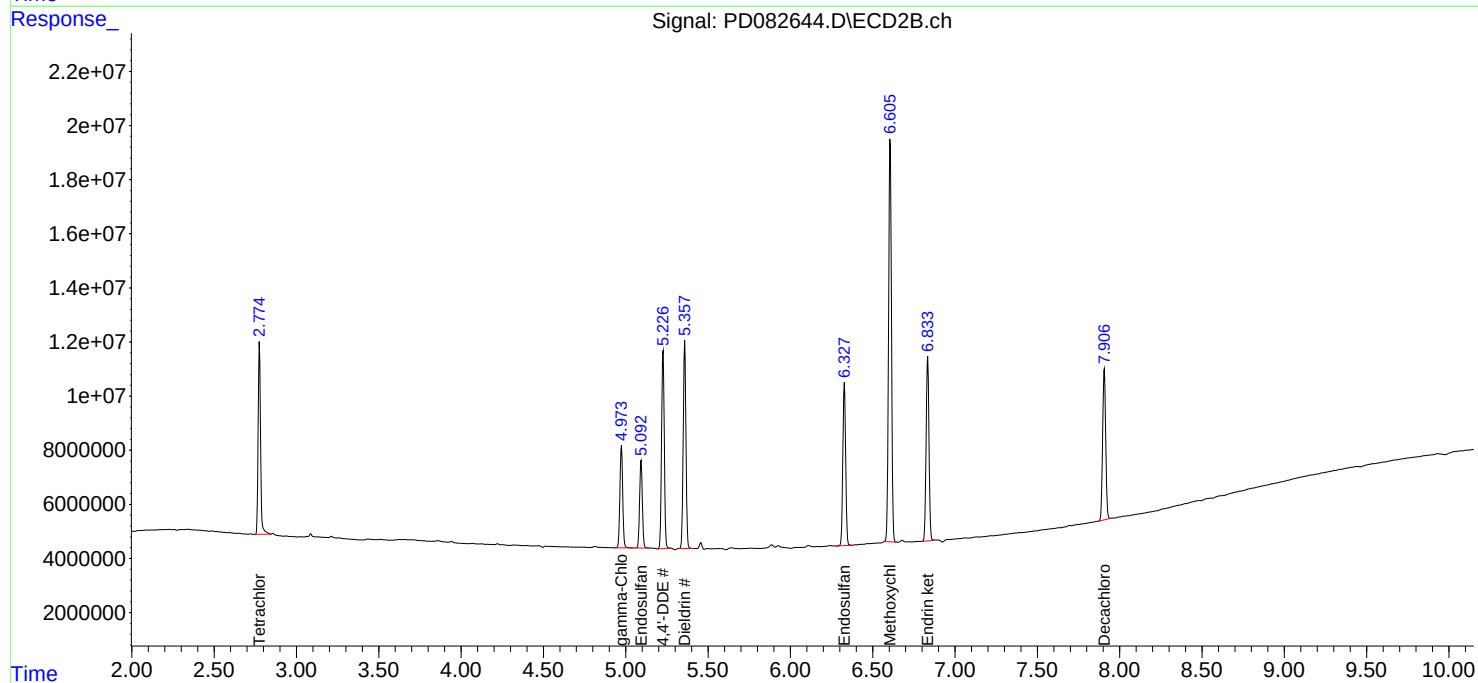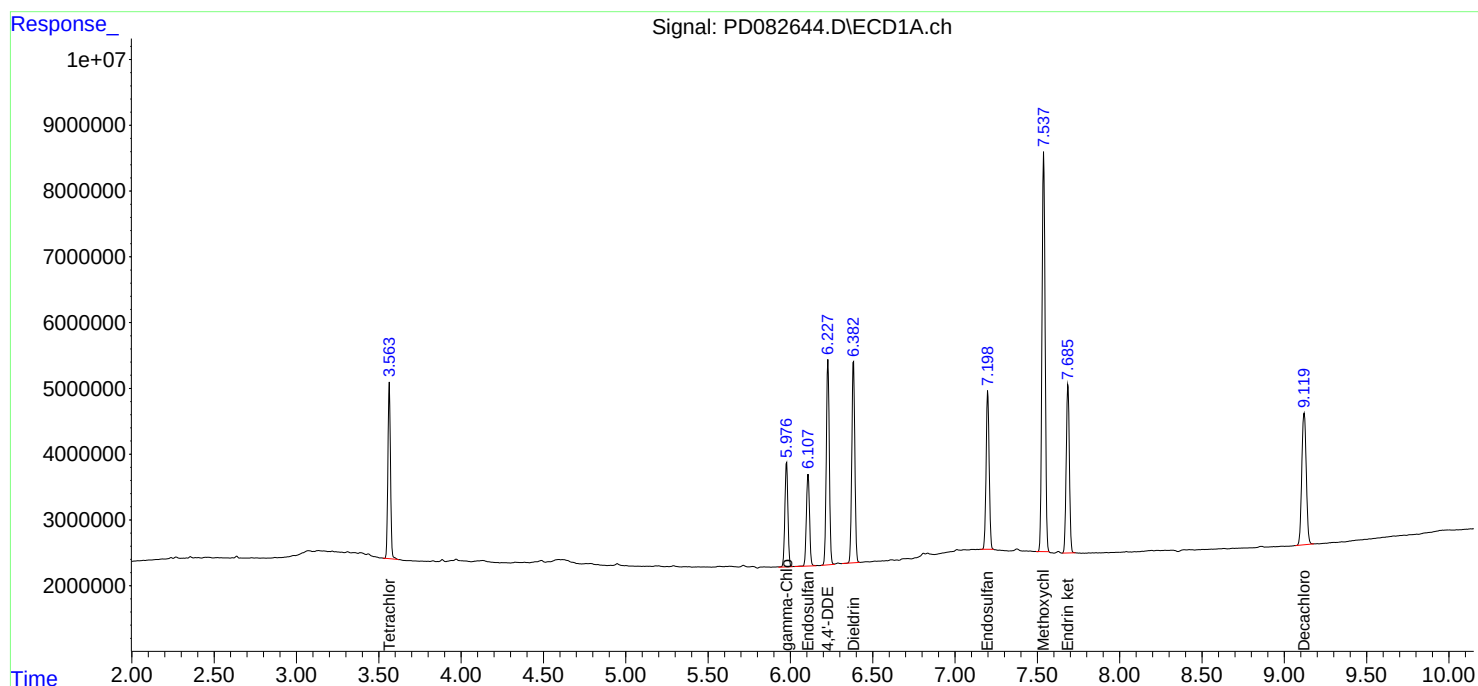


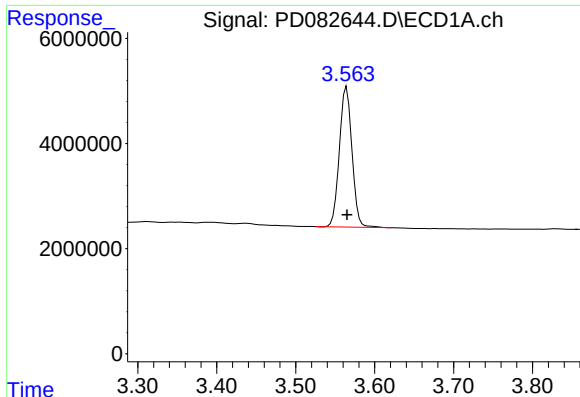

#1 Tetrachloro-m-xylene


R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 29527156
Conc: 19.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

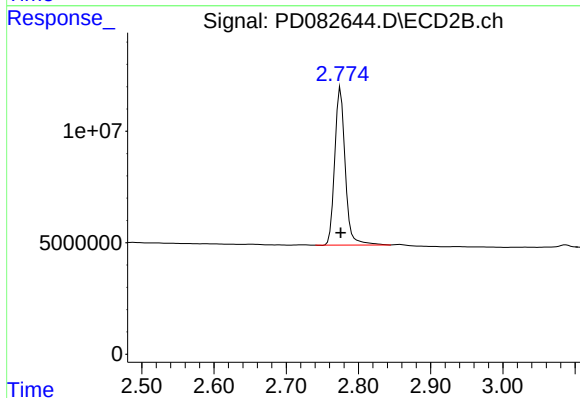


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 71673142
Conc: 18.77 ng/ml

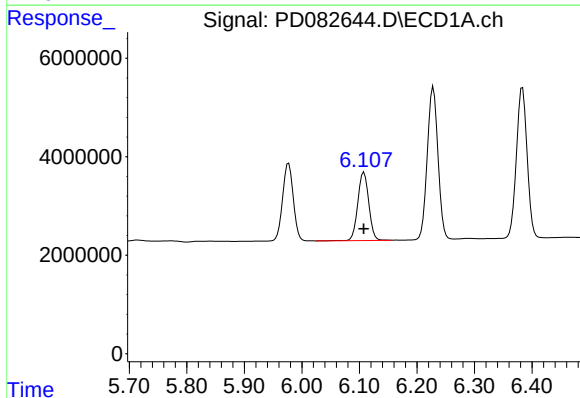


#9 Endosulfan I

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 18531857
Conc: 8.72 ng/ml

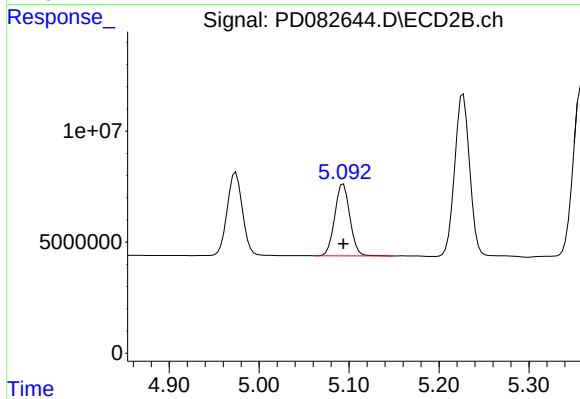

#9 Endosulfan I


R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 37762372
Conc: 8.33 ng/ml

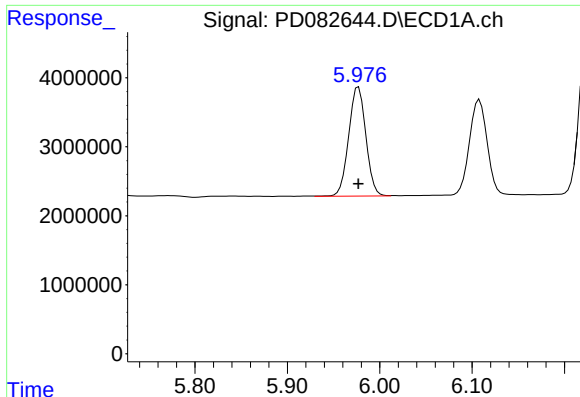

#10 gamma-Chlordane


R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 20459307
Conc: 9.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

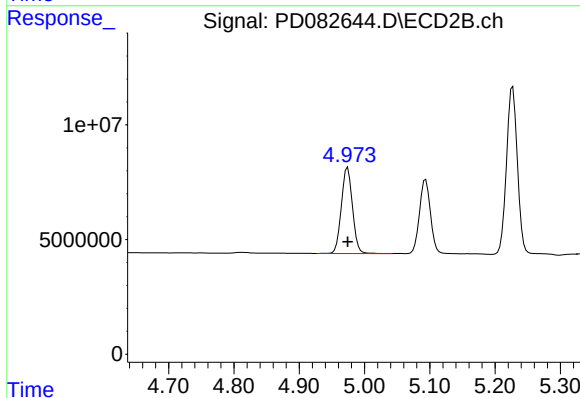


#10 gamma-Chlordane

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 44390306
Conc: 8.97 ng/ml

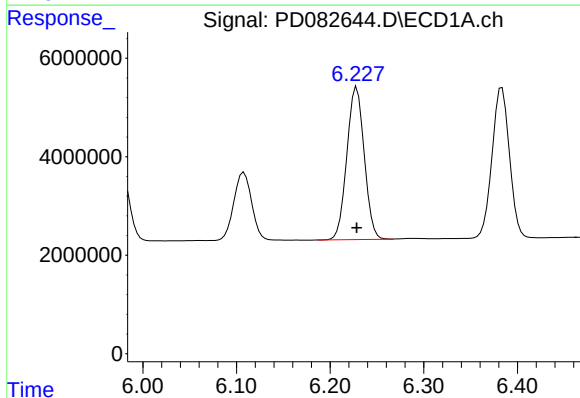


#12 4,4'-DDE

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 40024260
Conc: 18.75 ng/ml

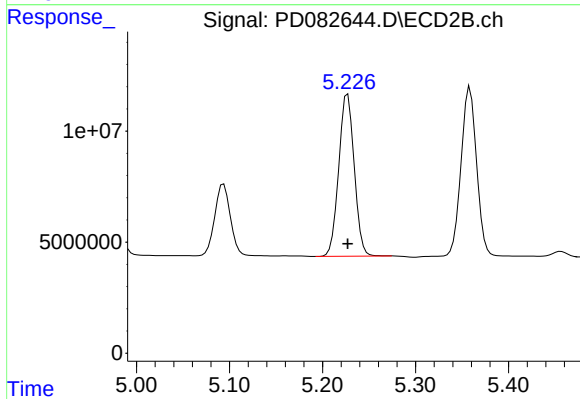

#12 4,4'-DDE


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 84460040
Conc: 18.35 ng/ml

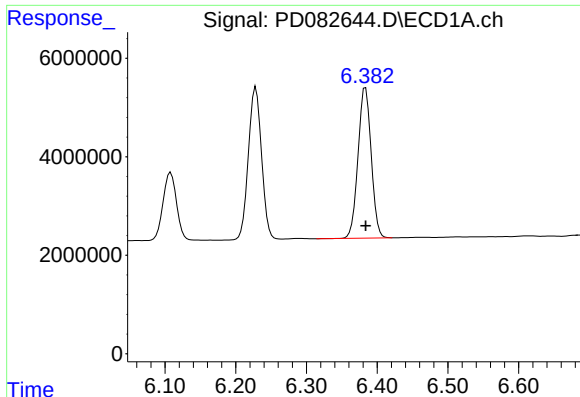

#13 Dieldrin


R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 39558067
Conc: 18.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

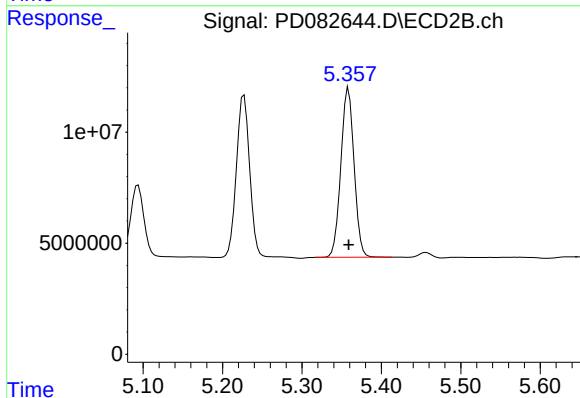


#13 Dieldrin

R.T.: 5.359 min
Delta R.T.: 0.000 min
Response: 88408551
Conc: 17.78 ng/ml

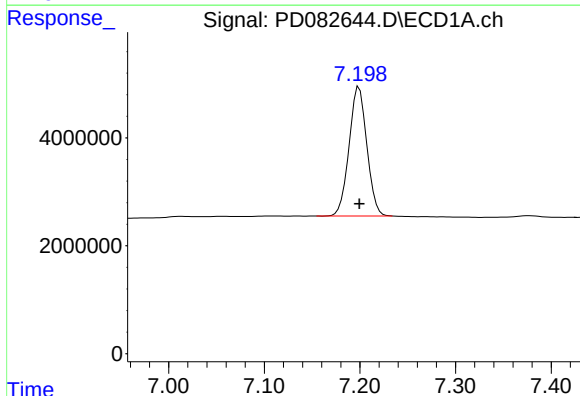


#19 Endosulfan Sulfate

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 31006889
Conc: 18.12 ng/ml

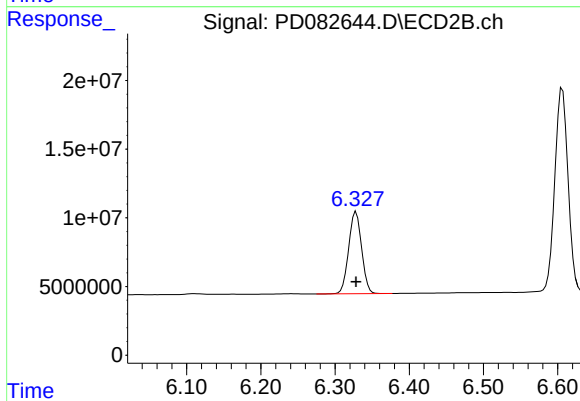

#19 Endosulfan Sulfate


R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 72387252
Conc: 18.33 ng/ml

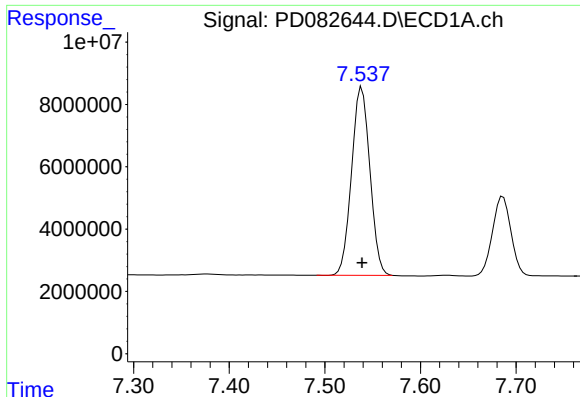

#20 Methoxychlor


R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 80757900
Conc: 91.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

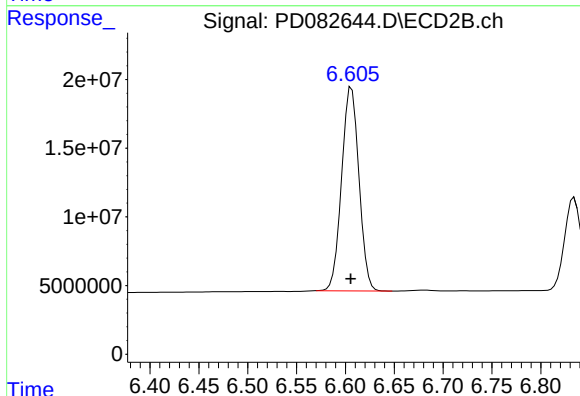


#20 Methoxychlor

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 183396399
Conc: 88.53 ng/ml

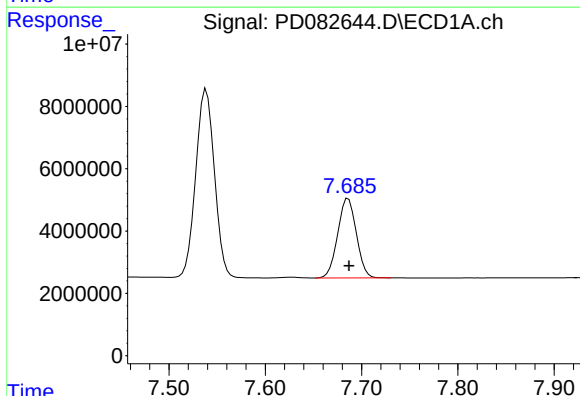


#21 Endrin ketone

R.T.: 7.686 min
Delta R.T.: 0.000 min
Response: 34259960
Conc: 18.46 ng/ml

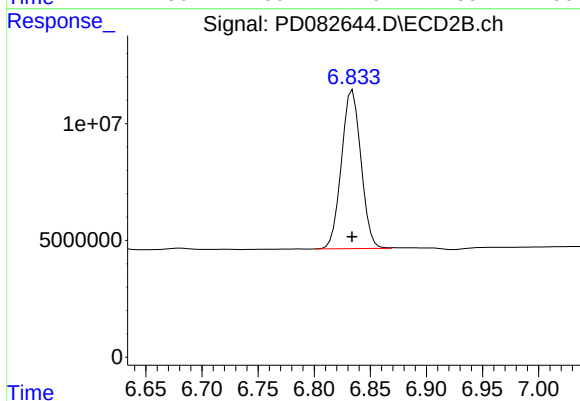

#21 Endrin ketone


R.T.: 6.834 min
Delta R.T.: 0.000 min
Response: 82056310
Conc: 18.13 ng/ml

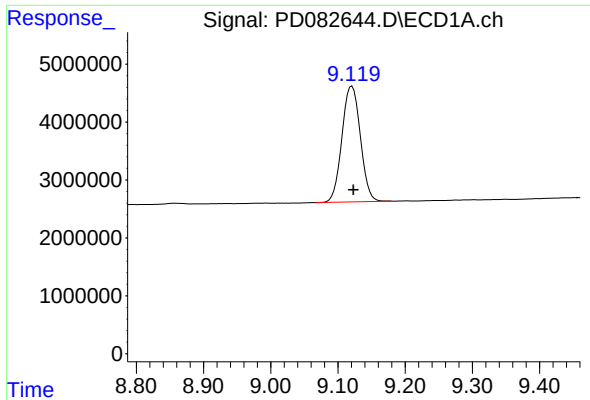

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.002 min
Response: 37983251
Conc: 19.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

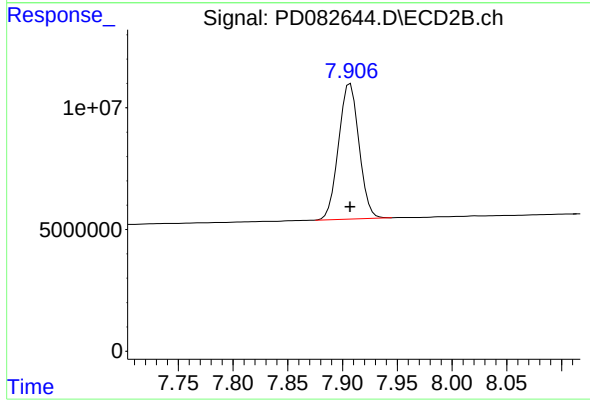

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 72316420
Conc: 18.92 ng/ml