

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
 Data File : PD082650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 12:31
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:04:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 29 14:02:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	154.3E6	461.1E6	99.165	99.188
28)	SA Decachlor...	9.120	7.906	190.0E6	377.1E6	98.894	97.694
Target Compounds							
23)	Chlordane-1	4.732	3.770	81739865	156.0E6	996.378	993.945
24)	Chlordane-2	5.263	4.345	81344543	173.2E6	983.708	982.542
25)	Chlordane-3	5.976	4.974	345.2E6	523.0E6	1019.541	1002.175
26)	Chlordane-4	6.059	5.037	402.9E6	480.2E6	1010.590	978.919
27)	Chlordane-5	6.911	5.932	70522119	178.3E6	1017.307	1000.141



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
Data File : PD082650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 12:31
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:04:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 14:02:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

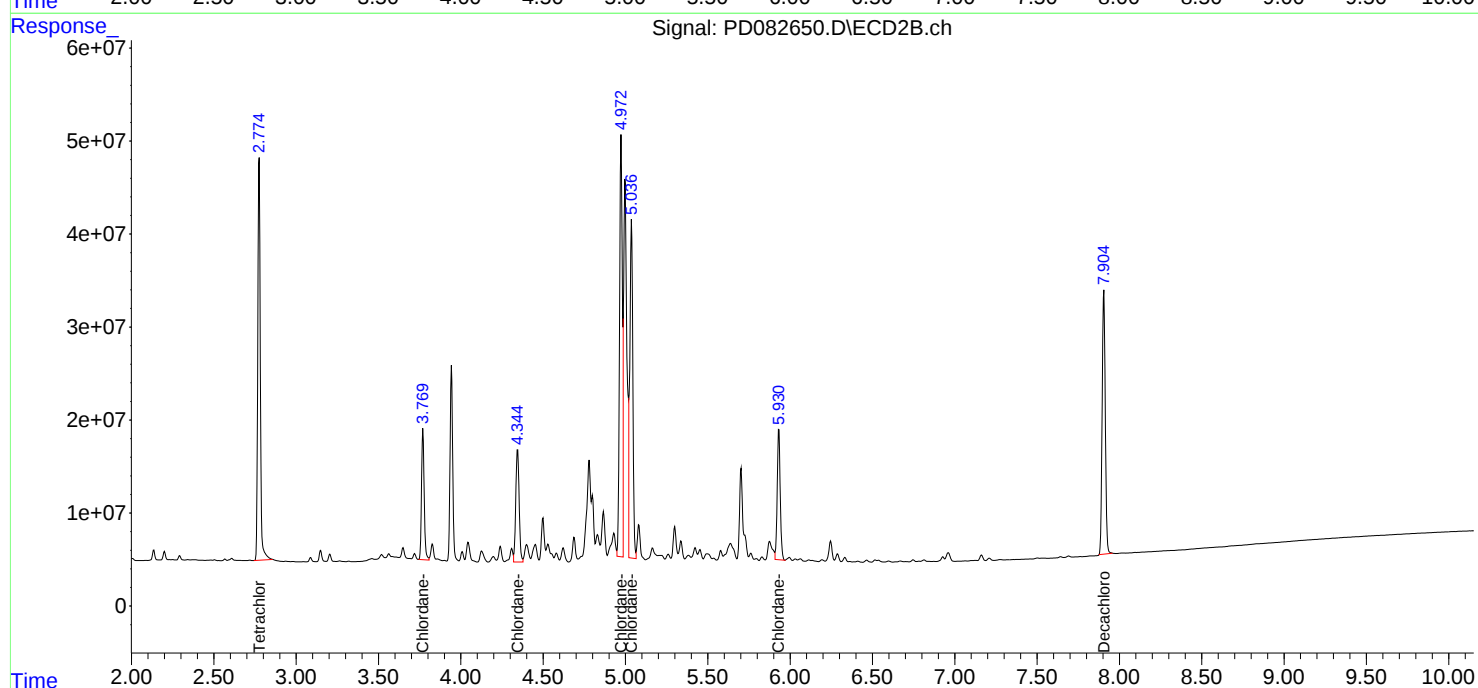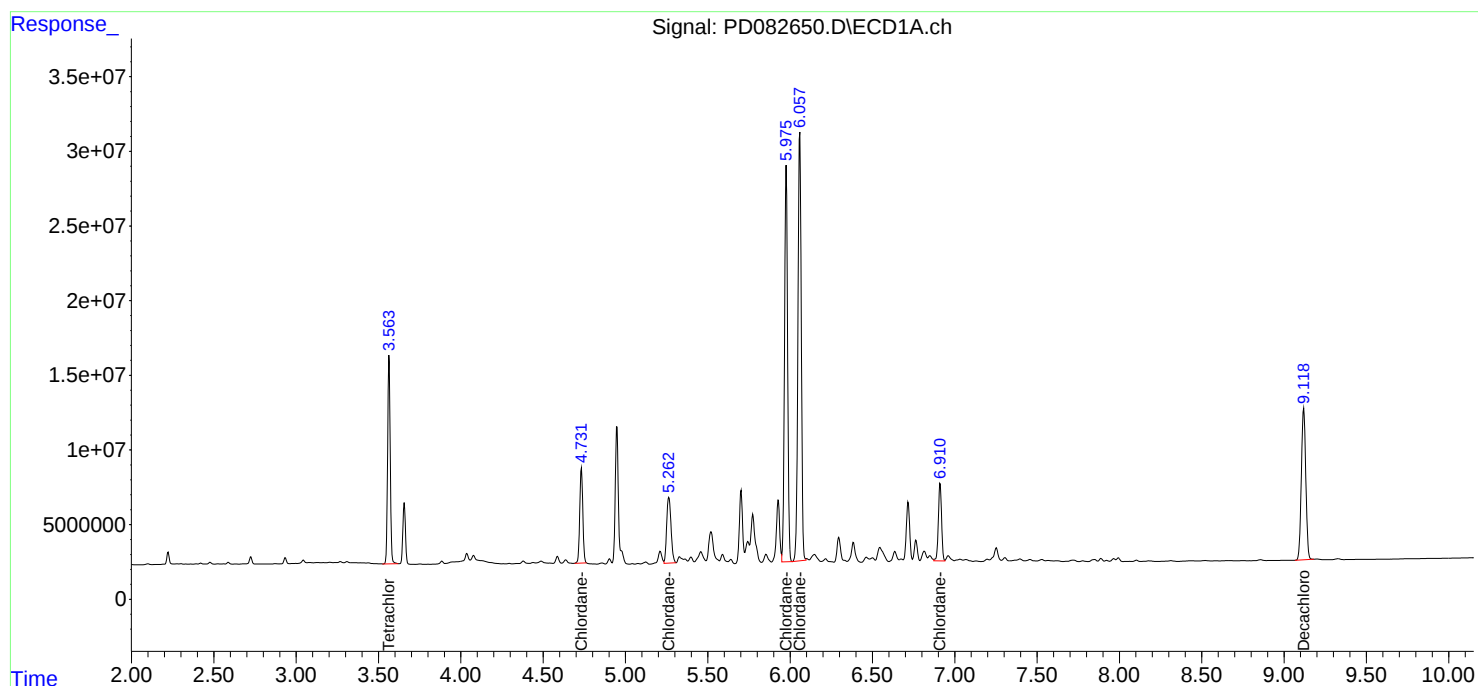


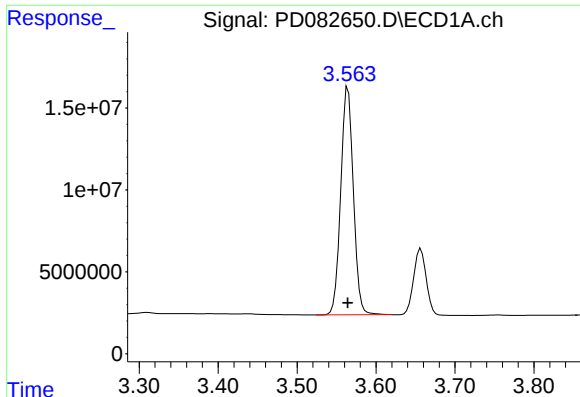

#1 Tetrachloro-m-xylene


R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 154289238
Conc: 99.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

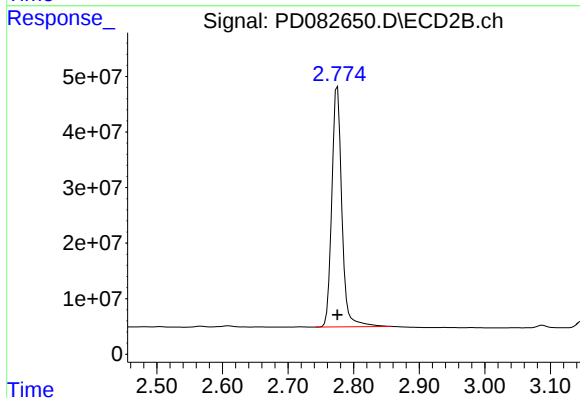


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 461140408
Conc: 99.19 ng/ml

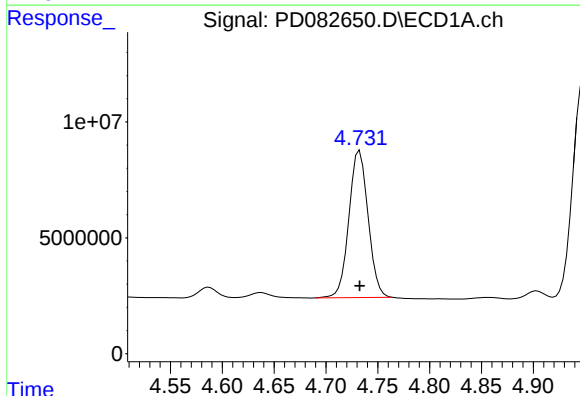


#23 Chlordane-1

R.T.: 4.732 min
Delta R.T.: 0.000 min
Response: 81739865
Conc: 996.38 ng/ml

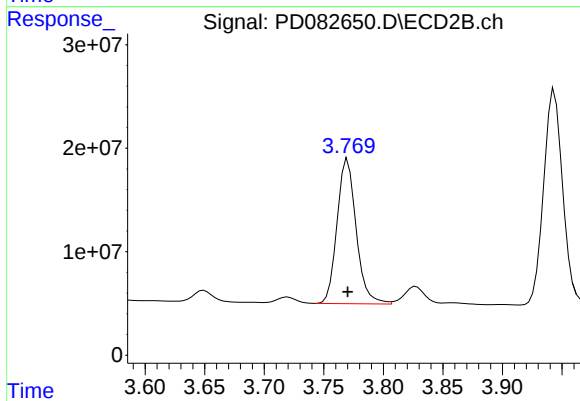

#23 Chlordane-1


R.T.: 3.770 min
Delta R.T.: 0.000 min
Response: 156016635
Conc: 993.95 ng/ml

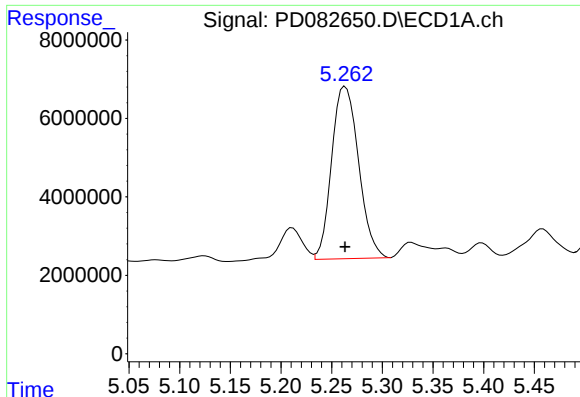

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 81344543
Conc: 983.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

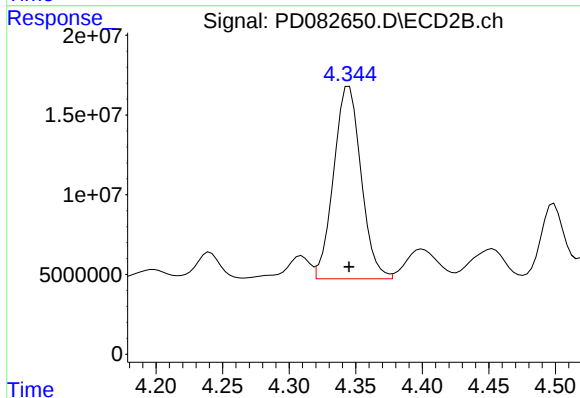


#24 Chlordane-2

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 173218990
Conc: 982.54 ng/ml

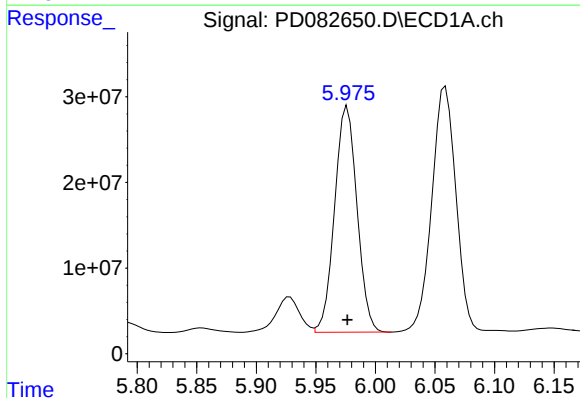


#25 Chlordane-3

R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 345208322
Conc: 1019.54 ng/ml

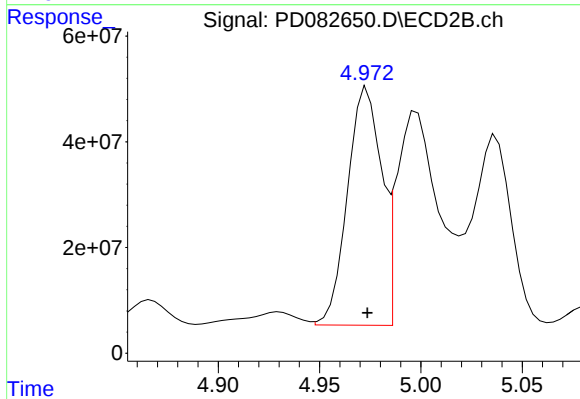

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 523039522
Conc: 1002.18 ng/ml

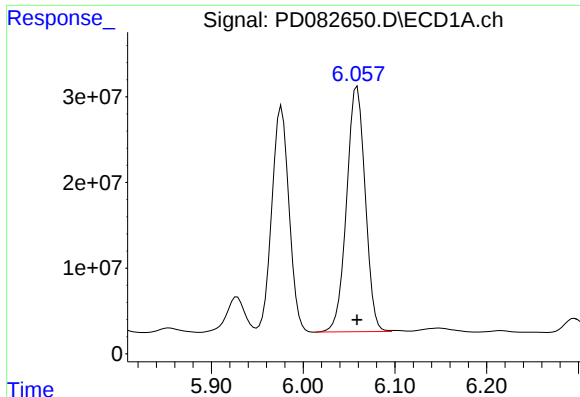

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 402903509
Conc: 1010.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

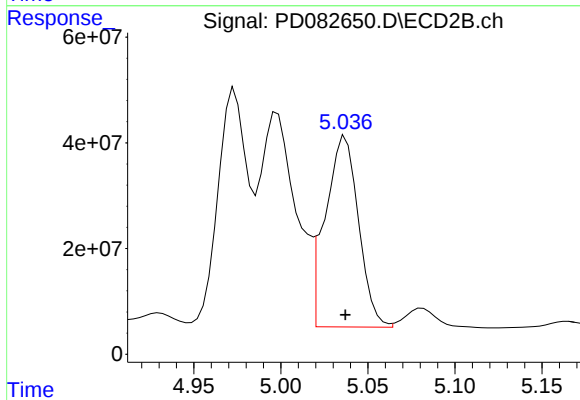


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 480181222
Conc: 978.92 ng/ml

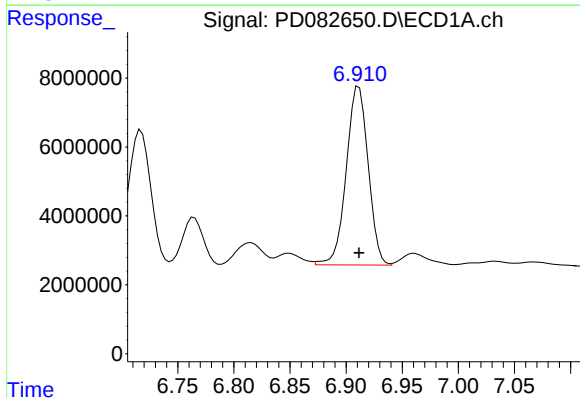


#27 Chlordane-5

R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 70522119
Conc: 1017.31 ng/ml

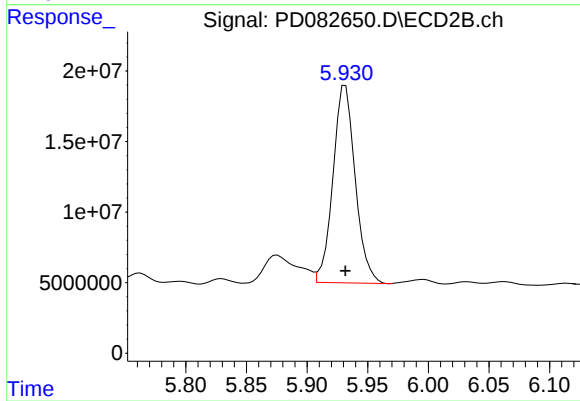

#27 Chlordane-5


R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 178330274
Conc: 1000.14 ng/ml

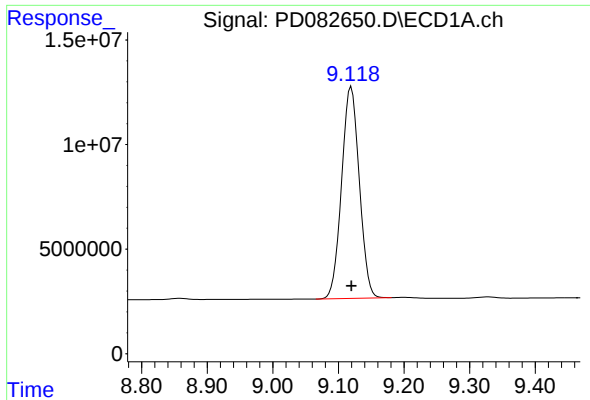

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 189957470
Conc: 98.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

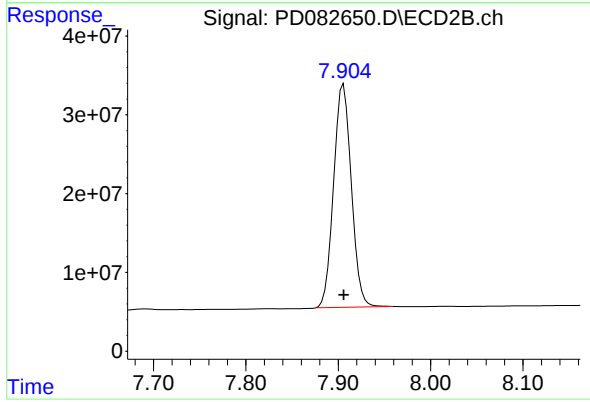

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 377118933
Conc: 97.69 ng/ml