

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
 Data File : PD082653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 13:11
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:08:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 29 14:02:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	39147089	116.3E6	25.417	25.337
28)	SA Decachlor...	9.120	7.906	50277771	100.0E6	26.234	26.014
Target Compounds							
23)	Chlordane-1	4.733	3.770	20527441	40192926	252.955	257.175
24)	Chlordane-2	5.264	4.345	21905892	46059621	263.279	261.382
25)	Chlordane-3	5.977	4.974	84230528	127.6E6	250.494	248.371
26)	Chlordane-4	6.059	5.037	101.5E6	121.4E6	254.879	250.262
27)	Chlordane-5	6.912	5.931	16821738	43972941	247.162	250.378


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
Data File : PD082653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 13:11
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:08:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 14:02:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

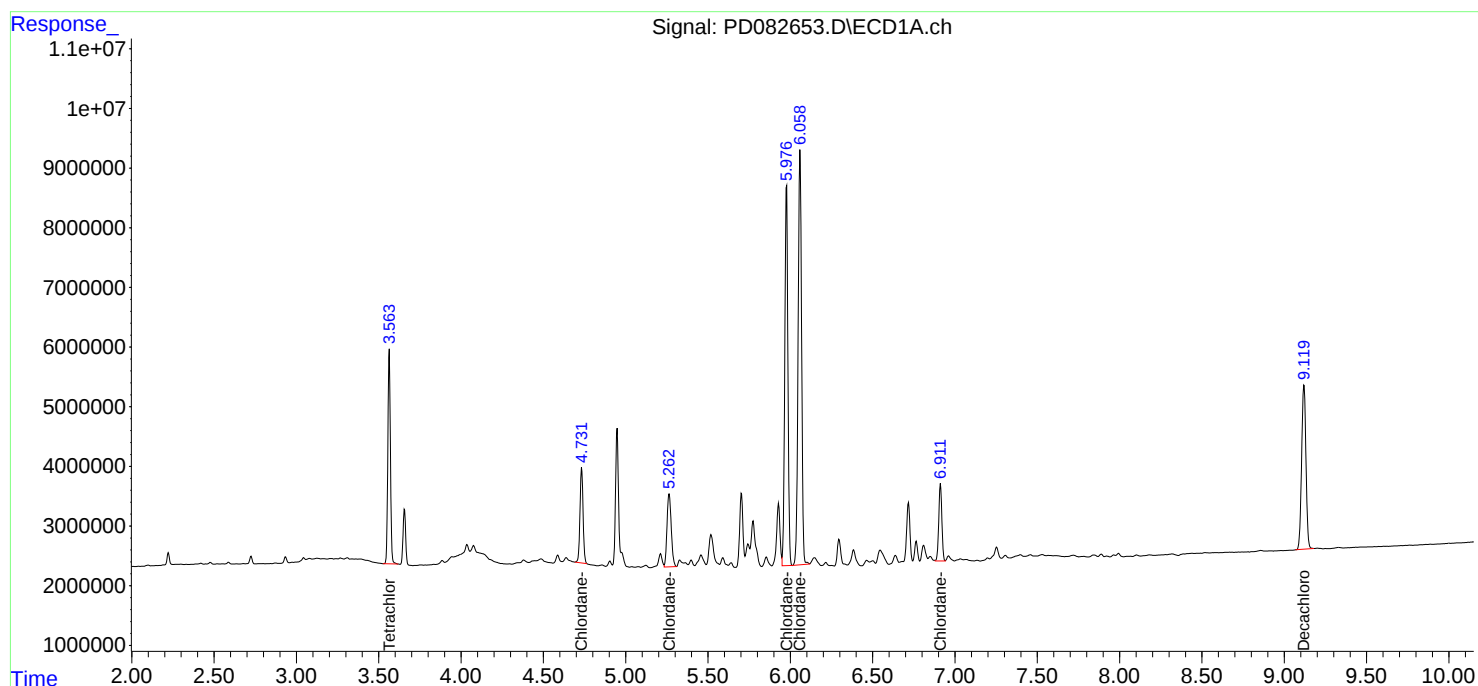


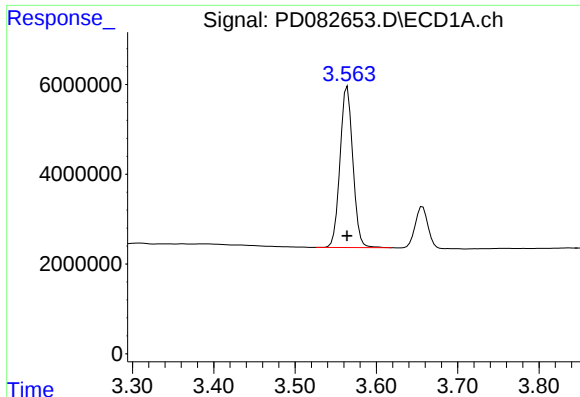

#1 Tetrachloro-m-xylene


R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 39147089
Conc: 25.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

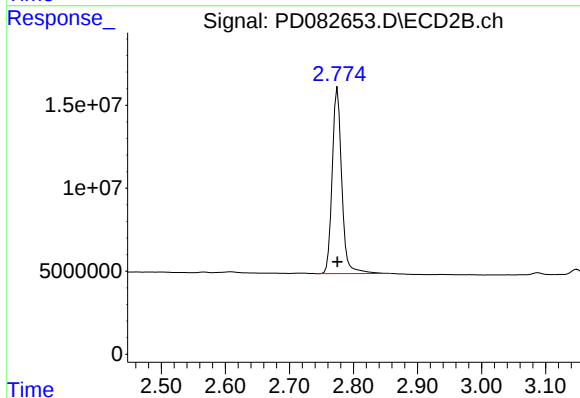


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 116278559
Conc: 25.34 ng/ml

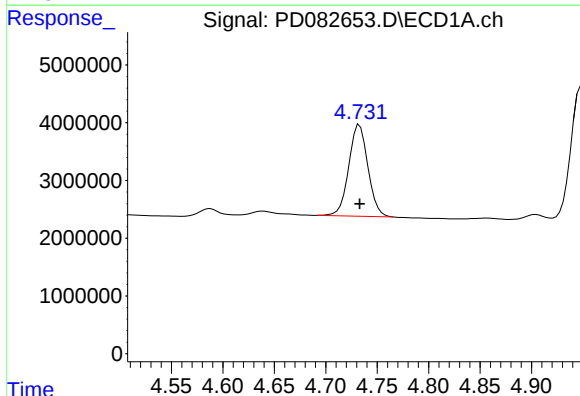


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 20527441
Conc: 252.95 ng/ml

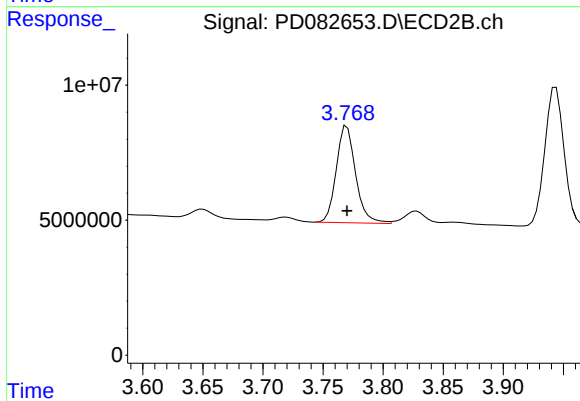

#23 Chlordane-1


R.T.: 3.770 min
Delta R.T.: 0.000 min
Response: 40192926
Conc: 257.17 ng/ml

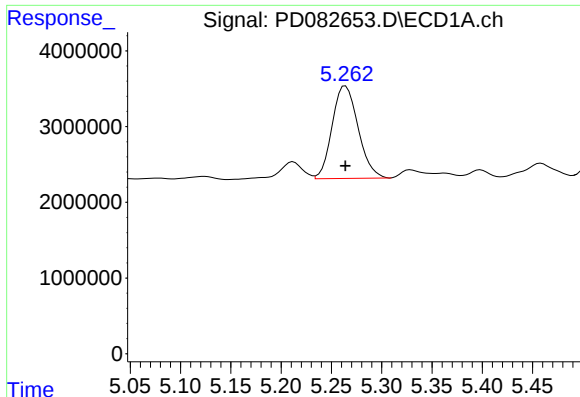

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 21905892
Conc: 263.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

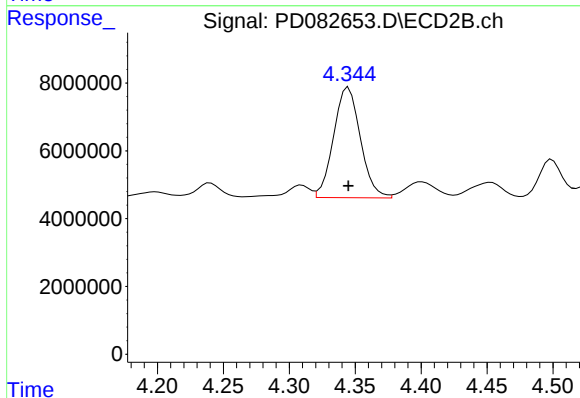


#24 Chlordane-2

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 46059621
Conc: 261.38 ng/ml

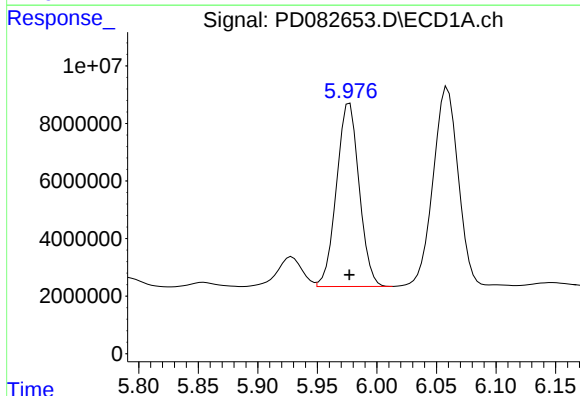


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 84230528
Conc: 250.49 ng/ml

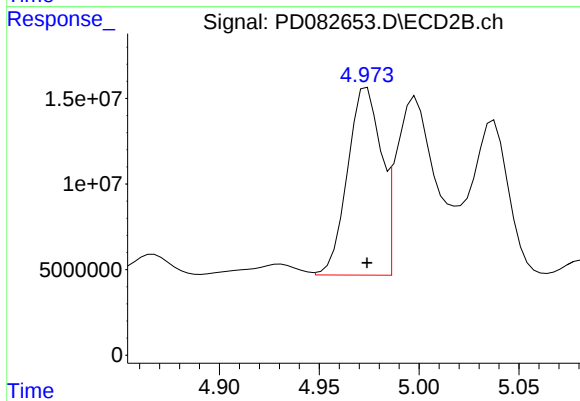

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 127588492
Conc: 248.37 ng/ml

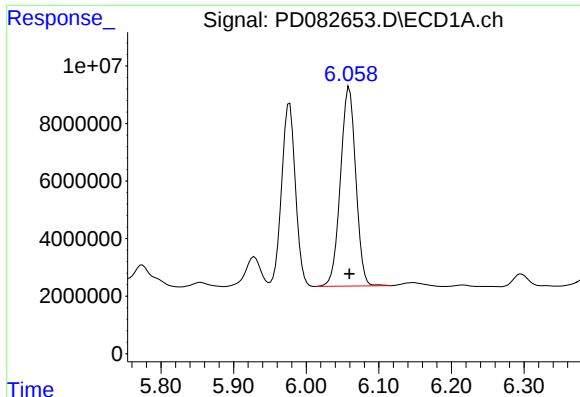

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 101461744
Conc: 254.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

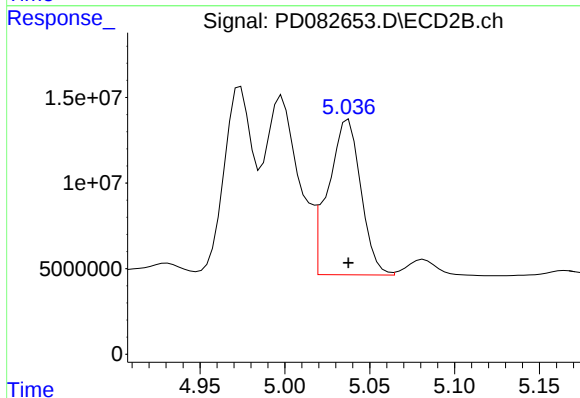


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 121407909
Conc: 250.26 ng/ml

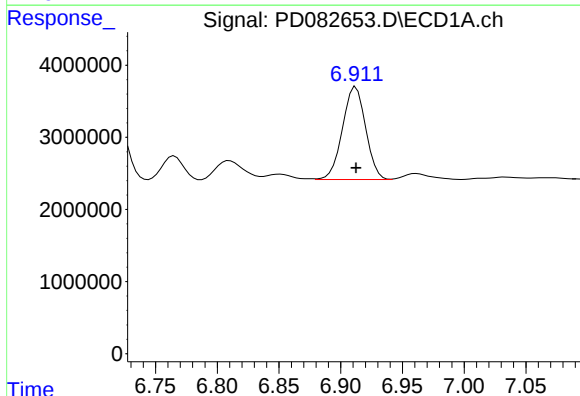


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 16821738
Conc: 247.16 ng/ml

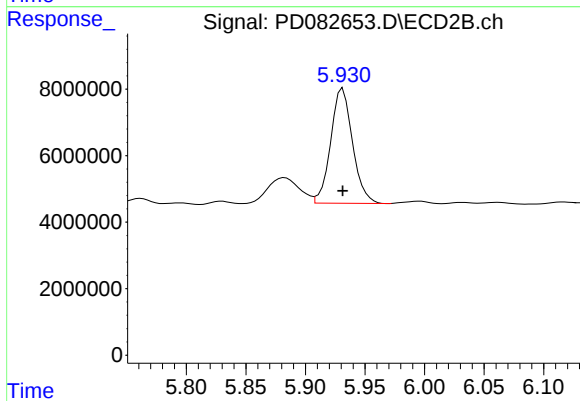

#27 Chlordane-5


R.T.: 5.931 min
Delta R.T.: 0.000 min
Response: 43972941
Conc: 250.38 ng/ml

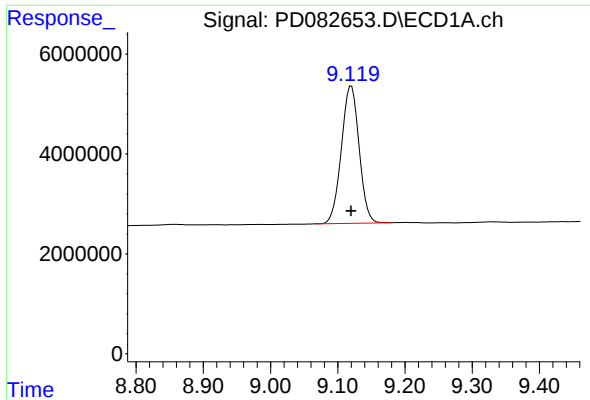

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 50277771
Conc: 26.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

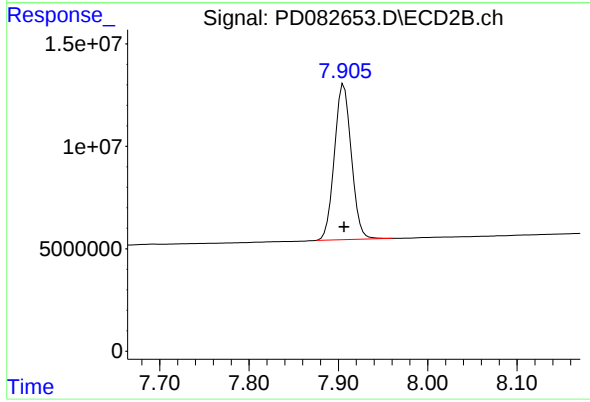

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 100042798
Conc: 26.01 ng/ml