

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
 Data File : PD062628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 14:33
 Operator : AR\AJ
 Sample : M2177-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG576

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:13:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 23:17:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.973	10589340	124.0E6	11.061	10.214
27)	SA Decachlor...	8.202	9.035	22151017	198.5E6	20.637	18.183
Target Compounds							
10)	B trans-Chl...	5.381	6.085	1135445	72121937	0.906m	4.404m#
11)	B cis-Chlor...	5.439	6.154	900164	15232734	0.733	0.981 #
12)	B 4,4'-DDE	5.603	6.310	611941	16011178	0.494	1.022 #
15)	B Endosulfa...	6.280	6.901	987545	14180513	0.952	1.133m
16)	A 4,4'-DDD	6.120	6.799	504900	12235038	0.507m	0.984m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
Data File : PD062628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 14:33
Operator : AR\AJ
Sample : M2177-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 23:17:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

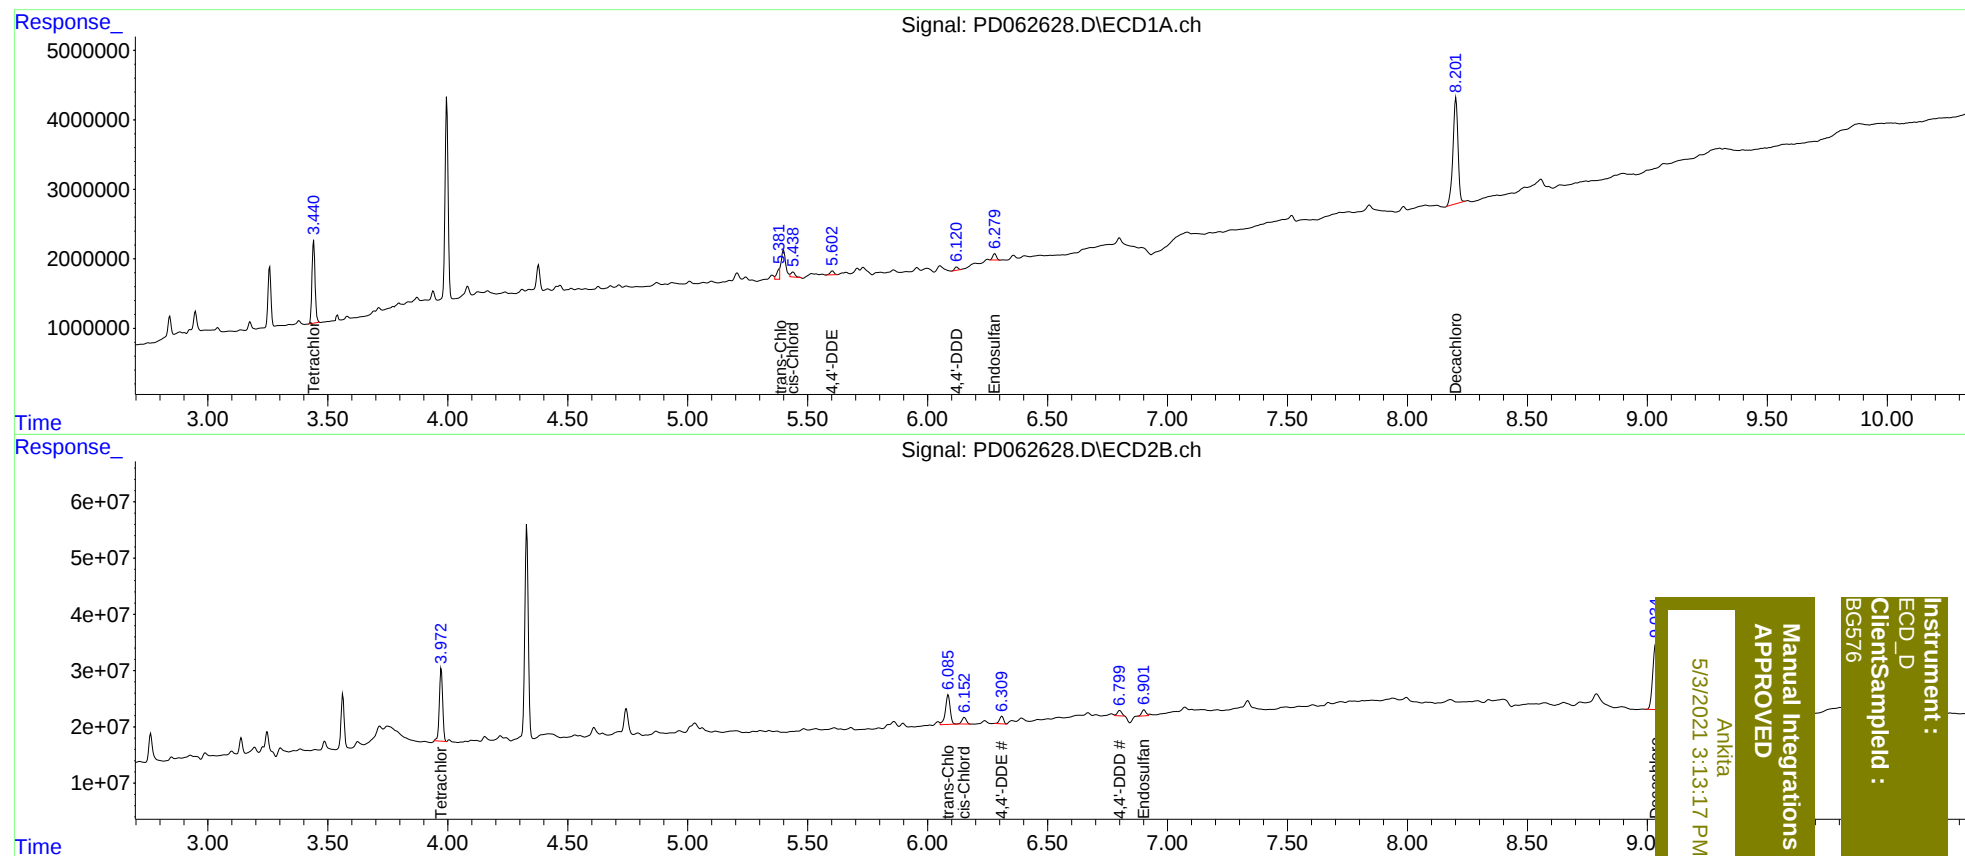

Manual Integrations
APPROVED

Ankita

5/3/2021 3:13:17 PM

Instrument :
ECD_D
ClientSample :
BG576