

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
 Data File : PD062655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 20:50
 Operator : AR\AJ
 Sample : M2129-03MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 E0AB9MSD

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:14:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 23:26:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	12812442	175.6E6	13.383	14.463m
27)	SA Decachlor...	8.201	9.034	15923421	201.3E6	14.835	18.443
Target Compounds							
2)	A alpha-BHC	3.877	4.360	51581169	608.1E6	36.841	32.158m
3)	MA gamma-BHC...	4.160	4.647	49755397	599.0E6	37.247	34.676
4)	MA Heptachlor	4.461	5.154	50974140	598.3E6	39.699	34.378
5)	MB Aldrin	4.710	5.459	49379118	582.5E6	37.909	33.673
6)	B beta-BHC	4.411	4.817	21450965	239.1E6	34.551	31.326
7)	B delta-BHC	4.616	5.033	21490183	260.6E6	15.793	14.045
8)	B Heptachlo...	5.153	5.845	46471629	510.0E6	37.922	31.800
9)	A Endosulfan I	5.493	6.202	39485683	453.4E6	35.312	30.914
10)	B trans-Chl...	5.380	6.079	45966271	588.6E6	36.666	35.940
11)	B cis-Chlor...	5.439	6.152	44134406	498.9E6	35.942	32.144
12)	B 4,4'-DDE	5.604	6.308	108.7E6	999.9E6	87.846	63.813m#
13)	MA Dieldrin	5.735	6.458	98237537	1047.2E6	77.934m	67.531m
14)	MA Endrin	5.994	6.678	83928174	833.1E6	79.321	66.801
15)	B Endosulfa...	6.267	6.887	79883180	851.0E6	77.025	67.996
16)	A 4,4'-DDD	6.120	6.800	78249712	857.1E6	78.582	68.959
17)	MA 4,4'-DDT	6.361	7.099	73352518	754.9E6	78.314	63.576
18)	B Endrin al...	6.436	7.011	66749093	705.4E6	74.810	64.653
19)	B Endosulfa...	6.650	7.234	65611695	741.7E6	65.637	58.121
20)	A Methoxychlor	6.909	7.557	207.2E6	1417.1E6	388.417	250.002m#
21)	B Endrin ke...	7.142	7.704	91508364	817.0E6	78.085	66.388

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
Data File : PD062655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 20:50
Operator : AR\AJ
Sample : M2129-03MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 23:26:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

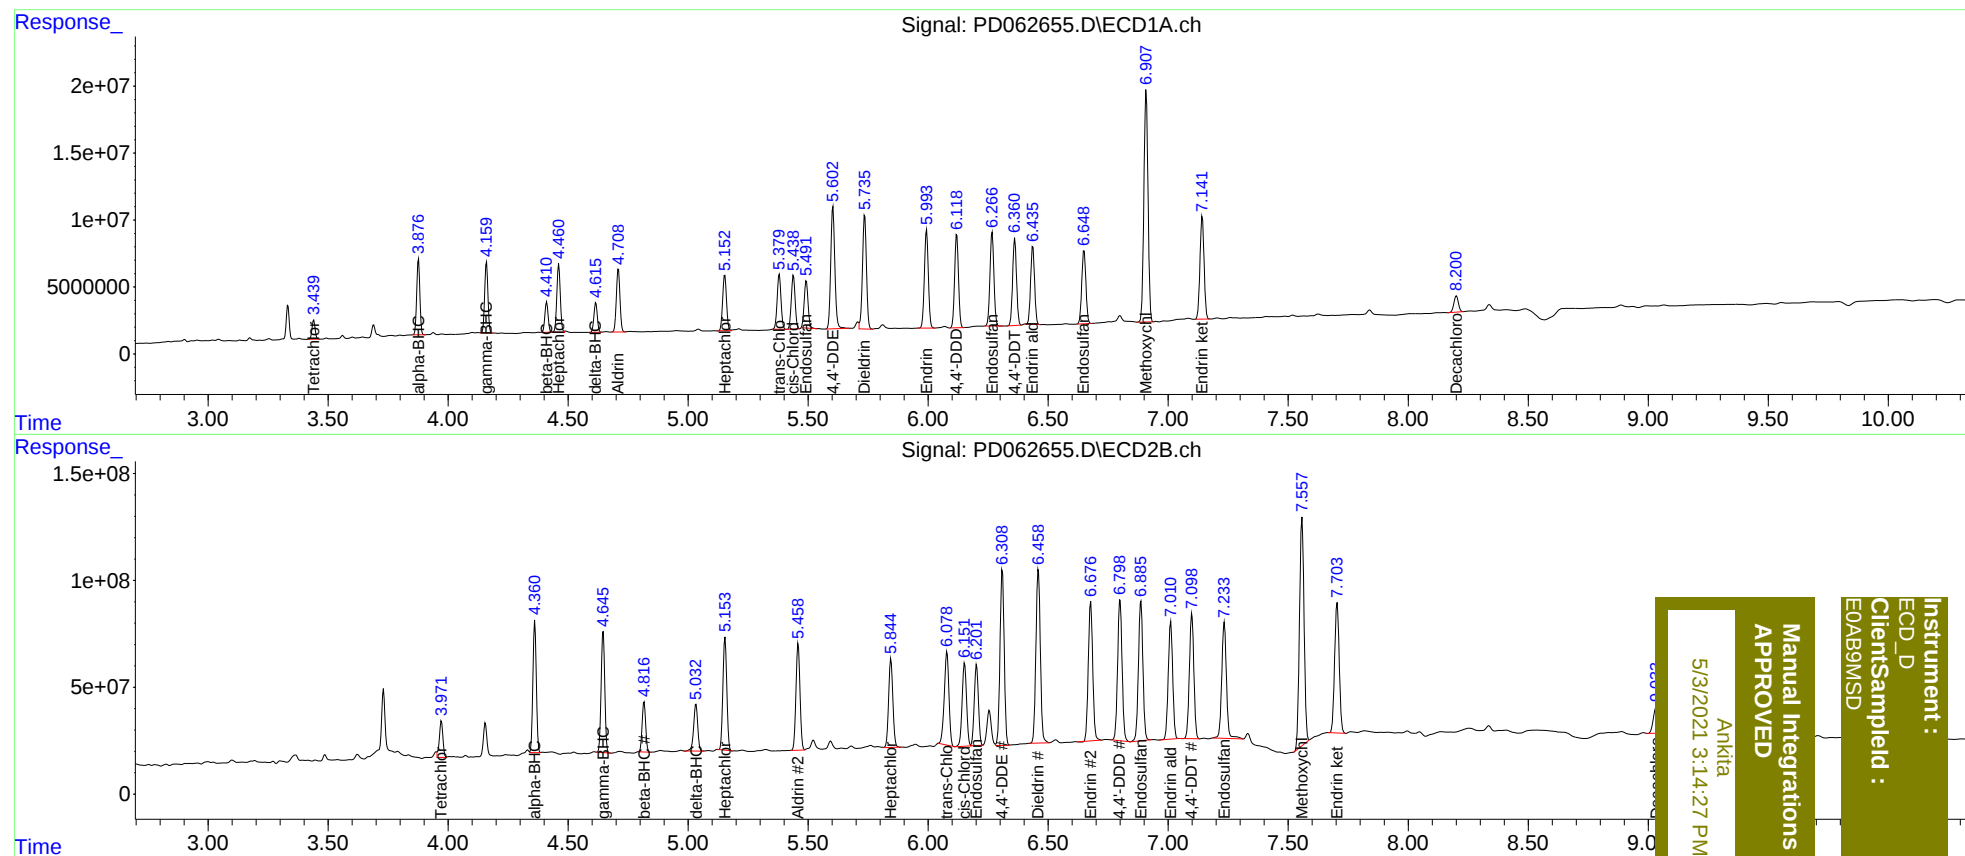

Manual Integrations
APPROVED

5/3/2021 3:14:27 PM

Instrument :
ECD_D
ClientSampled :
E0A89MSD

Ankita