

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
 Data File : PD062615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 11:31
 Operator : AR\AJ
 Sample : PB136040BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 PLCS040

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:12:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 23:13:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.972	20299989	259.1E6	21.203	21.339m
2)	SA Decachlor...	8.202	9.036	46455664	469.5E6	43.280	43.011
Target Compounds							
2)	A alpha-BHC	3.877	4.362	6335019	94896808	4.525	5.018
3)	MA gamma-BHC...	4.161	4.645	6102918	87217755	4.569	5.049m
4)	MA Heptachlor	4.462	5.155	5732366	82996666	4.464	4.769
5)	MB Aldrin	4.711	5.459	5806164	83820409	4.457	4.846
6)	B beta-BHC	4.412	4.817	2901533	35643637	4.673	4.669
7)	B delta-BHC	4.616	5.033	5823609	92685400	4.280	4.996
8)	B Heptachlo...	5.154	5.846	5668931	82775275	4.626	5.161
9)	A Endosulfan I	5.493	6.203	5107507	71026420	4.568	4.843
10)	B trans-Chl...	5.381	6.080	5971916	73282293	4.764	4.475
11)	B cis-Chlor...	5.439	6.153	5606912	72600912	4.566	4.677
12)	B 4,4'-DDE	5.603	6.310	10720549	144.9E6	8.663	9.244
13)	MA Dieldrin	5.737	6.460	11253501	148.8E6	8.928	9.597
14)	MA Endrin	5.994	6.677	10125760	114.5E6	9.570	9.182
15)	B Endosulfa...	6.268	6.887	9844560	137.8E6	9.492	11.011
16)	A 4,4'-DDD	6.121	6.800	9098472	141.0E6	9.137	11.345
17)	MA 4,4'-DDT	6.362	7.099	7116009	98977018	7.597	8.336
18)	B Endrin al...	6.437	7.011	8813098	107.4E6	9.877	9.843
19)	B Endosulfa...	6.650	7.234	8697455	123.8E6	8.701	9.701
20)	A Methoxychlor	6.909	7.558	23319714	253.9E6	43.706	44.788
21)	B Endrin ke...	7.143	7.705	11420016	120.9E6	9.745	9.820

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
Data File : PD062615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 11:31
Operator : AR\AJ
Sample : PB136040BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 23:13:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

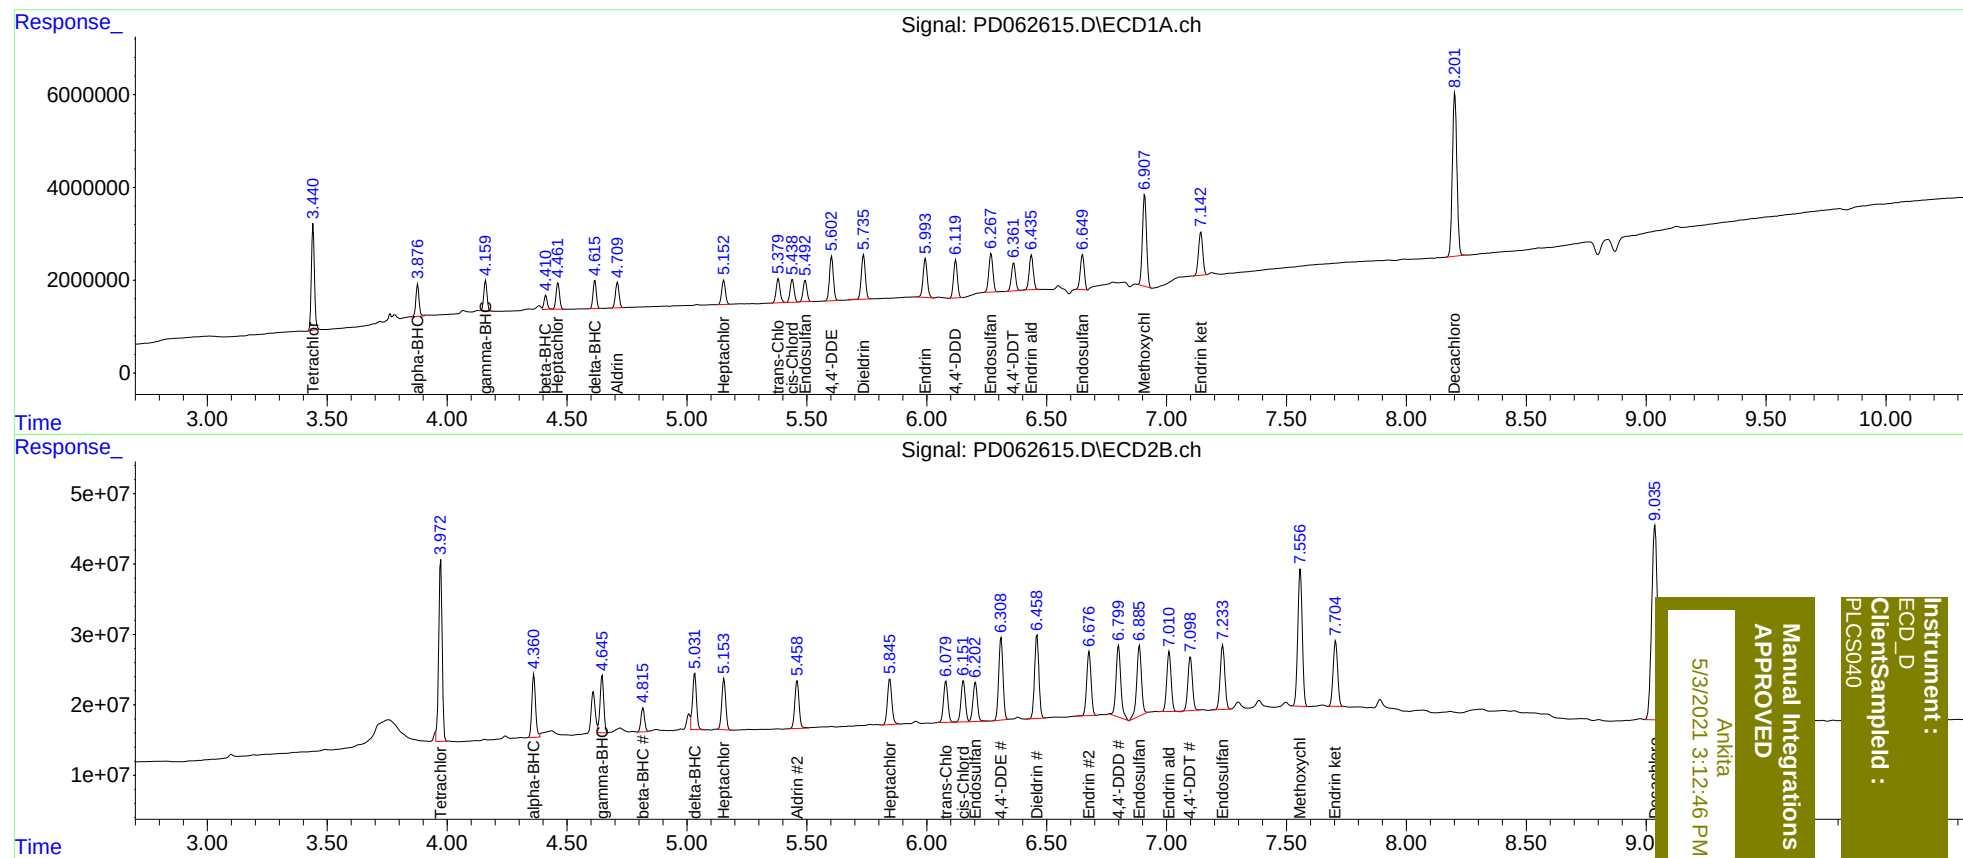

Manual Integrations
APPROVED

Ankita
5/3/2021 3:12:46 PM

Instrument :
ECD_D
ClientSample :
PLCS040