

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
 Data File : PD062632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 15:28
 Operator : AR\AJ
 Sample : INDA333
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3033

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 23:18:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.973	18253599	229.7E6	19.066	18.912
27)	SA Decachlor...	8.202	9.036	40493507	399.2E6	37.725	36.570
Target Compounds							
2)	A alpha-BHC	3.877	4.362	26683811	354.3E6	19.059	18.735
3)	MA gamma-BHC...	4.161	4.646	25136002	317.5E6	18.817	18.382
4)	MA Heptachlor	4.462	5.155	24234043	318.4E6	18.873	18.294
9)	A Endosulfan I	5.493	6.202	20165666	268.1E6	18.034	18.277
13)	MA Dieldrin	5.737	6.460	47674842	566.8E6	37.821	36.553
14)	MA Endrin	5.994	6.678	37058506	419.7E6	35.024	33.649
16)	A 4,4'-DDD	6.120	6.800	38433201	455.8E6	38.597	36.673
17)	MA 4,4'-DDT	6.362	7.099	33753568	394.3E6	36.037	33.206
20)	A Methoxychlor	6.909	7.558	97664366	961.0E6	183.042	169.550

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043021\
Data File : PD062632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 15:28
Operator : AR\AJ
Sample : INDA333
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 23:18:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

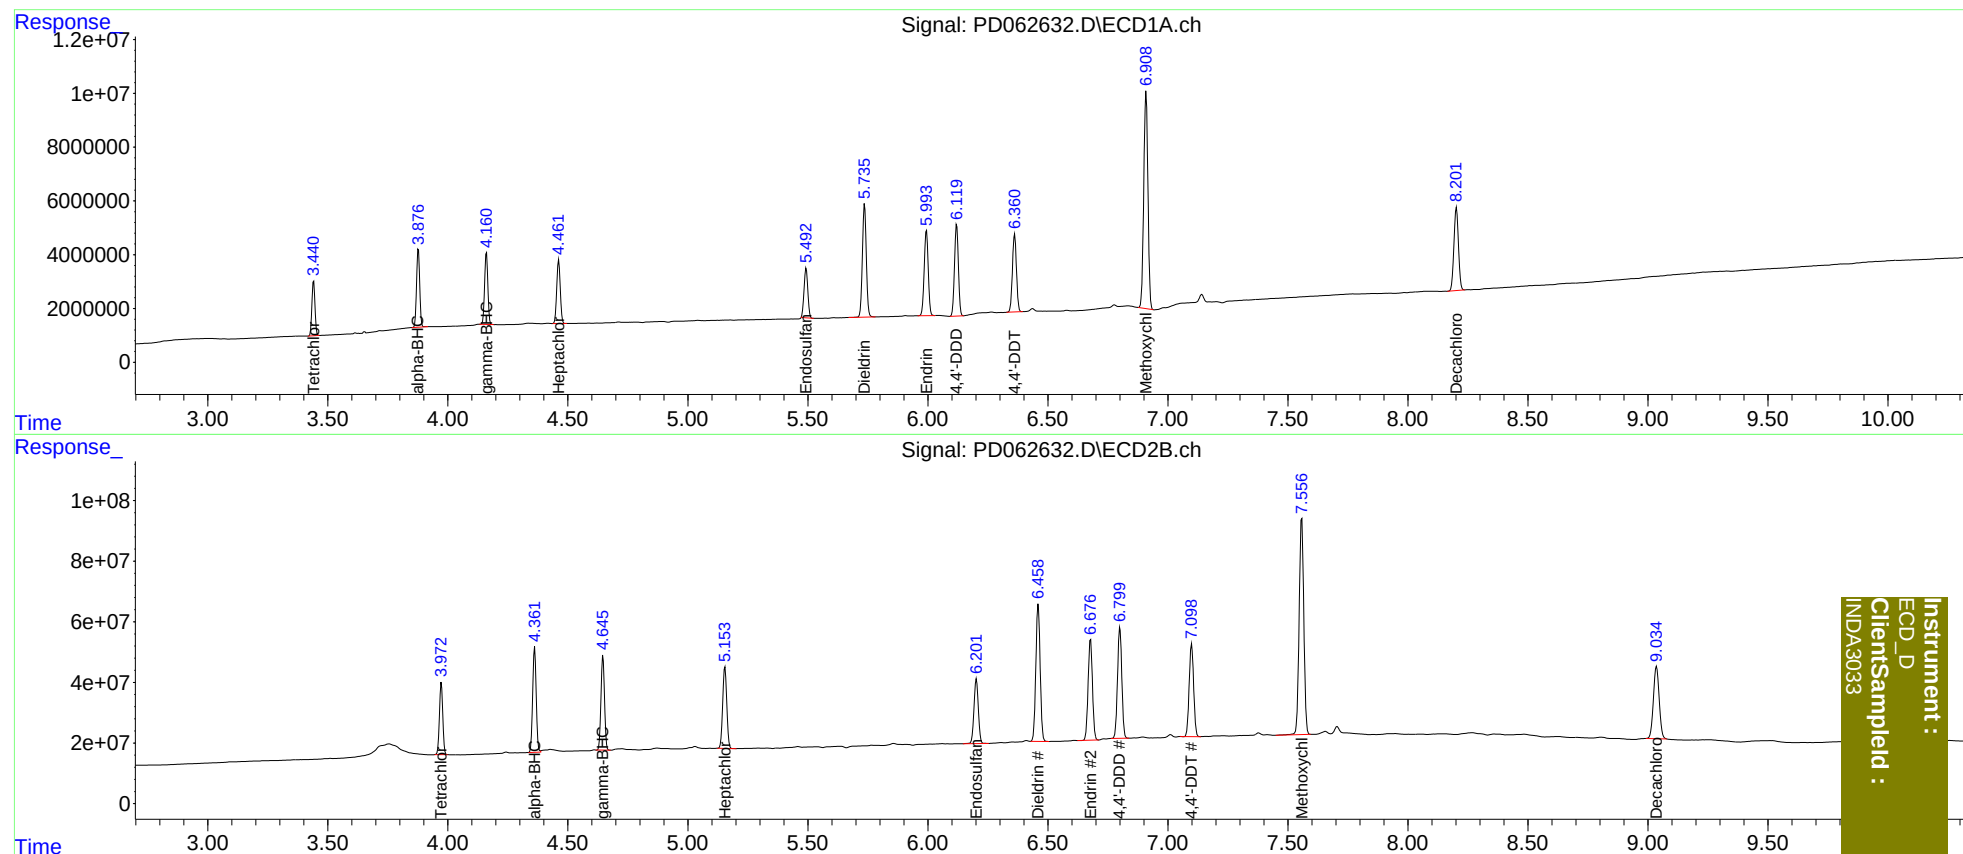

Instrument :
ECD_D
ClientSampled :
INDA3033