

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043024\
 Data File : PD082663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 15:52
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 21:39:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 16:11:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	0.000	3.621	0	335267	<MDL
6) B	beta-BHC	0.000	3.857f	0	276362	0.121
8) B	Heptachlo...	0.000	4.663f	0	80030	<MDL
9) A	Endosulfan I	0.000	5.124	0	676309	0.157
12) B	4,4'-DDE	0.000	5.163f	0	68197	<MDL
14) MA	Endrin	0.000	5.654	0	479014	0.113
15) B	Endosulfa...	0.000	5.886f	0	298326	<MDL
17) MA	4,4'-DDT	0.000	6.057	0	105932	<MDL
18) B	Endrin al...	0.000	6.087	0	66940	<MDL
19) B	Endosulfa...	0.000	6.347	0	45287	<MDL
20) A	Methoxychlor	0.000	6.609	0	46864	<MDL
24)	Toxaphene-3	0.000	6.609	0	46864	0.520
25)	Toxaphene-4	0.000	6.751	0	29185	0.240

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043024\
Data File : PD082663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 15:52
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 21:39:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 16:11:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

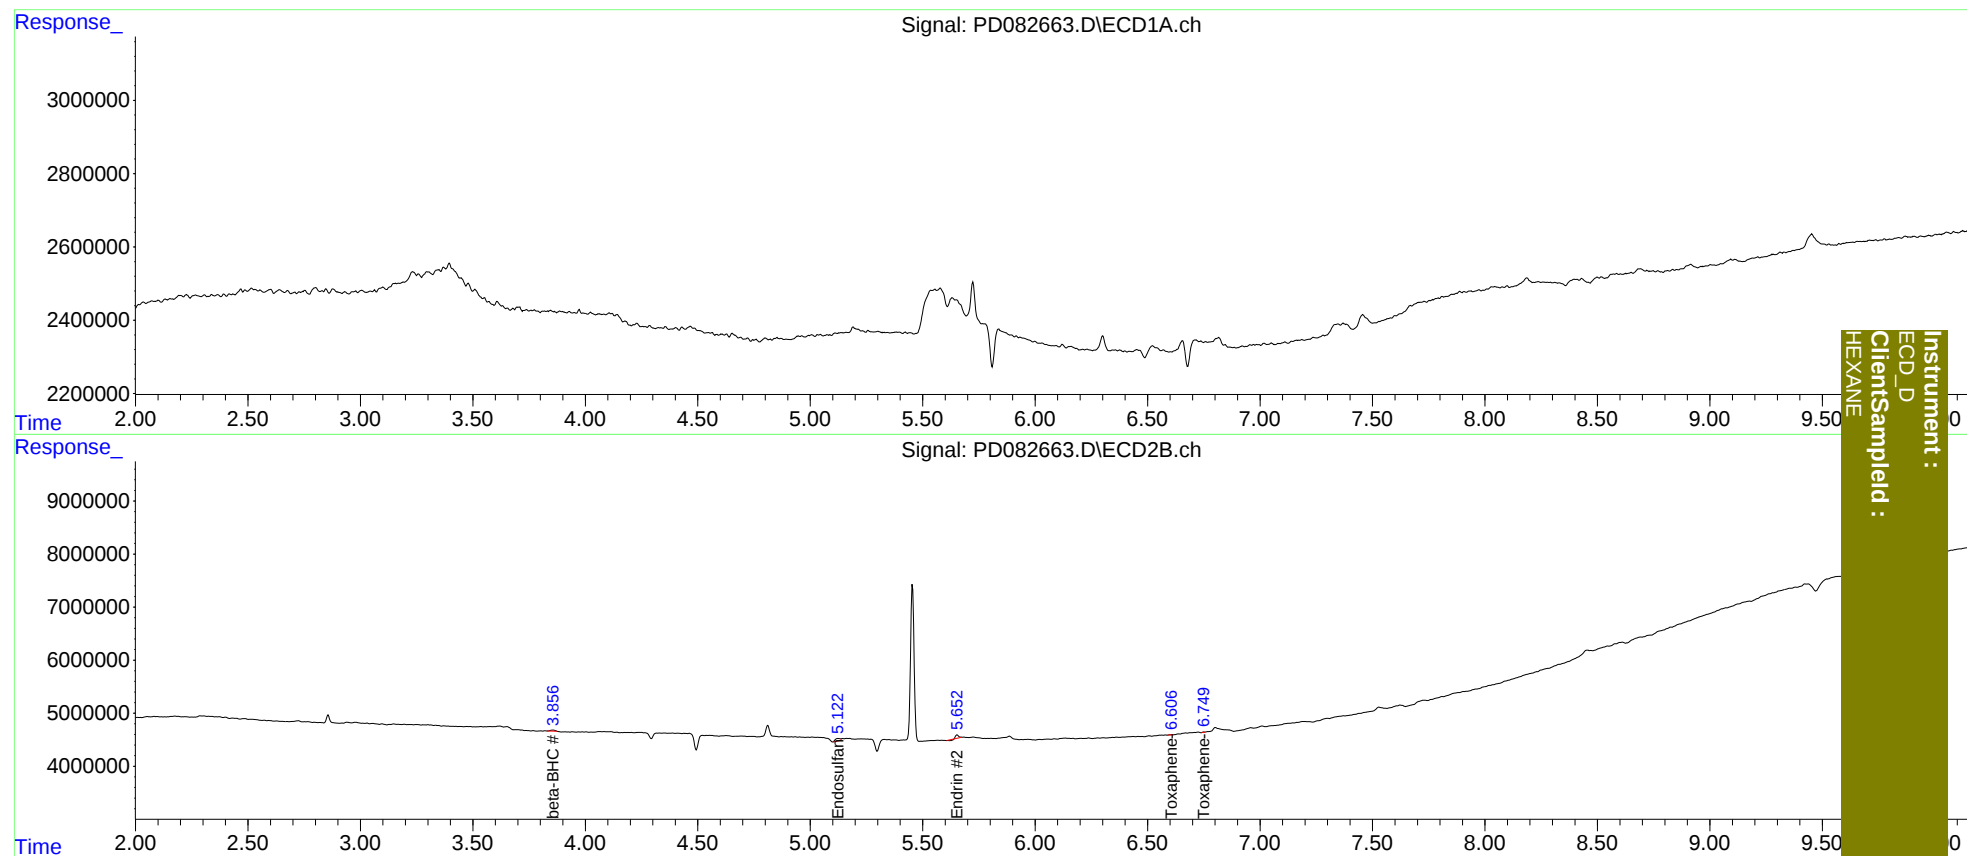


Instrument :
ECD_D
ClientSampled :
HEXANE

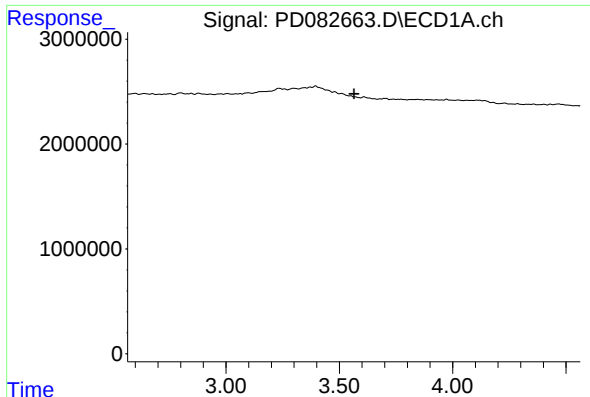

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

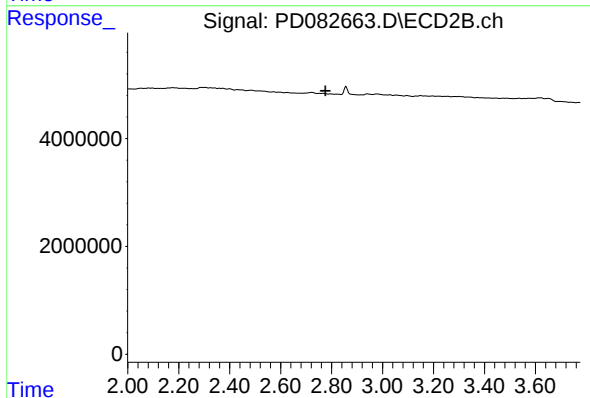


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.776 min
Response: 0
Conc: N.D.

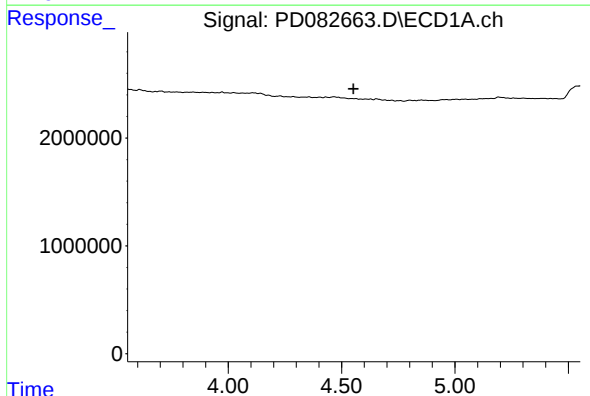


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.553 min
Response: 0
Conc: N.D.

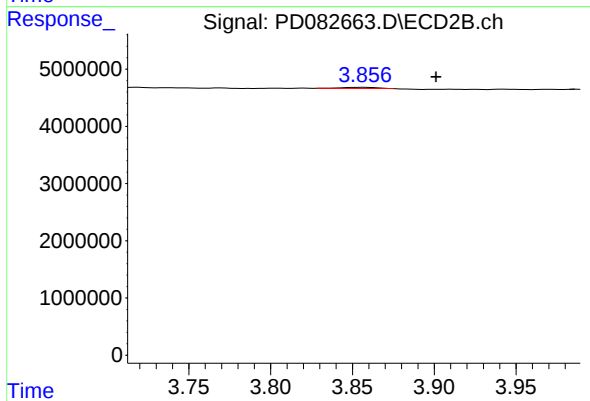

#6 beta-BHC


R.T.: 3.857 min
Delta R.T.: -0.044 min
Response: 276362
Conc: 0.12 ng/ml

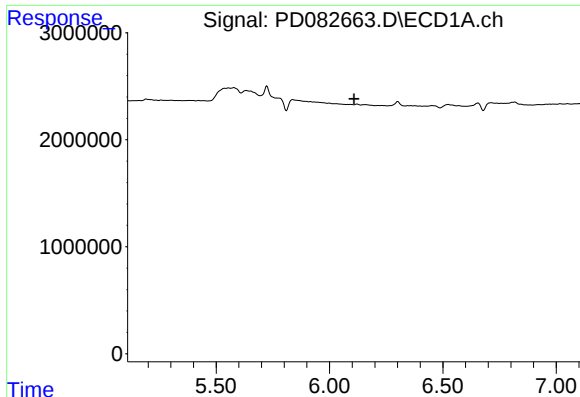

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

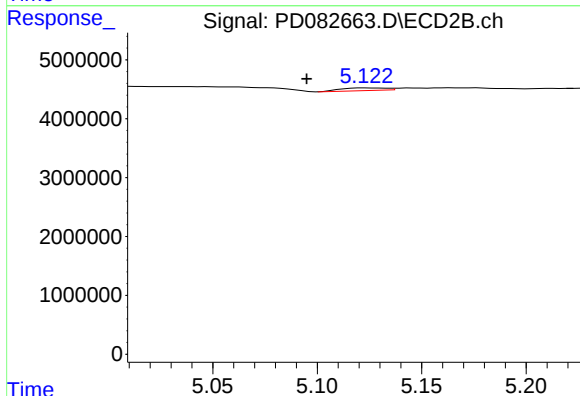


#9 Endosulfan I

R.T.: 5.124 min
Delta R.T.: 0.029 min
Response: 676309
Conc: 0.16 ng/ml

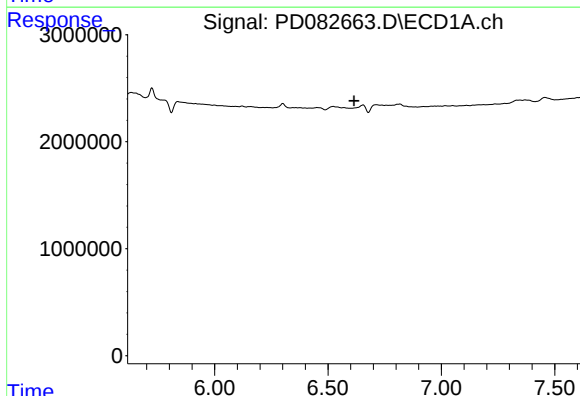


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.616 min
Response: 0
Conc: N.D.

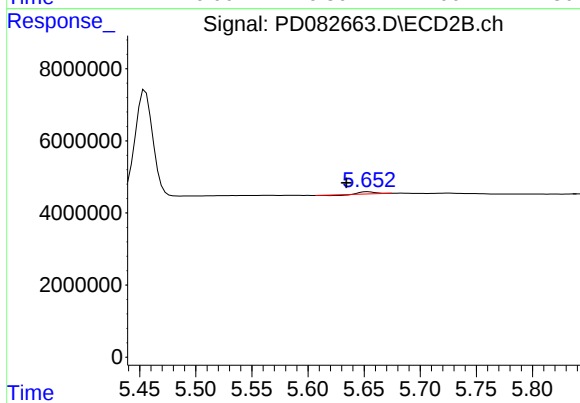

#14 Endrin


R.T.: 5.654 min
Delta R.T.: 0.019 min
Response: 479014
Conc: 0.11 ng/ml

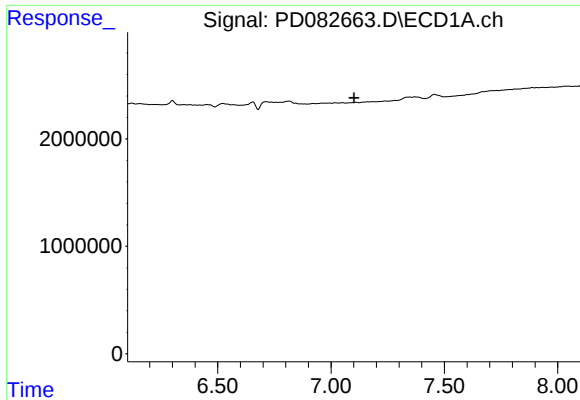

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

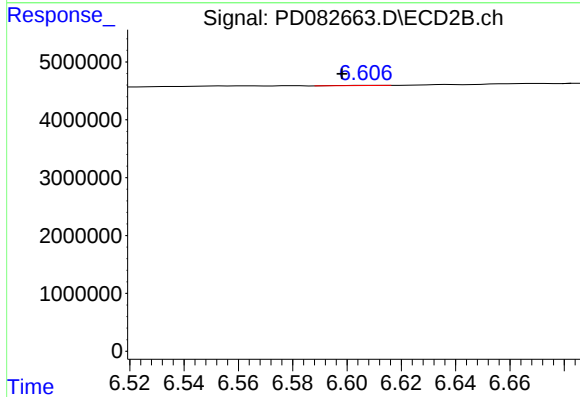


#24 Toxaphene-3

R.T.: 6.609 min
Delta R.T.: 0.011 min
Response: 46864
Conc: 0.52 ng/ml

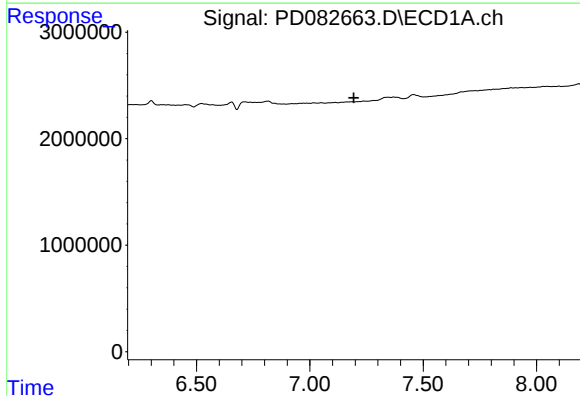


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.194 min
Response: 0
Conc: N.D.

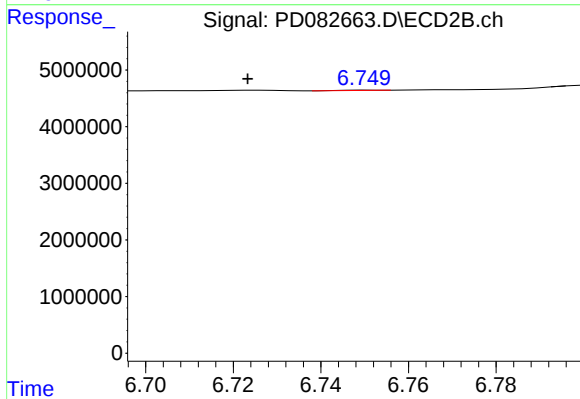

#25 Toxaphene-4


R.T.: 6.751 min
Delta R.T.: 0.027 min
Response: 29185
Conc: 0.24 ng/ml

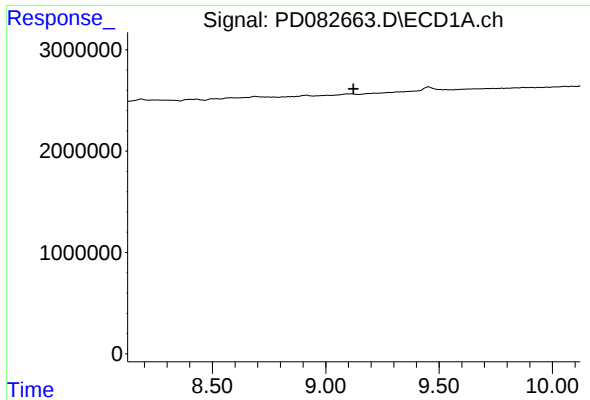

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

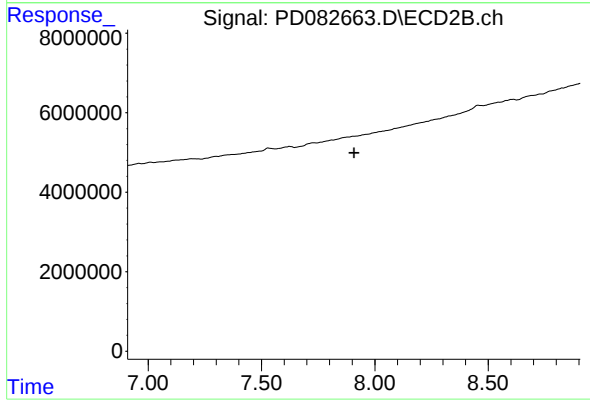

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.909 min
Response: 0
Conc: N.D.