

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043024\
 Data File : PD082667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 17:30
 Operator : AR\AJ
 Sample : P2203-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/30/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 05:21:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 16:11:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.775	22725178	55045221	16.071	15.729
27) SA Decachlor...	9.122	7.907	30672630	58148478	15.742	15.408
Target Compounds						
7) B delta-BHC	4.821	4.139	7349614	19946809	3.121m	3.642
10) B trans-Chl...	5.970	4.951	12345222	15682685	5.916m	3.322m#
14) MA Endrin	6.612	5.601	10801250	21417326	5.912	5.060m
17) MA 4,4'-DDT	7.035	6.026	3492910	10020297	2.171m	2.666

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD043024\
Data File : PD082667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 17:30
Operator : AR\AJ
Sample : P2203-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 05:21:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 16:11:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

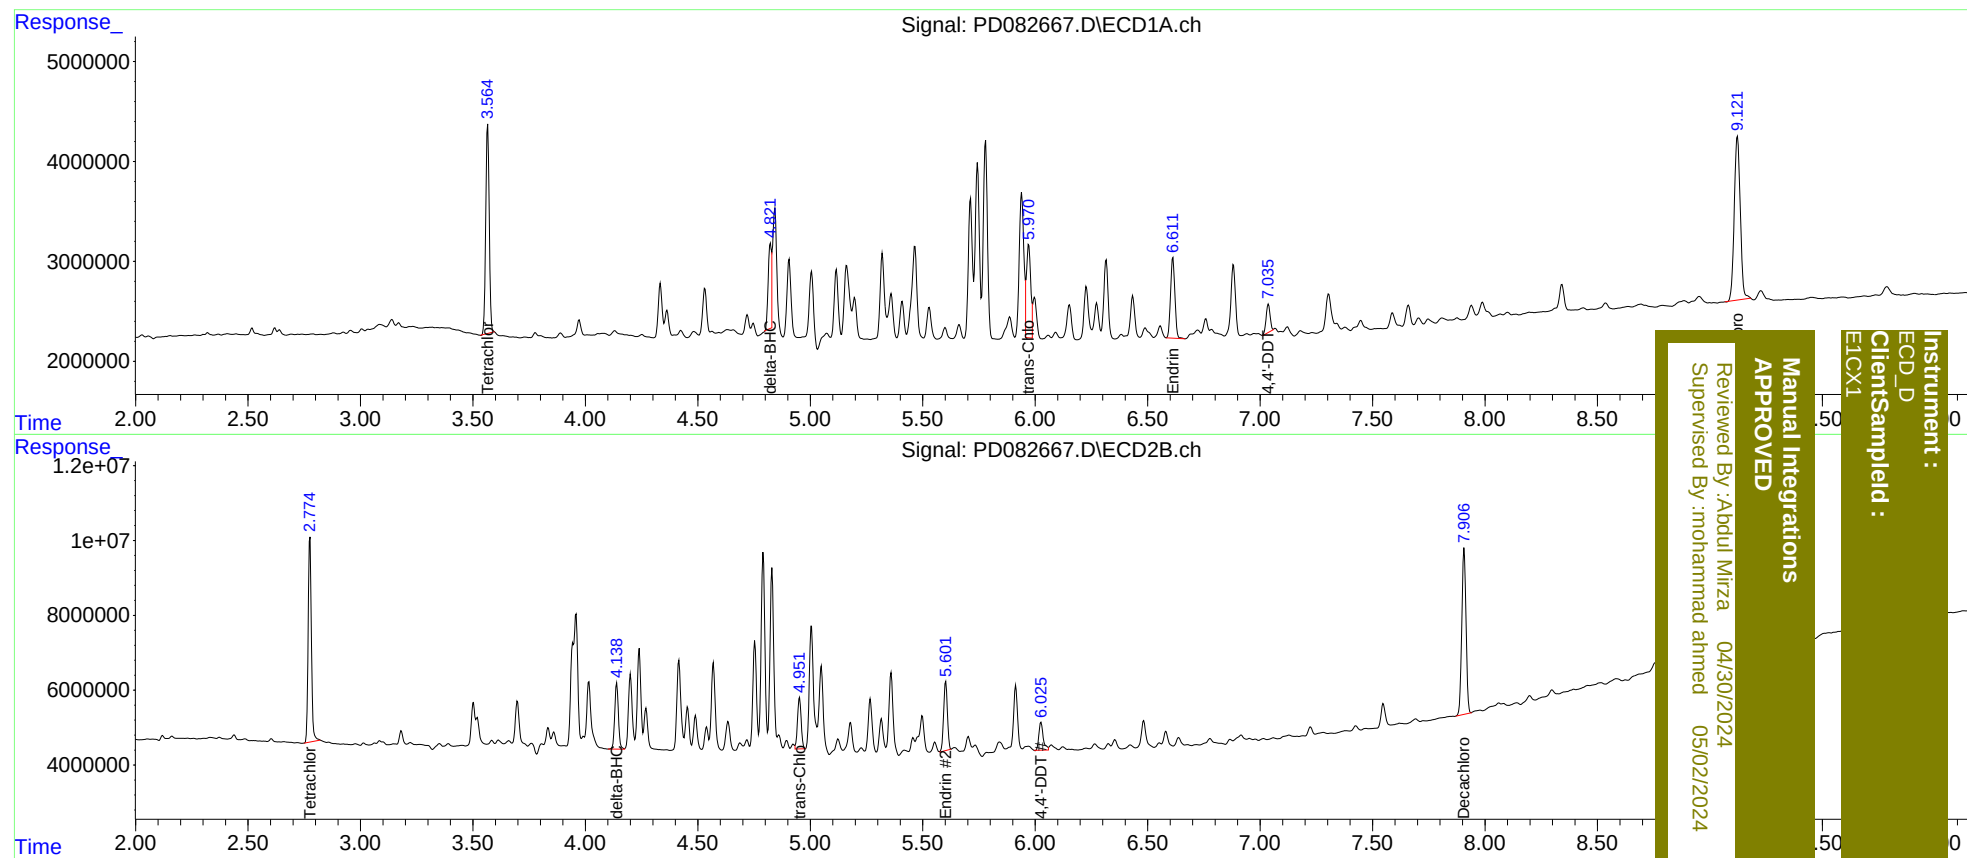

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/30/2024
Supervised By: mohammad ahmed 05/02/2024

Instrument :
ECD_D
ClientSampled :
EICX1