

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050119\
 Data File : PD053130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 May 2019 17:07
 Operator : AJ\SJ
 Sample : PIBLK04
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:13:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042319CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 03:53:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.217	4.040	31551708	630.3E6	22.491	24.769
27) SA	Decachlor...	7.810	9.149	53740226	628.1E6	37.370	32.781
Target Compounds							
8) B	Heptachlo...	0.000	5.917	0 85810847	N.D.		2.793
9) A	Endosulfan I	0.000	6.251	0 29206374	N.D.		0.998
11) B	cis-Chlor...	0.000	6.251	0 29206374	N.D.		0.985


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050119\
Data File : PD053130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 May 2019 17:07
Operator : AJ\SJ
Sample : PIBLK04
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:13:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042319CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 03:53:52 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

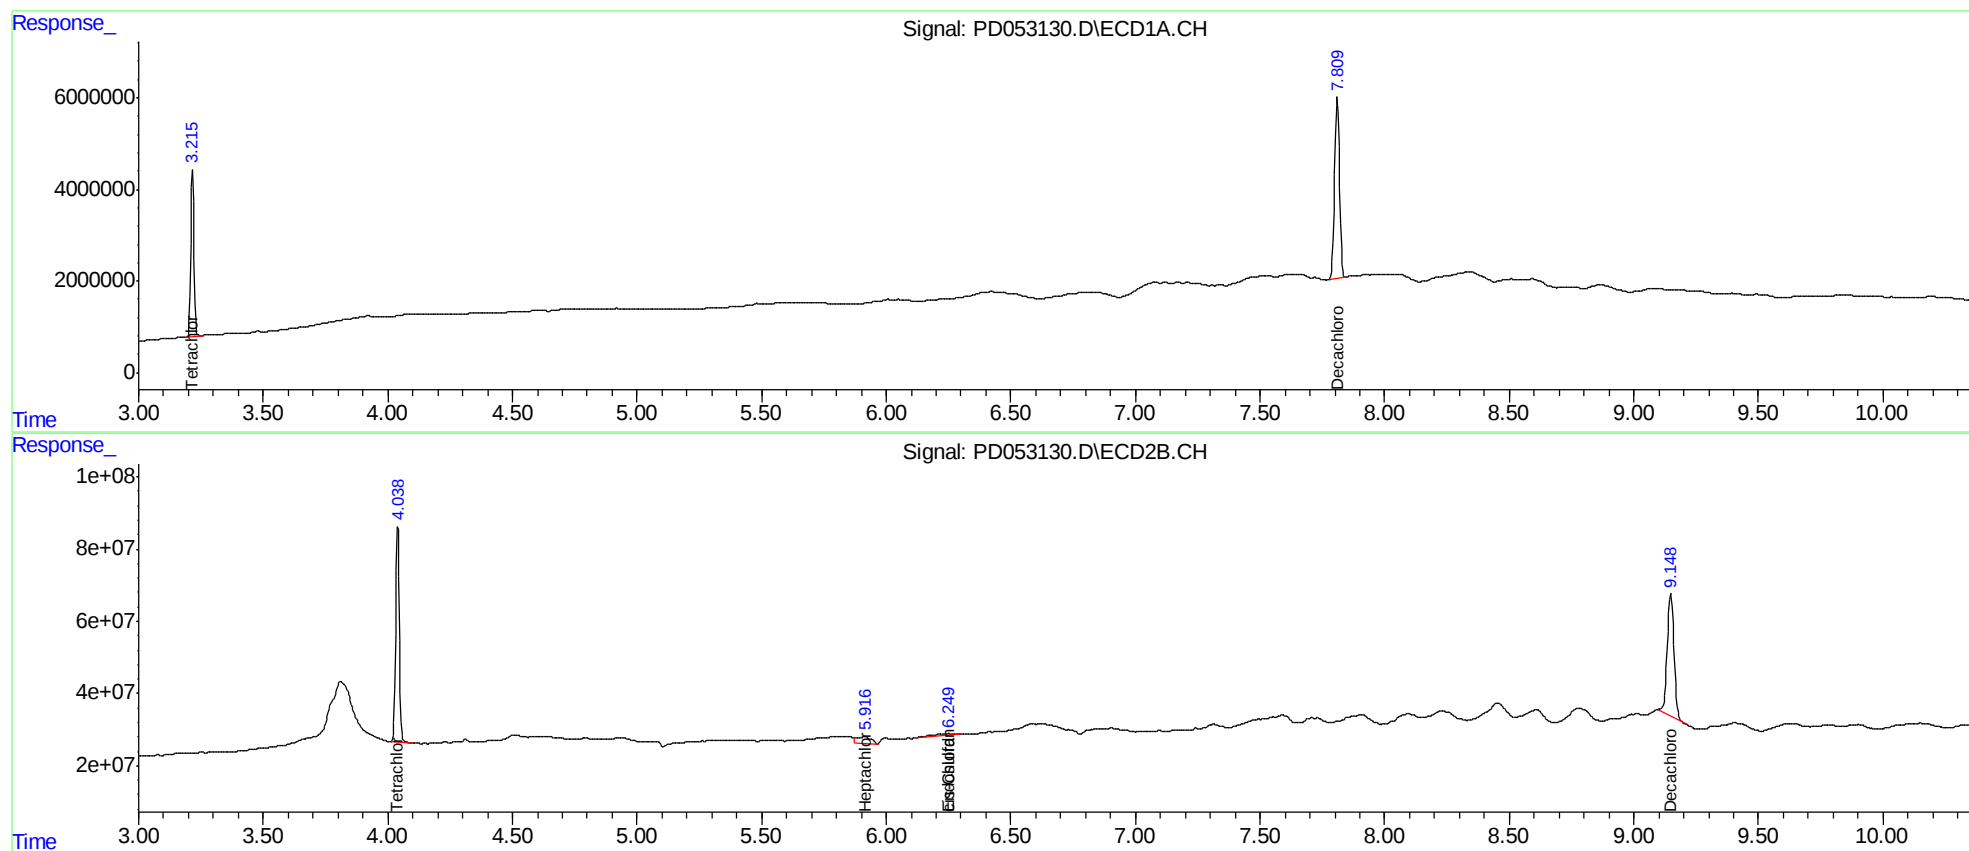


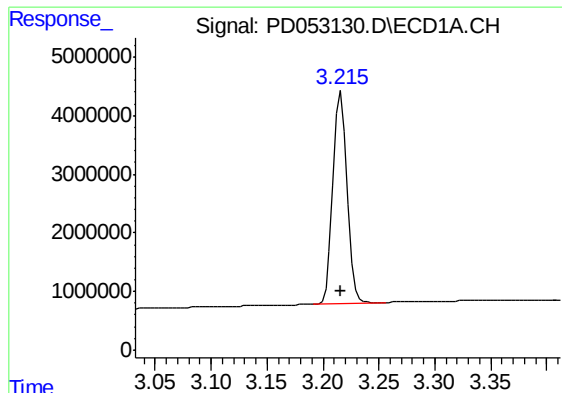

#1 Tetrachloro-m-xylene


R.T.: 3.217 min
Delta R.T.: 0.000 min
Response: 31551708
Conc: 22.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK04

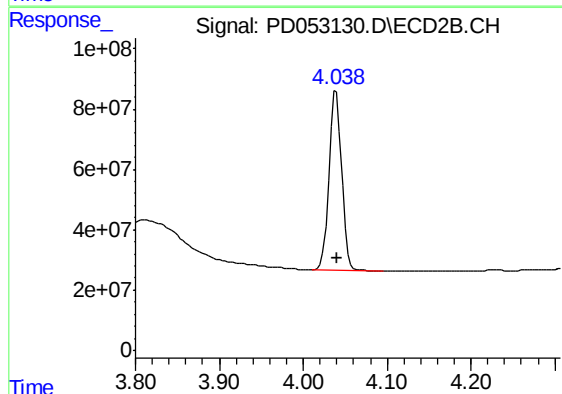


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 630263986
Conc: 24.77 ng/ml

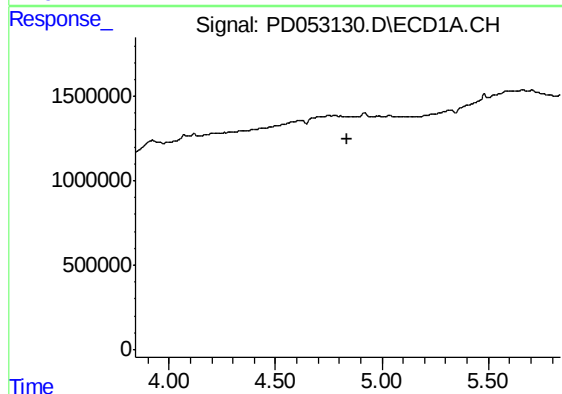


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

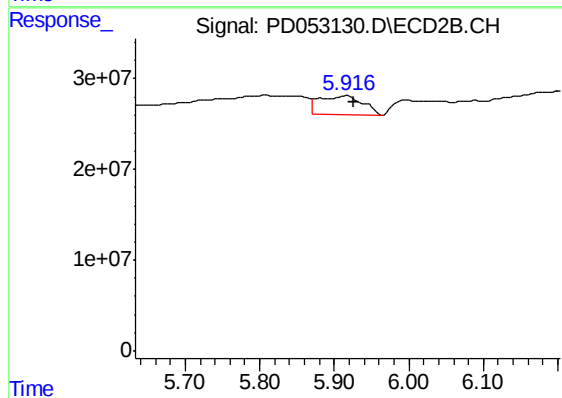

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: -0.009 min
Response: 85810847
Conc: 2.79 ng/ml

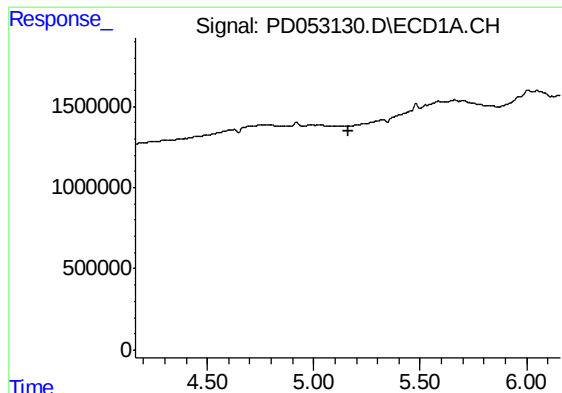

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK04

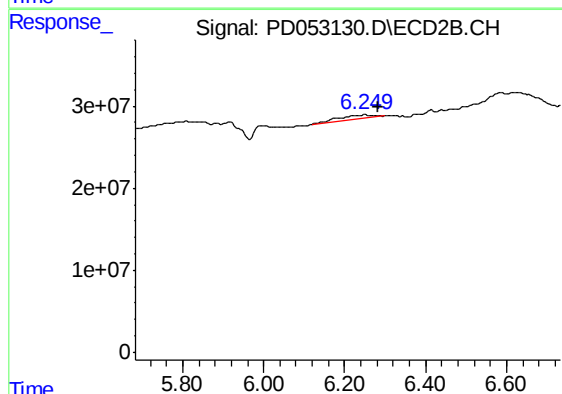


#9 Endosulfan I

R.T.: 6.251 min
Delta R.T.: -0.034 min
Response: 29206374
Conc: 1.00 ng/ml

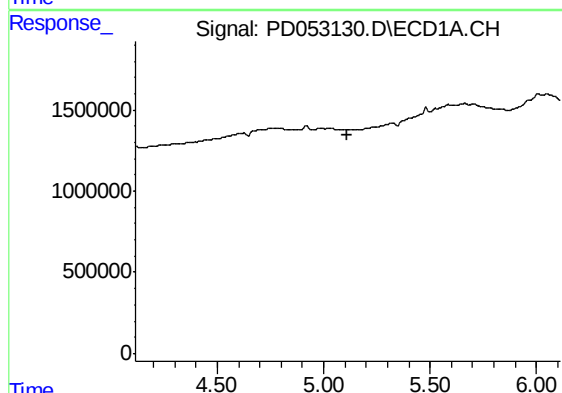


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.113 min
Response: 0
Conc: N.D.

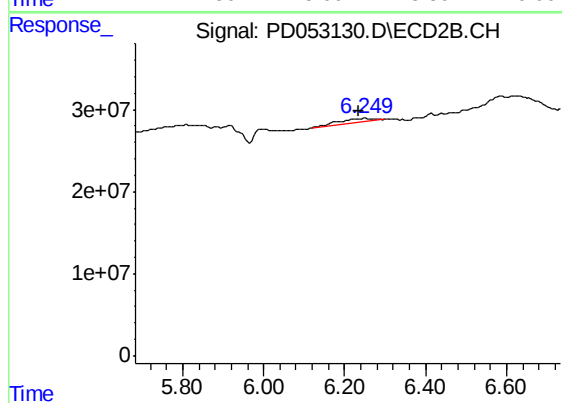

#11 cis-Chlordane


R.T.: 6.251 min
Delta R.T.: 0.016 min
Response: 29206374
Conc: 0.98 ng/ml

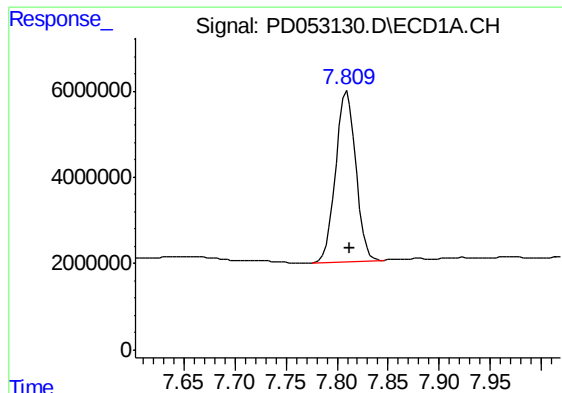

#27 Decachlorobiphenyl

R.T.: 7.810 min
Delta R.T.: -0.003 min
Response: 53740226
Conc: 37.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK04

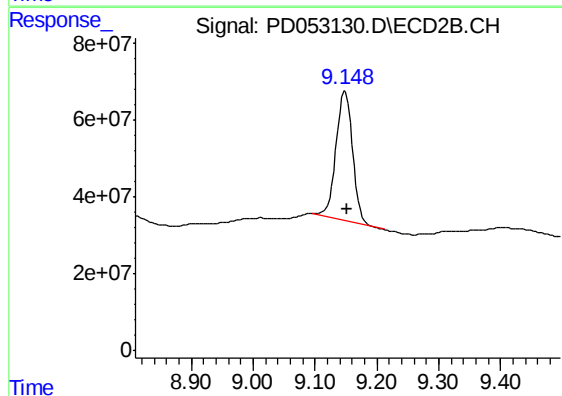

#27 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.004 min
Response: 628065351
Conc: 32.78 ng/ml