

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
 Data File : PD075073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 12:37
 Operator : AR\AJ
 Sample : 02374-04MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9D6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/02/2023
 Supervised By :Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:26:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.771	30888214	14082664	13.828m	13.584
27) SA Decachlor...	9.096	7.923	64995055	19893223	27.213m	20.709
Target Compounds						
2) A alpha-BHC	4.004	3.274	169.2E6	64929877	46.116m	45.091
3) MA gamma-BHC...	4.338	3.603	155.1E6	63916681	45.372m	45.933m
4) MA Heptachlor	4.932	3.946	157.0E6	58516527	45.310	41.955
5) MB Aldrin	5.276	4.227	163.8E6	64719398	48.921	49.217
6) B beta-BHC	4.536	3.901	57486093	25957227	38.999	38.142
7) B delta-BHC	4.784	4.131	119.7E6	49080442	39.985	34.891
8) B Heptachlo...	5.703	4.729	143.4E6	50852914	47.739	41.418
9) A Endosulfan I	6.089	5.101	123.9E6	37162376	42.565m	32.571
10) B trans-Chl...	5.959	4.980	160.2E6	59370198	53.530m	49.008
11) B cis-Chlor...	6.040	5.045	145.9E6	55818361	46.798	45.082
12) B 4,4'-DDE	6.210	5.234	240.2E6	101.2E6	81.782m	89.429
13) MA Dieldrin	6.367	5.366	298.2E6	121.6E6	93.825	96.900
14) MA Endrin	6.598	5.642	246.4E6	99003291	90.937	89.577
15) B Endosulfa...	6.816	5.936	242.4E6	96984330	83.700	88.907
16) A 4,4'-DDD	6.729	5.790	228.9E6	78931398	94.660m	81.695
17) MA 4,4'-DDT	7.046	6.041	236.3E6	83372114	94.043	84.045
18) B Endrin al...	6.947	6.115	171.8E6	61745803	76.744	69.524
19) B Endosulfa...	7.183	6.338	211.0E6	80368614	80.911	78.166
20) A Methoxychlor	7.523	6.618	601.8E6	222.6E6	417.435	402.922
21) B Endrin ke...	7.670	6.846	253.4E6	90157686	87.601	75.610

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
Data File : PD075073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 12:37
Operator : AR\AJ
Sample : 02374-04MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:26:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

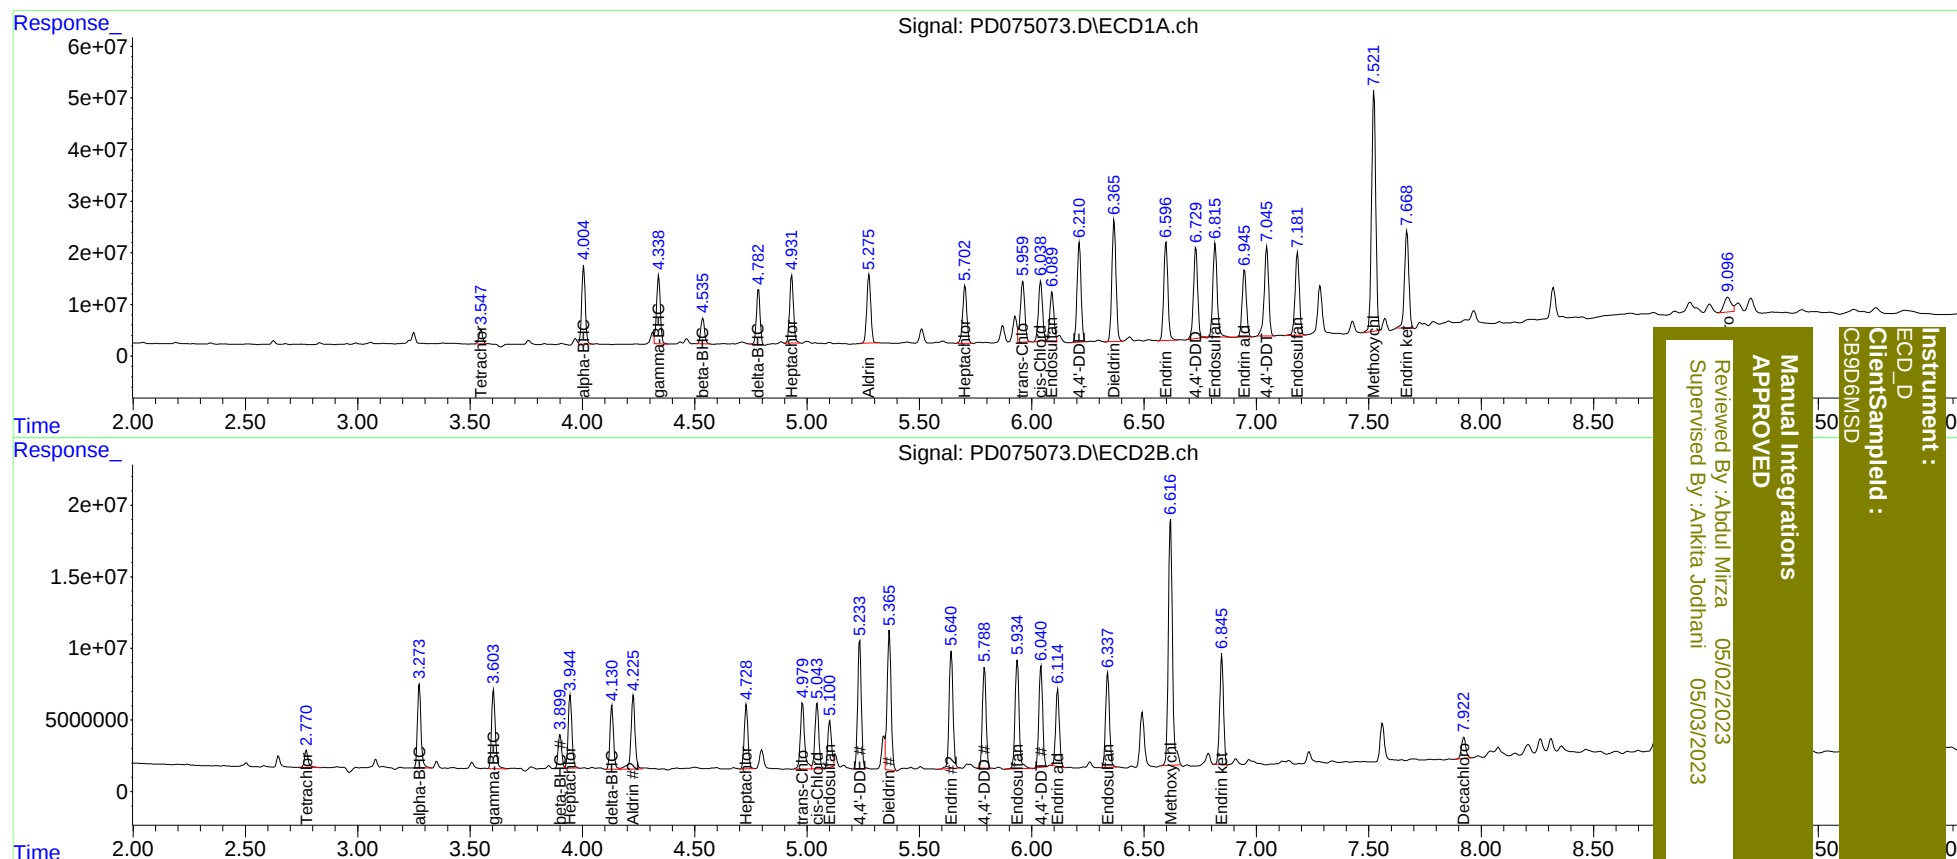

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 05/02/2023
Supervised By: Ankita Jodhani 05/03/2023

Instrument :
ECD_D
Client Sampled :
CB9D6MSD