

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
 Data File : PD075085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 17:11
 Operator : AR\AJ
 Sample : 02419-27DL2 40X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW924DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/02/2023
 Supervised By : Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:27:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	4.343	3.615	14285161	765135	4.178m 0.550 #
6) B	beta-BHC	4.513	3.859f	70300560	6258363	47.692m 9.196m#
12) B	4,4'-DDE	6.206	5.183f	112.9E6	24331164	38.444m 21.510m#
14) MA	Endrin	6.592	5.607	153.3E6	62738587	56.587 56.765m
17) MA	4,4'-DDT	7.016	6.033	156.8E6	69219910	62.393m 69.778m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
Data File : PD075085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 17:11
Operator : AR\AJ
Sample : 02419-27DL2 40X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:27:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

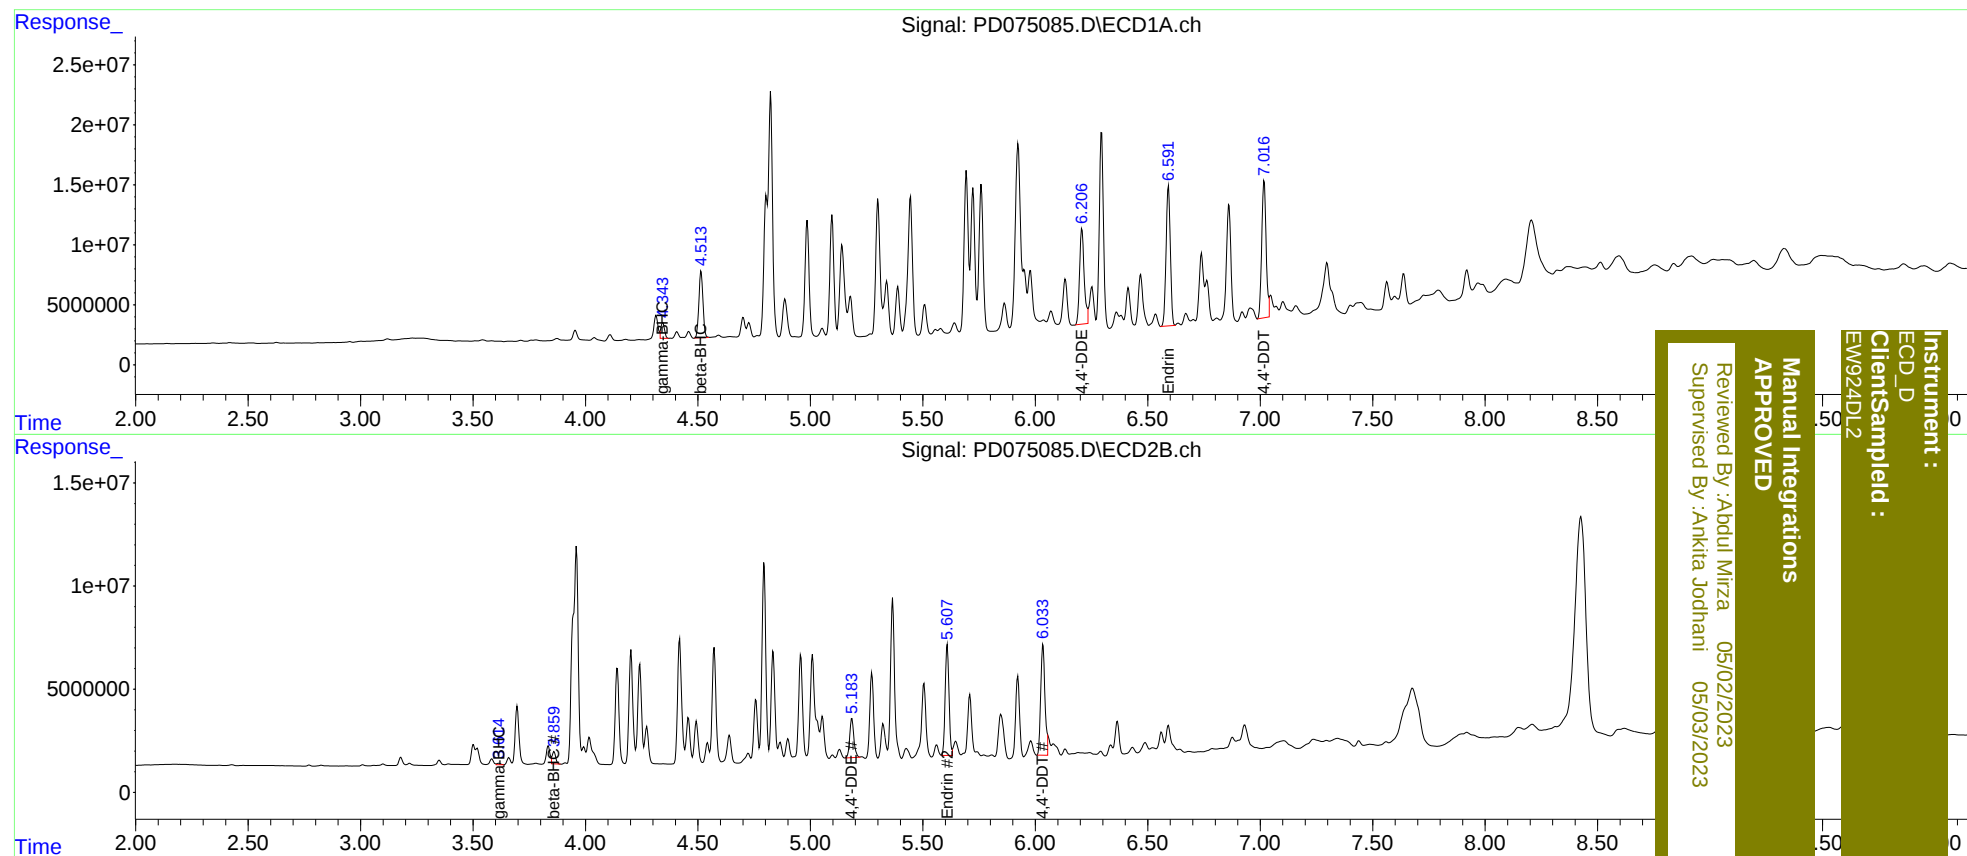

Reviewed By: Abdul Mirza 05/02/2023
Supervised By: Ankita Jodhani 05/03/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW924DL2