

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
 Data File : PD075071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 11:43
 Operator : AR\AJ
 Sample : 02374-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9D6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/03/2023
 Supervised By : Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 07:13:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.771	29474482	13921857	13.195m	13.429
2) SA Decachlor...	9.097	7.924	62003586	19771103	25.960m	20.582
Target Compounds						
10) B trans-Chl...	5.957	4.979	12952770	4150427	4.327m	3.426m
11) B cis-Chlor...	6.041	5.043	13332604	5024726	4.277	4.058m
12) B 4,4'-DDE	6.209	5.235	3711931	3067939	1.264m	2.712 #
13) MA Dieldrin	6.383	5.370	6253235	11036745	1.967m	8.793 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
Data File : PD075071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 11:43
Operator : AR\AJ
Sample : 02374-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 07:13:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

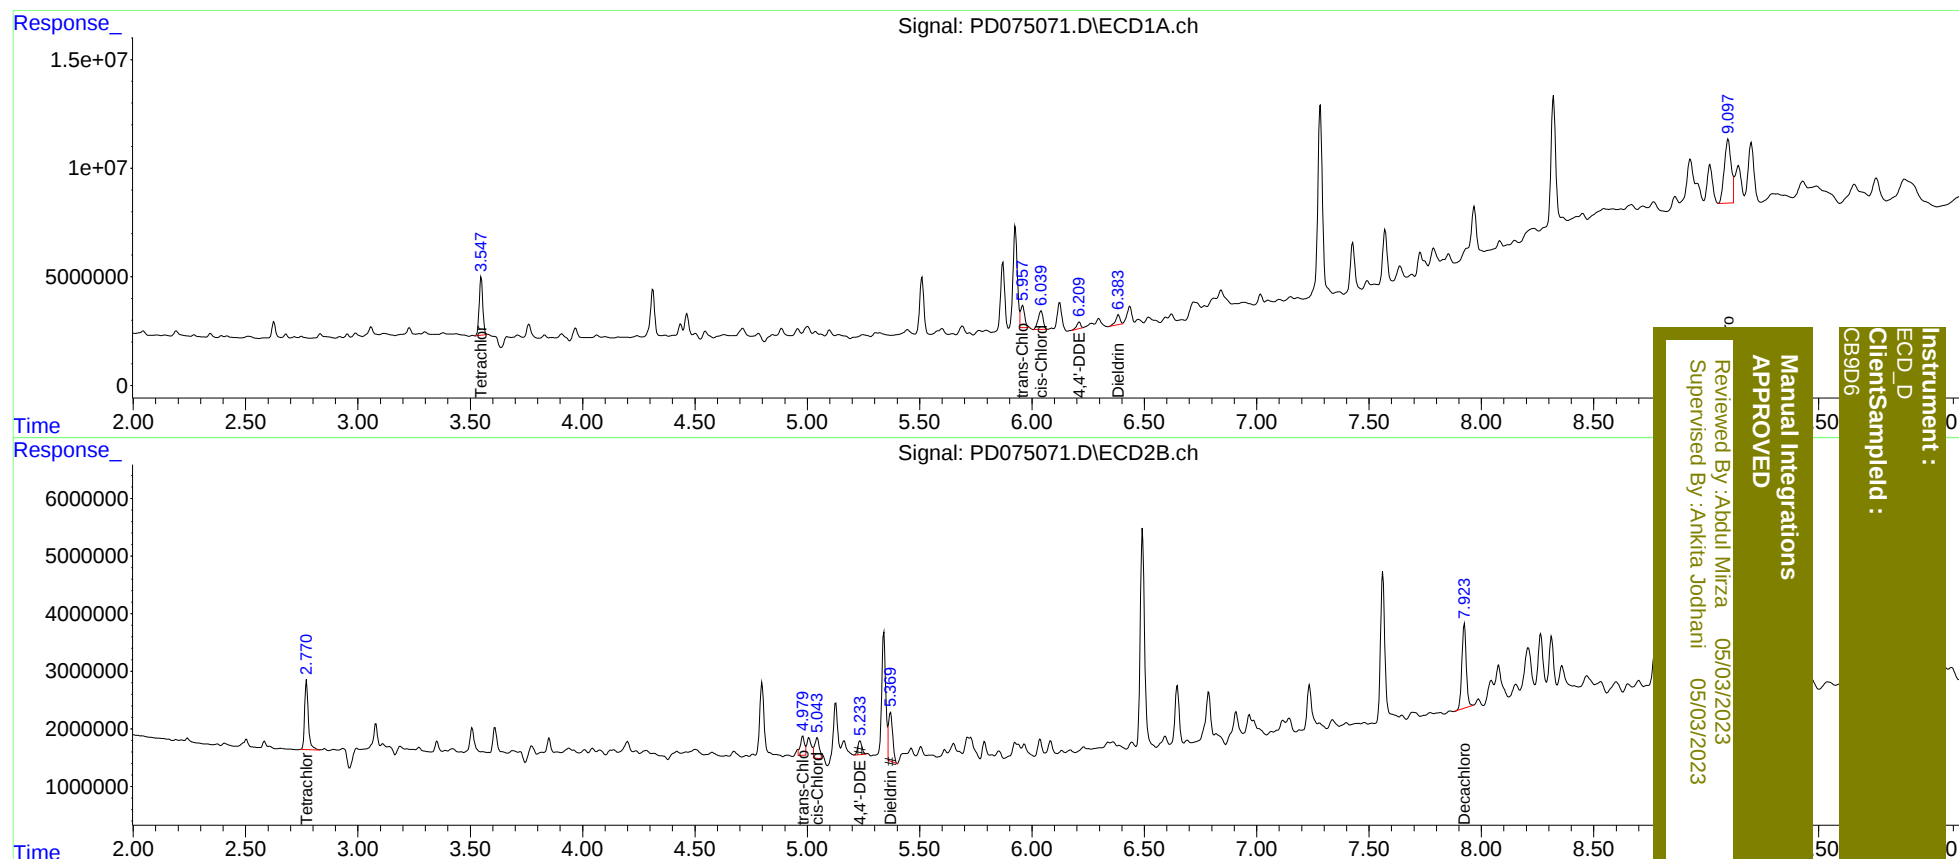

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/03/2023
Supervised By: Ankita Jodhani 05/03/2023

Instrument :
ECD_D
ClientSampled :
CB9D6