

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
 Data File : PD075087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 18:16
 Operator : AR\AJ
 Sample : 02419-28DL2 50X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW925DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/02/2023
 Supervised By : Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:27:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
7) B	delta-BHC	4.805	4.142	211.5E6	89943576	70.664m 63.940
14) MA	Endrin	6.594	5.608	258.0E6	109.5E6	95.252 99.082m
17) MA	4,4'-DDT	7.018	6.034	282.7E6	123.9E6	112.531m 124.878m


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050123\
Data File : PD075087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 18:16
Operator : AR\AJ
Sample : 02419-28DL2 50X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:27:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

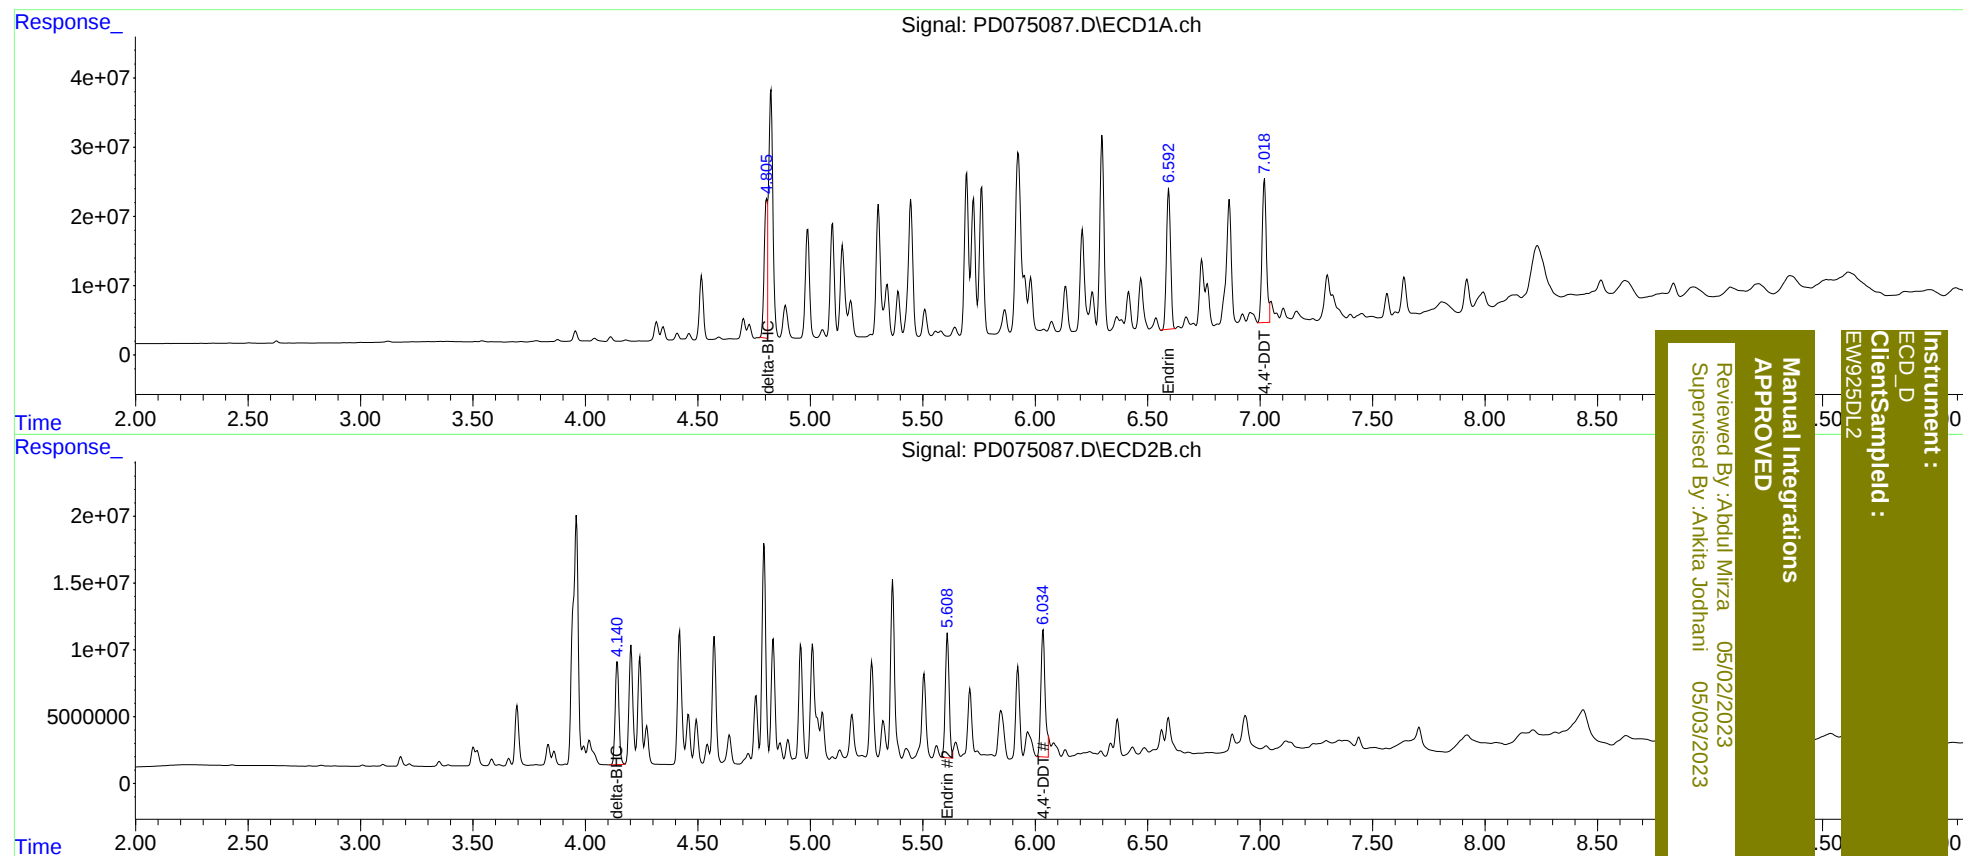

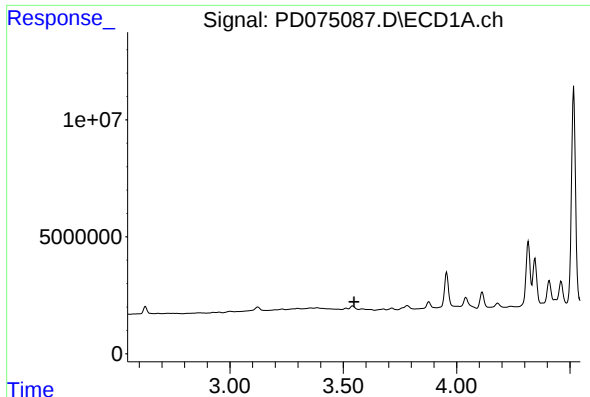


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EW925DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/03/2023

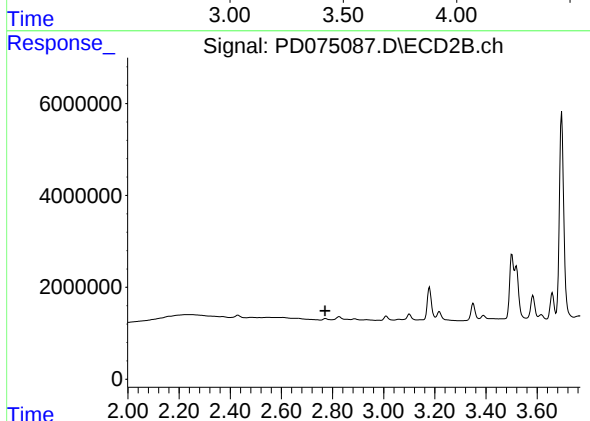


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.770 min
Response: 0
Conc: N.D.

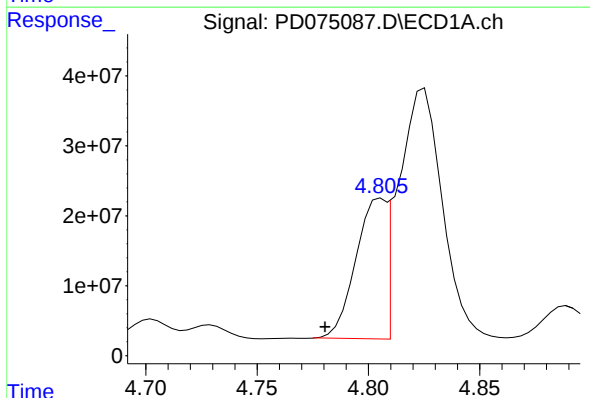


#7 delta-BHC

R.T.: 4.805 min
Delta R.T.: 0.024 min
Response: 211513137
Conc: 70.66 ng/ml m

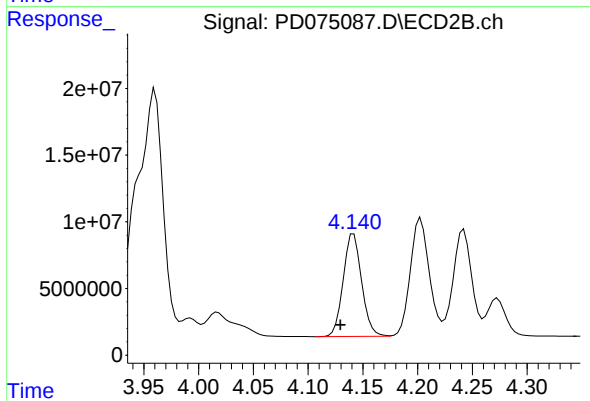

#7 delta-BHC

R.T.: 4.142 min
Delta R.T.: 0.012 min
Response: 89943576
Conc: 63.94 ng/ml

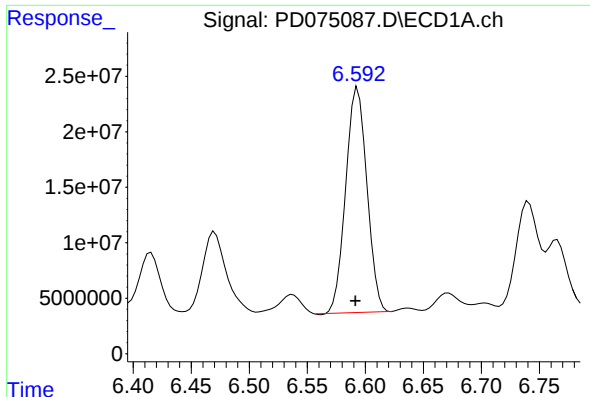


#14 Endrin

R.T.: 6.594 min
Delta R.T.: 0.002 min
Response: 258046523
Conc: 95.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW925DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/03/2023

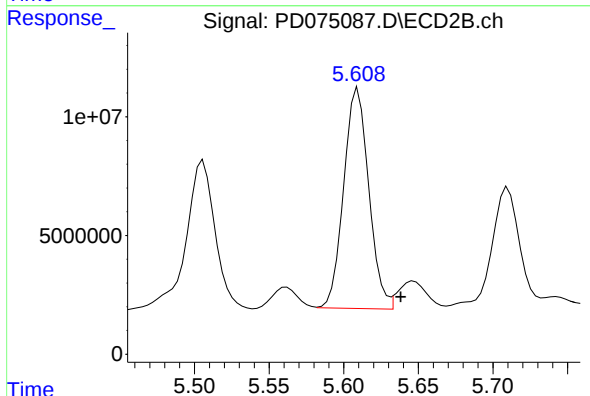


#14 Endrin

R.T.: 5.608 min
Delta R.T.: -0.030 min
Response: 109509517
Conc: 99.08 ng/ml m

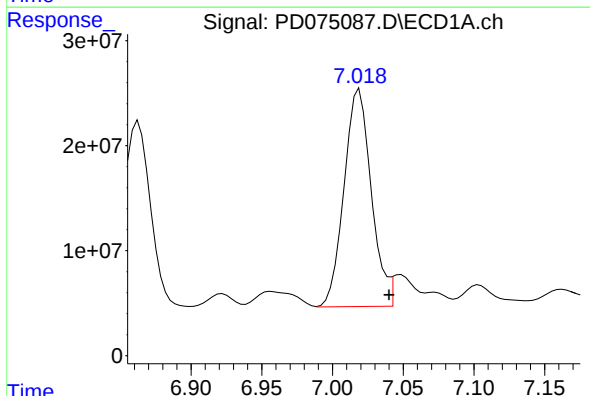


#17 4,4'-DDT

R.T.: 7.018 min
Delta R.T.: -0.022 min
Response: 282744508
Conc: 112.53 ng/ml m

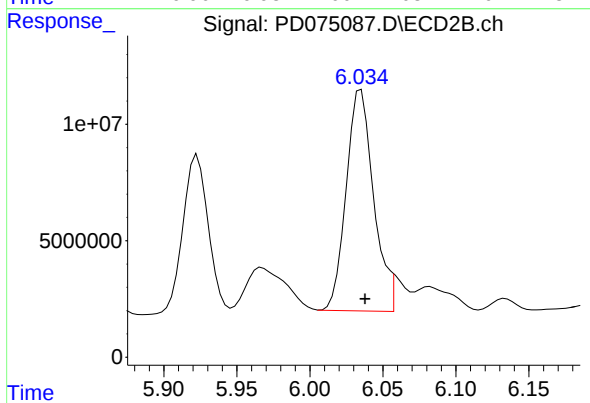

#17 4,4'-DDT

R.T.: 6.034 min
Delta R.T.: -0.004 min
Response: 123877991
Conc: 124.88 ng/ml m

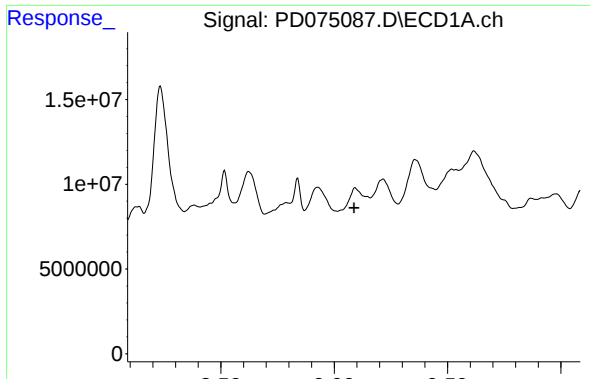


#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EW925DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/02/2023
Supervised By :Ankita Jodhani 05/03/2023

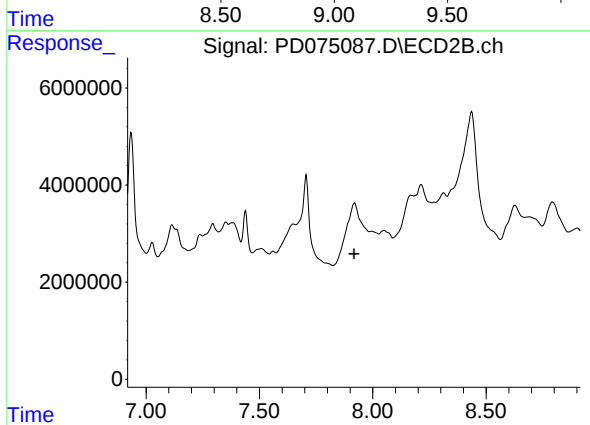

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.918 min
Response: 0
Conc: N.D.