

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050222\
 Data File : PD069364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 03:39
 Operator : AR\AJ
 Sample : N2562-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW468

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/03/2022
 Supervised By : mohammad ahmed 05/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 06:29:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.169	18580031	117.7E6	14.665	9.749m#
2)	SA Decachlor...	8.197	9.358	37254954	453.7E6	28.016	64.514m#
Target Compounds							
12)	B 4,4'-DDE	5.603	6.544	10883861	80388077	8.114m	7.389m
13)	MA Dieldrin	5.739	6.724	48256071	287.0E6	31.004	23.792m
16)	A 4,4'-DDD	6.123	7.036	12877203	217.3E6	10.562m	23.203m#
17)	MA 4,4'-DDT	6.365	7.342	4375534	50907208	3.567	5.655 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050222\
Data File : PD069364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 03:39
Operator : AR\AJ
Sample : N2562-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 06:29:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

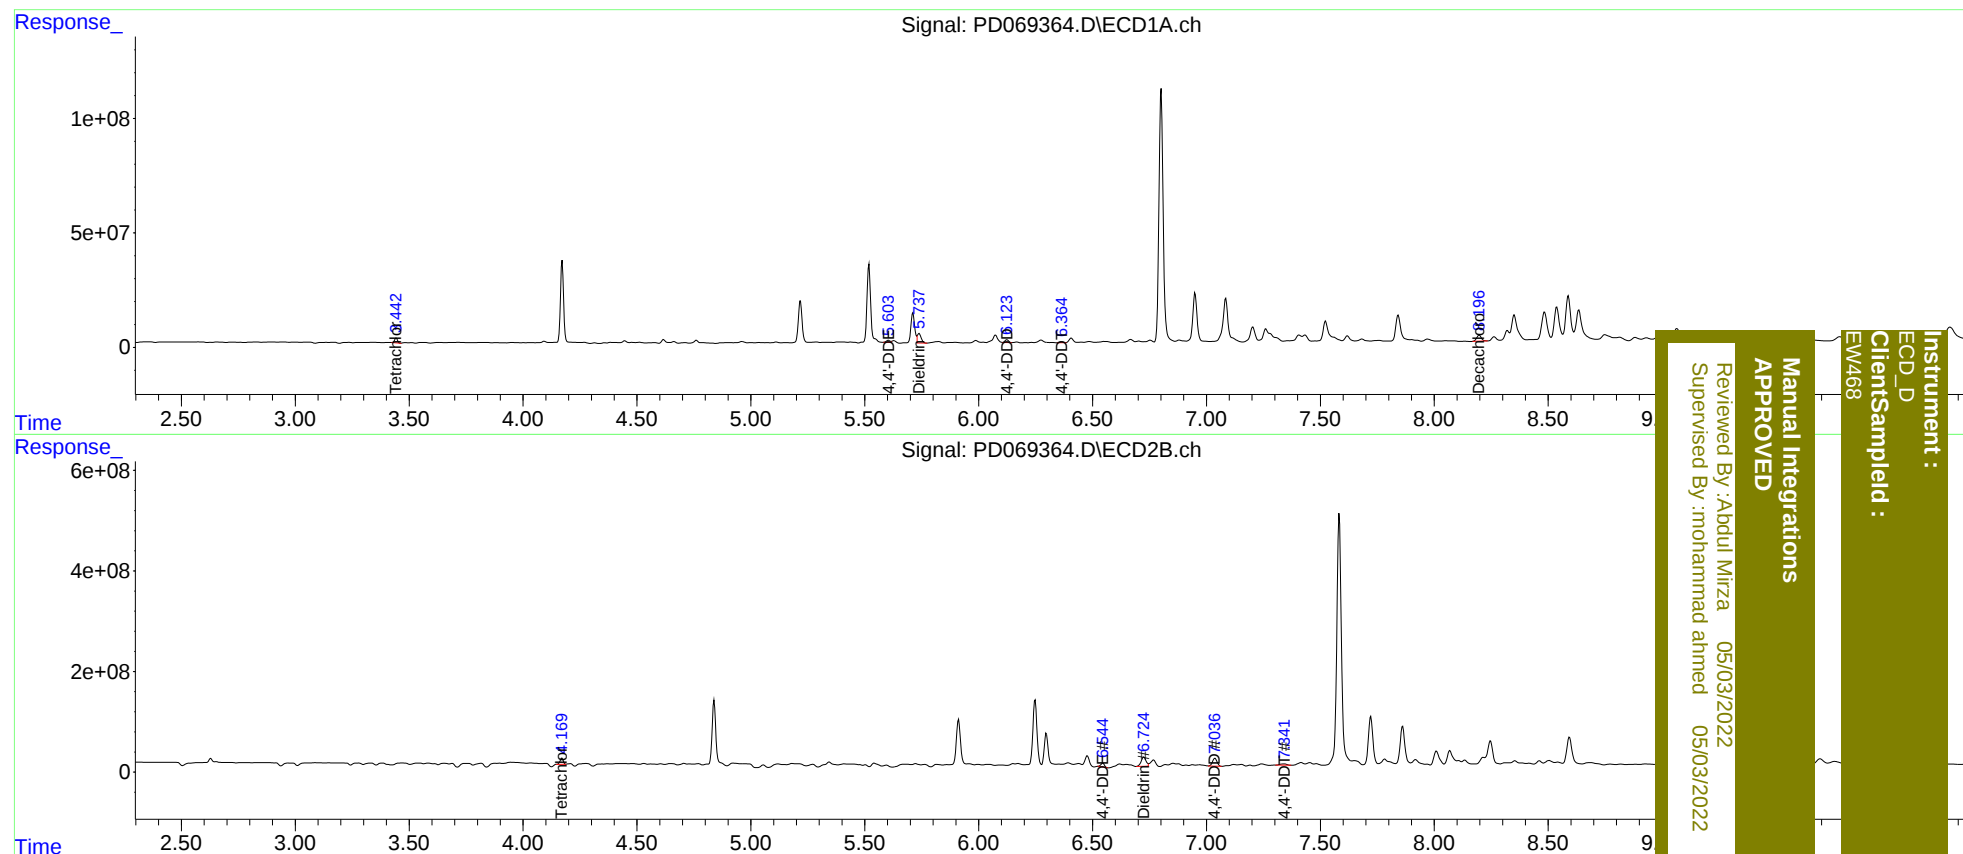

Reviewed By : Abdul Miza 05/03/2022
Supervised By : mohammad ahmed 05/03/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW/468