

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050222\
 Data File : PD069369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 04:48
 Operator : AR\AJ
 Sample : N2562-19MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW478MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/03/2022
 Supervised By : mohammad ahmed 05/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 06:31:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	16090830	163.3E6	12.700	13.532
27)	SA Decachlor...	8.196	9.365	32932294	152.0E6	24.765	21.616
Target Compounds							
2)	A alpha-BHC	3.883	4.567	89189844	713.4E6	49.897	43.399
3)	MA gamma-BHC...	4.166	4.858	85692549	676.0E6	47.375	43.390
4)	MA Heptachlor	4.463	5.384	82732278	650.0E6	48.728	42.936
5)	MB Aldrin	4.710	5.697	82286596	634.5E6	51.655	44.452
6)	B beta-BHC	4.416	5.021	37045527	291.4E6	47.827	43.435
7)	B delta-BHC	4.620	5.247	49150048	307.0E6	30.792	26.149
8)	B Heptachlo...	5.154	6.085	77546556	501.7E6	52.679	45.029
9)	A Endosulfan I	5.492	6.448	71612668	502.9E6	49.075	42.340
10)	B trans-Chl...	5.380	6.322	77490406	555.9E6	51.688	43.818
11)	B cis-Chlor...	5.438	6.396	75992342	541.0E6	50.911	43.436
12)	B 4,4'-DDE	5.604	6.547	153.5E6	1020.0E6	114.413	93.758
13)	MA Dieldrin	5.736	6.706	160.0E6	1056.4E6	102.822	87.581
14)	MA Endrin	5.994	6.926	143.5E6	839.5E6	102.593	86.326
15)	B Endosulfa...	6.268	7.130	130.3E6	806.6E6	101.142	84.161m
16)	A 4,4'-DDD	6.121	7.037	121.8E6	863.8E6	99.926	92.250
17)	MA 4,4'-DDT	6.361	7.341	122.3E6	781.8E6	99.682	86.848
18)	B Endrin al...	6.437	7.256	104.1E6	645.3E6	104.841	90.325
19)	B Endosulfa...	6.649	7.481	115.2E6	698.2E6	91.969	79.569
20)	A Methoxychlor	6.912	7.794	315.9E6	1740.6E6	465.463	422.376
21)	B Endrin ke...	7.143	7.955	147.5E6	805.1E6	102.114	87.211

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050222\
Data File : PD069369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 04:48
Operator : AR\AJ
Sample : N2562-19MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 06:31:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

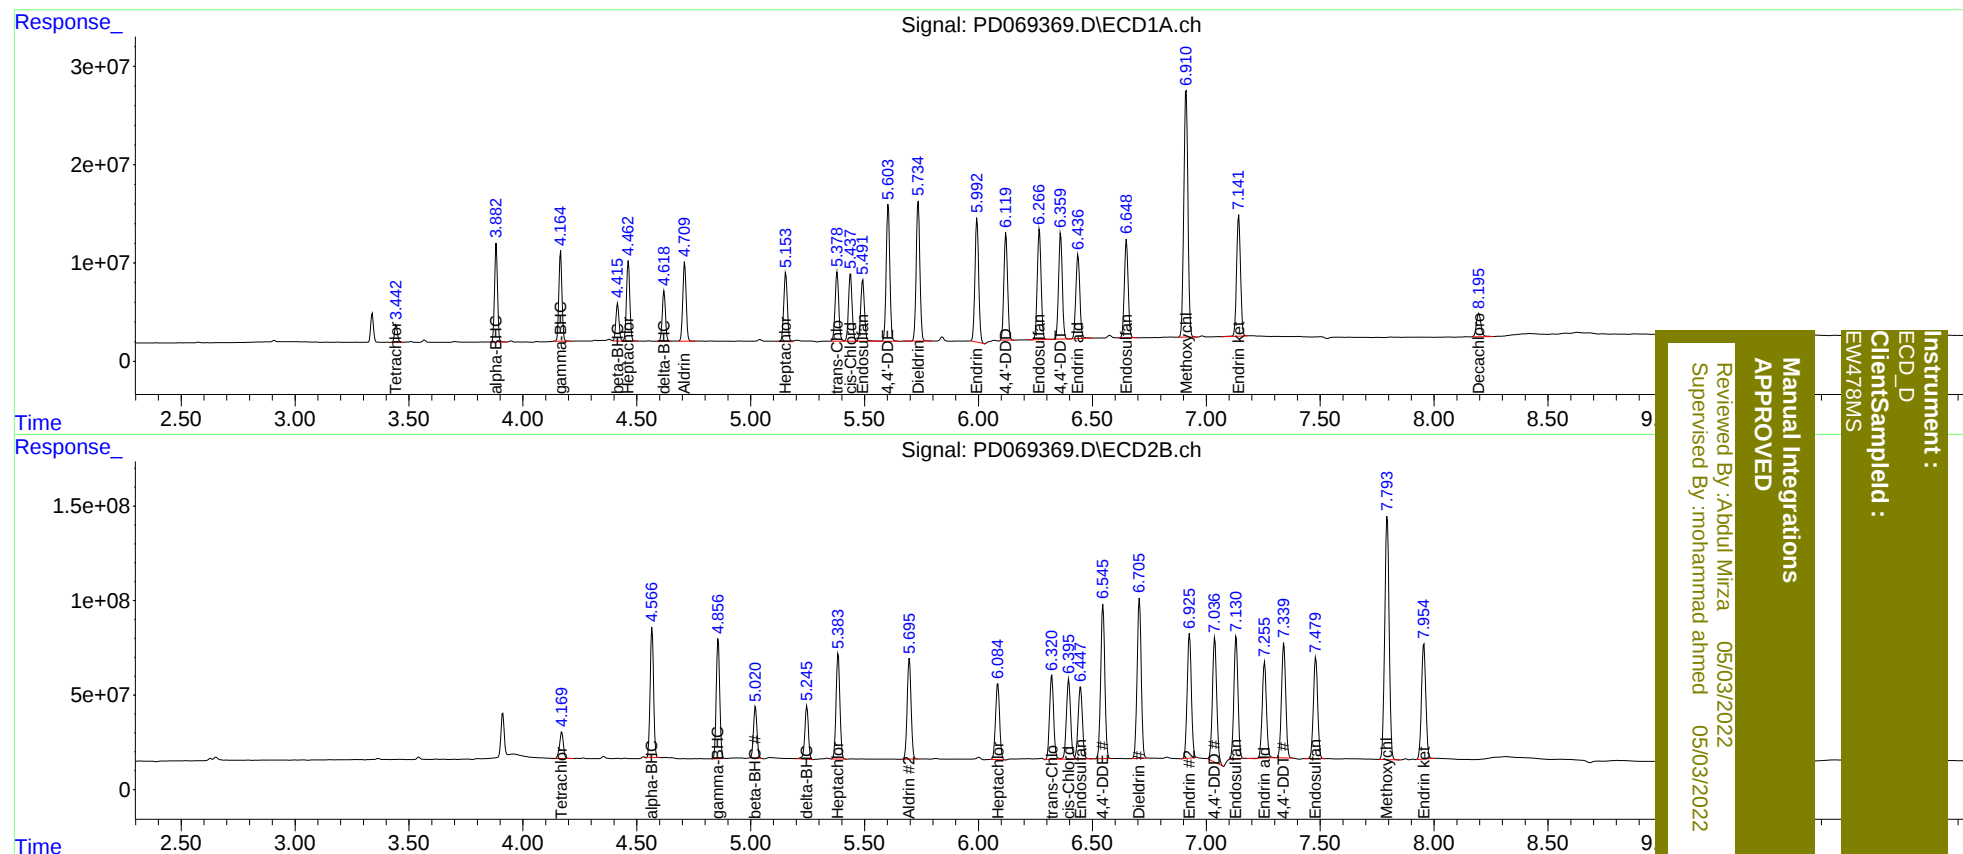

Reviewed By: Abdul Miza 05/03/2022
Supervised By: mohammad ahmed 05/03/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW/478MS