

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050222\
 Data File : PD069370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 05:02
 Operator : AR\AJ
 Sample : N2562-20MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW478MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/03/2022
 Supervised By : mohammad ahmed 05/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 06:31:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.171	16624159	168.8E6	13.121	13.989
27)	SA Decachlor...	8.197	9.365	29925262	143.5E6	22.504	20.401
Target Compounds							
2)	A alpha-BHC	3.882	4.567	92484914	742.0E6	51.740	45.137
3)	MA gamma-BHC...	4.166	4.858	88768867	696.1E6	49.076	44.678
4)	MA Heptachlor	4.463	5.385	86445498	673.7E6	50.915	44.500
5)	MB Aldrin	4.710	5.697	87153304	653.4E6	54.711	45.771
6)	B beta-BHC	4.416	5.021	38419033	300.3E6	49.600	44.762
7)	B delta-BHC	4.620	5.247	51923008	314.7E6	32.529	26.807
8)	B Heptachlo...	5.154	6.085	81260984	525.7E6	55.202	47.189
9)	A Endosulfan I	5.493	6.448	74971603	523.3E6	51.377	44.059
10)	B trans-Chl...	5.380	6.322	80634516	574.3E6	53.786	45.266
11)	B cis-Chlor...	5.438	6.396	79253910	562.2E6	53.096	45.137
12)	B 4,4'-DDE	5.604	6.546	158.6E6	1050.2E6	118.248	96.532
13)	MA Dieldrin	5.736	6.706	166.0E6	1091.7E6	106.641	90.506
14)	MA Endrin	5.994	6.926	149.3E6	866.9E6	106.707	89.143
15)	B Endosulfa...	6.269	7.130	136.2E6	828.0E6	105.673	86.396m
16)	A 4,4'-DDD	6.121	7.037	127.8E6	895.5E6	104.853	95.634
17)	MA 4,4'-DDT	6.361	7.340	128.5E6	811.5E6	104.770	90.148
18)	B Endrin al...	6.438	7.255	108.8E6	670.0E6	109.575	93.780
19)	B Endosulfa...	6.650	7.480	120.5E6	725.6E6	96.154	82.692
20)	A Methoxychlor	6.912	7.794	330.2E6	1796.2E6	486.540	435.859
21)	B Endrin ke...	7.143	7.955	155.0E6	833.5E6	107.320	90.283

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050222\
Data File : PD069370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 05:02
Operator : AR\AJ
Sample : N2562-20MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 06:31:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

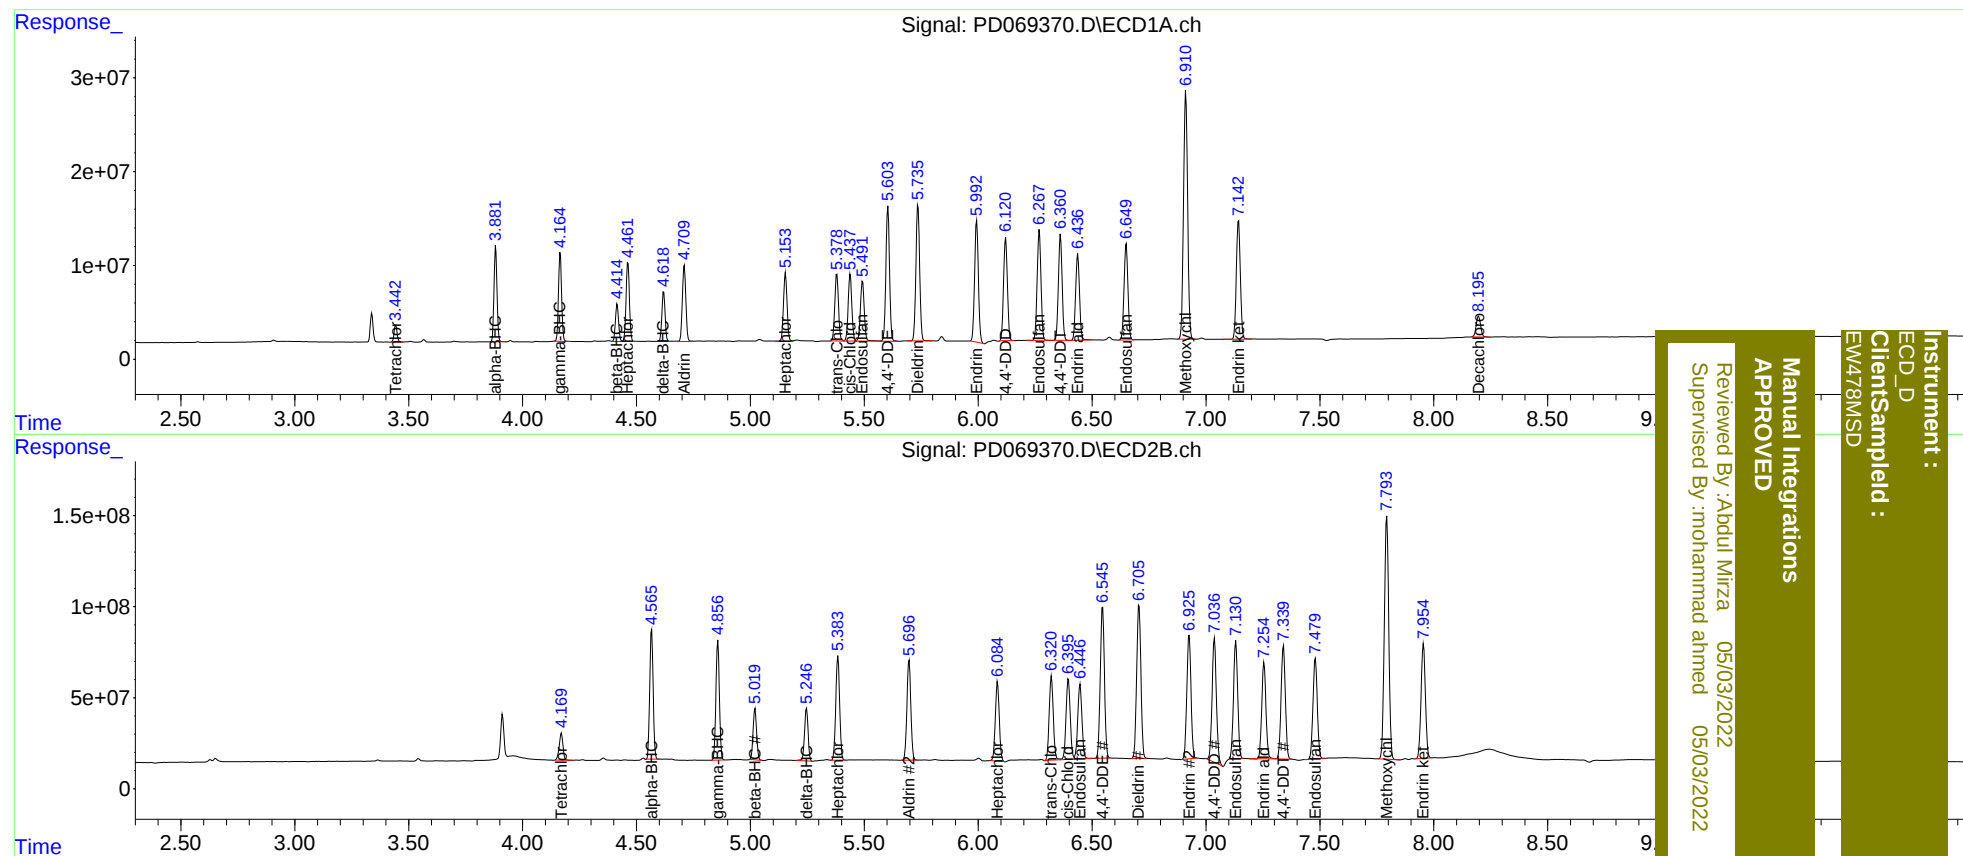

Reviewed By: Abdul Miza 05/03/2022
Supervised By: mohammad ahmed 05/03/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW478MSD