

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
 Data File : PD075123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 17:18
 Operator : AR\AJ
 Sample : 02447-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:54:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.771	33803267	11261875	15.133	10.863 #
27)	SA Decachlor...	9.094	7.922	266.6E6	388.8E6	111.602	404.760 #
Target Compounds							
2)	A alpha-BHC	4.041f	0.000	61447822	0	16.744	N.D. #
4)	MA Heptachlor	4.887f	3.960	129.4E6	2154.0E6	37.342	1544.368 #
5)	MB Aldrin	5.268	4.242	-2062402	753.6E6	N.D.	573.077
6)	B beta-BHC	4.515	3.860f	558.8E6	54198021	379.077	79.639 #
7)	B delta-BHC	4.824f	4.142	1678.9E6	736.7E6	560.891	523.705
8)	B Heptachlo...	5.695	4.724	2722.3E6	40121341	906.459	32.678 #
9)	A Endosulfan I	6.072	5.098	169.3E6	1435038	58.137	1.258 #
10)	B trans-Chl...	5.951	4.958	-600455459	424.9E6	N.D.	350.753
11)	B cis-Chlor...	6.035	5.054	201.3E6	379.4E6	64.572	306.448 #
12)	B 4,4'-DDE	6.209	5.234	684.4E6	70702349	233.000	62.504 #
13)	MA Dieldrin	6.364	5.367	237.5E6	1528.8E6	74.726	1217.961 #
14)	MA Endrin	6.593	5.648	2366.5E6	160.5E6	873.526	145.188 #
15)	B Endosulfa...	6.809	5.923	180.8E6	710.5E6	62.408	651.372 #
16)	A 4,4'-DDD	6.739	5.787	492.0E6	28707795	203.473	29.713 #
17)	MA 4,4'-DDT	7.045	6.036	741.3E6	946.6E6	295.019	954.196 #
18)	B Endrin al...	6.954	6.133	300.7E6	-22871723	134.364	N.D. #
19)	B Endosulfa...	7.159	6.335	732.4E6	600.7E6	280.918	584.276 #
20)	A Methoxychlor	7.491	6.593	204.5E6	1308.4E6	141.877	2368.679 #
22)	Toxaphene-1	6.254	5.010	411.8E6	1064.2E6	18442.259	161166.695 #
23)	Toxaphene-2	6.470	5.681	909.6E6	97761	32829.113	13.375 #
24)	Toxaphene-3	6.670	5.983	122.6E6	167.9E6	6415.390	20009.659 #
25)	Toxaphene-4	7.159	6.593	732.4E6	1308.4E6	12026.753	53315.935 #
26)	Toxaphene-5	7.640f	6.687f	3707.9E6	200.1E6	83371.356	6004.414 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
Data File : PD075123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 17:18
Operator : AR\AJ
Sample : 02447-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:54:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

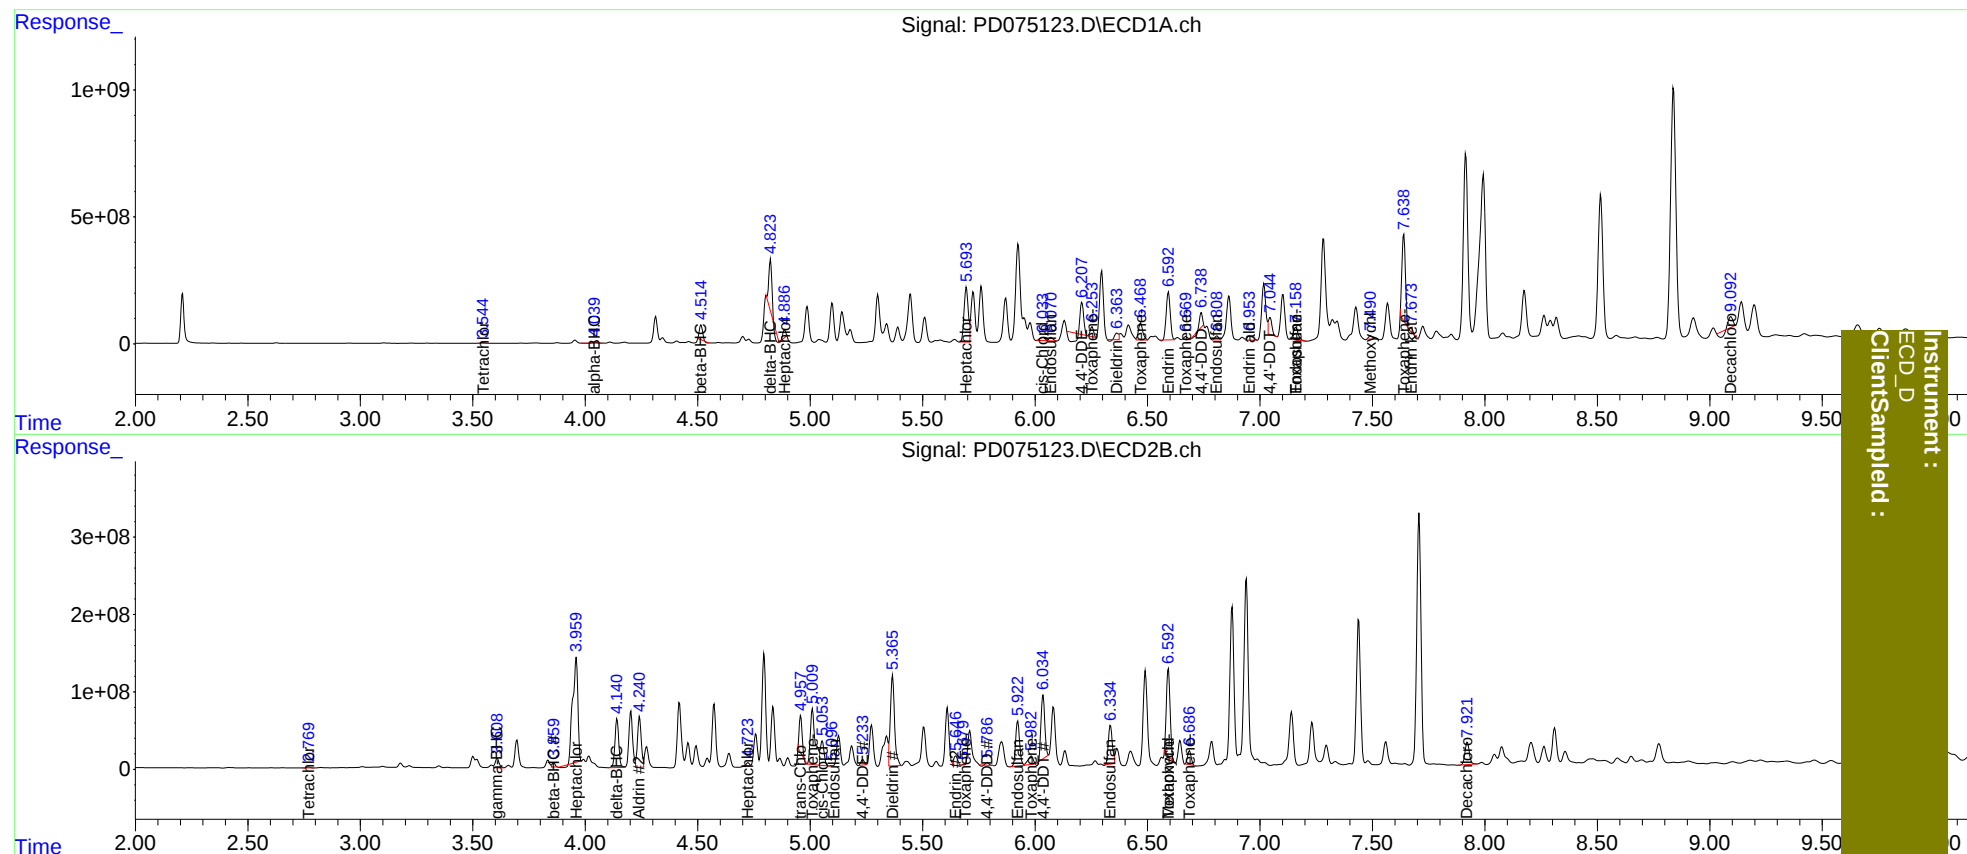

Instrument :
ECD_D
Client Sampled :