

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
 Data File : PD075102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 10:52
 Operator : AR\AJ
 Sample : 02419-28DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW925DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/04/2023
 Supervised By : Ankita Jodhani 05/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:49:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.770	18547651	3054556	8.303m	2.946m#
2) SA Decachlor...	9.092	7.919	50202098	21843001	21.019m	22.739
Target Compounds						
7) B delta-BHC	4.803	4.141	1756.7E6	742.5E6	586.883m	527.866
14) MA Endrin	6.591	5.607	2375.1E6	890.8E6	876.706	805.978m
17) MA 4,4'-DDT	7.015	6.032	2545.6E6	977.3E6	1013.137m	985.185m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
Data File : PD075102.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 10:52
Operator : AR\AJ
Sample : 02419-28DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:49:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

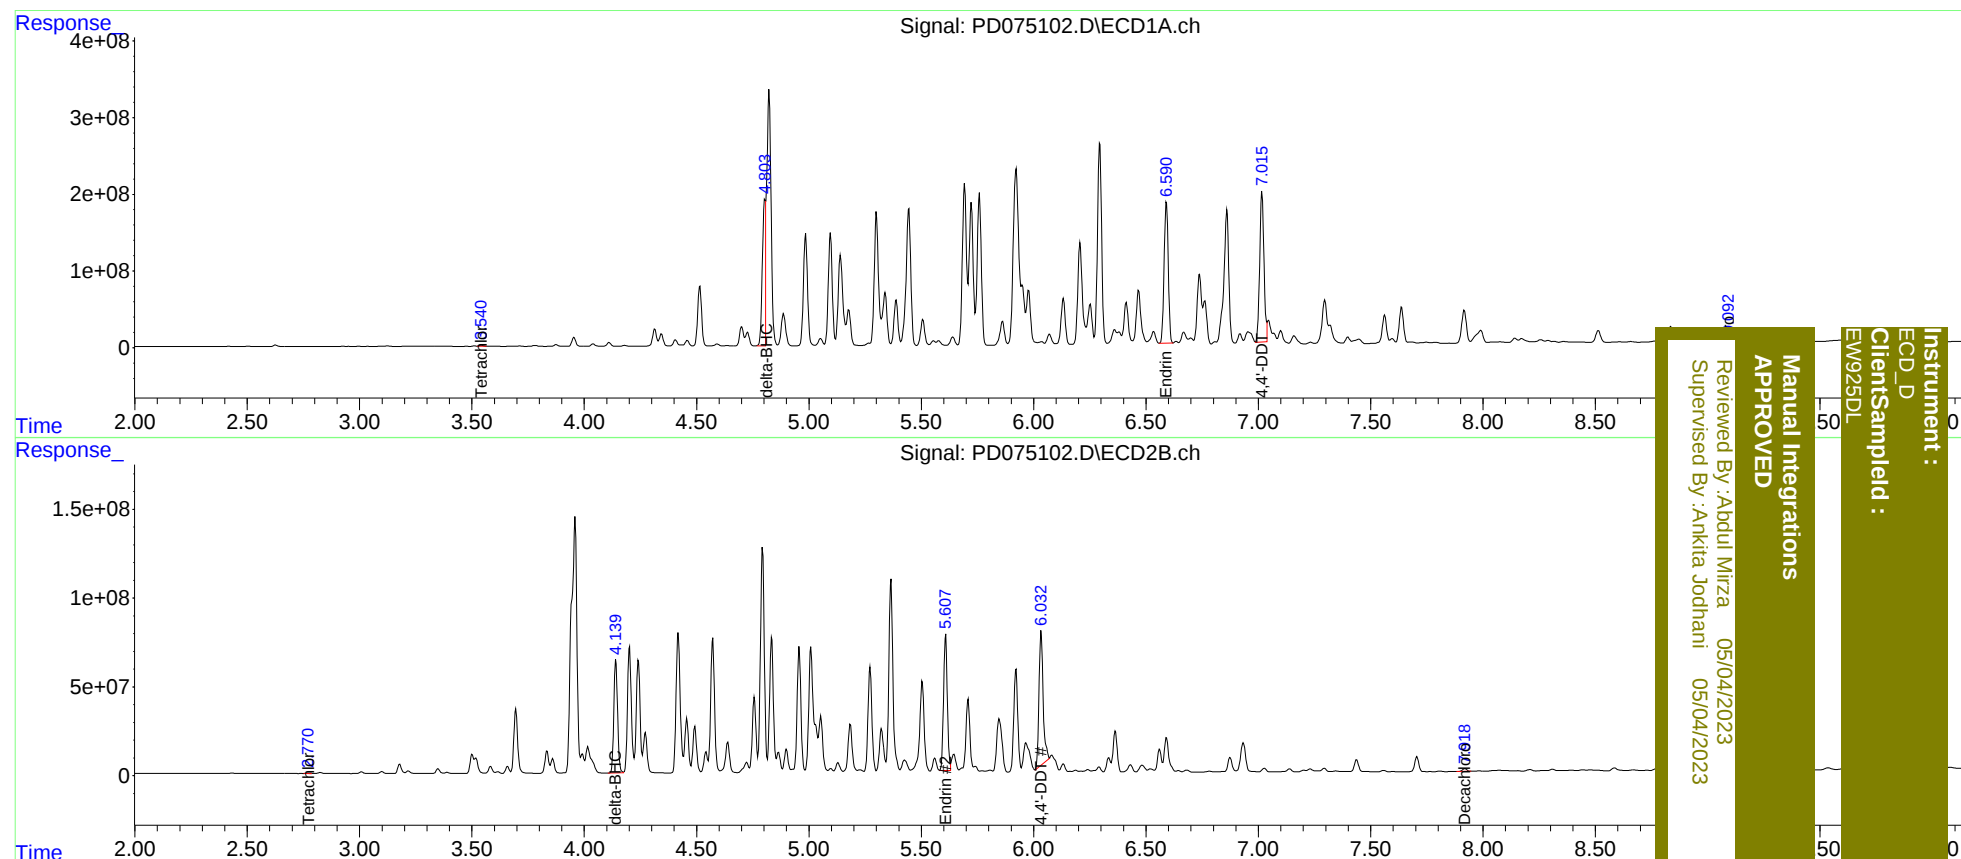

Reviewed By: Abdul Mirza 05/04/2023
Supervised By: Ankita Jodhani 05/04/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW925DL