

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
 Data File : PD075129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 19:59
 Operator : AR\AJ
 Sample : 02447-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW933

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/04/2023
 Supervised By : Ankita Jodhani 05/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:56:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.788	44328722	11702740	19.845	11.289 #
2) SA Decachlor...	9.082	7.933	141.0E6	65725009	59.017m	68.420m
Target Compounds						
3) MA gamma-BHC...	4.343	3.600	291.5E6	71516844	85.271m	51.395 #
14) MA Endrin	6.593	5.626	3250.7E6	1203.8E6	1199.925	1089.204
17) MA 4,4'-DDT	7.017	6.050	3587.1E6	1227.0E6	1427.655m	1236.931m
19) B Endosulfa...	7.160	6.351	270.8E6	146.5E6	103.872	142.477m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
Data File : PD075129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 19:59
Operator : AR\AJ
Sample : 02447-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:56:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

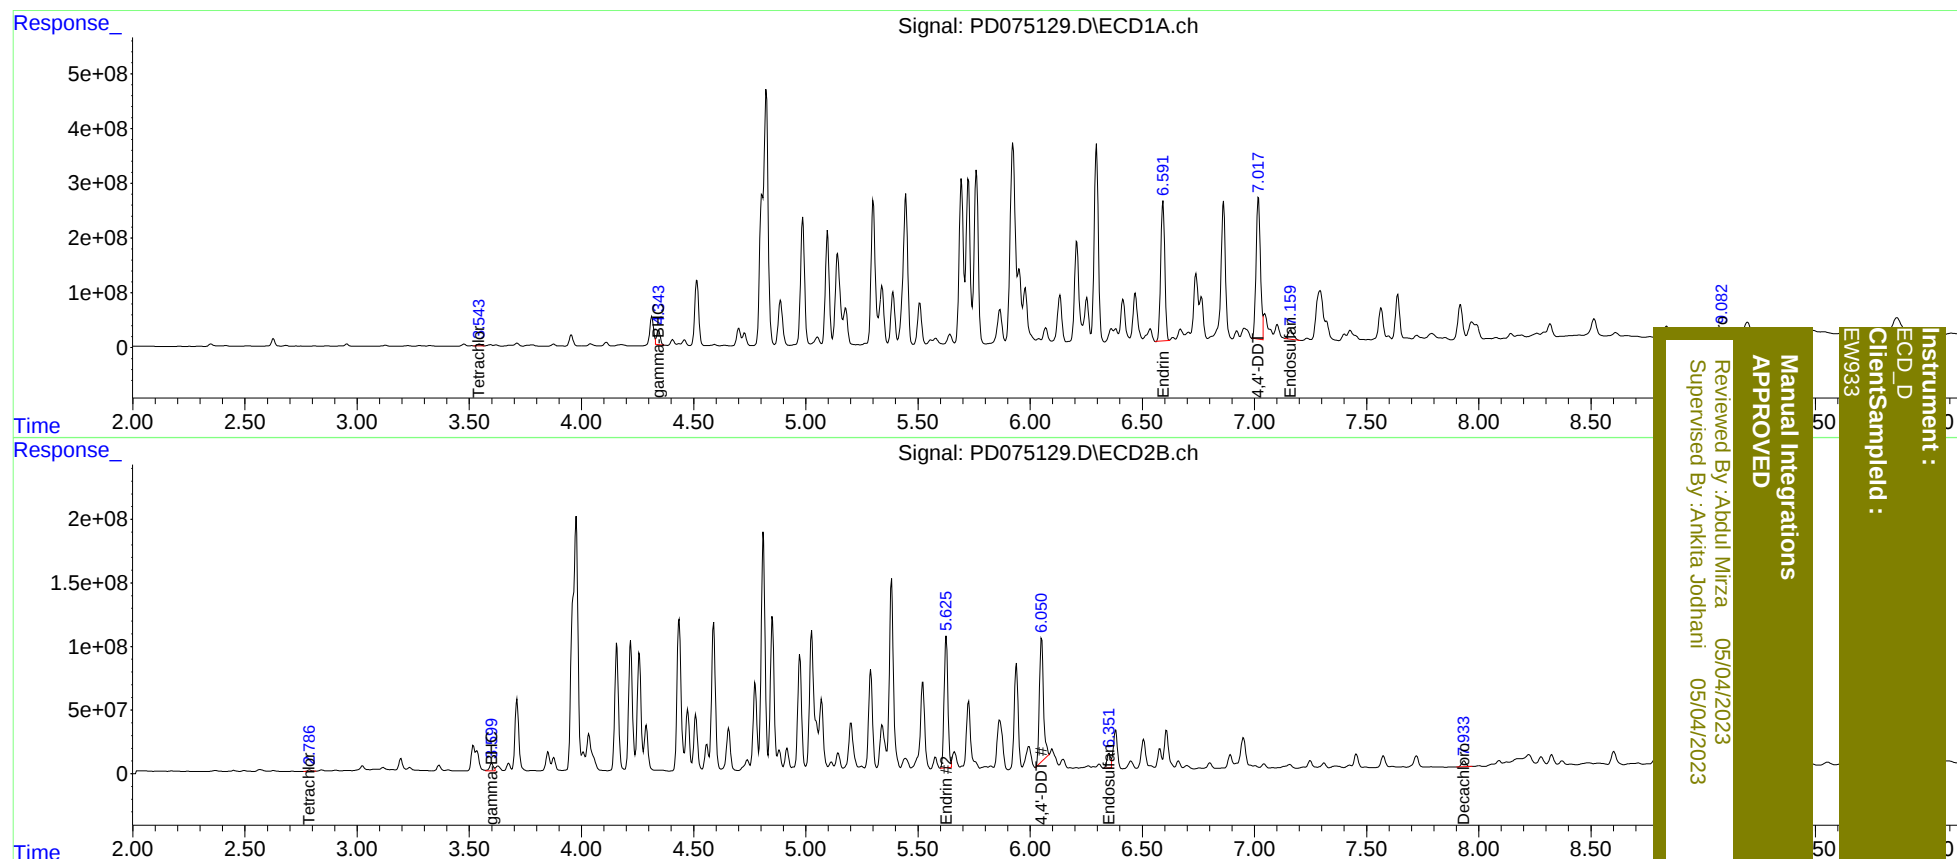

Reviewed By: Abdul Mirza 05/04/2023
Supervised By: Ankita Jodhani 05/04/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW/933