

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
 Data File : PD075135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 22:41
 Operator : AR\AJ
 Sample : 02447-19MSD
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW937MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/04/2023
 Supervised By : Ankita Jodhani 05/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:57:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.549	2.771	28317019	17645421	12.677	17.021 #
2) SA Decachlor...	9.083	7.916	871.6E6	55721832	364.932m	58.007m#
Target Compounds						
2) A alpha-BHC	4.005	3.274	145.6E6	56953772	39.669	39.552
3) MA gamma-BHC...	4.334	3.607	126.2E6	467.3E6	36.908m	335.799m#
4) MA Heptachlor	4.930	3.943	141.3E6	136.2E6	40.799m	97.661m#
5) MB Aldrin	5.274	4.227	167.6E6	82609860	50.043	62.822 #
6) B beta-BHC	4.534	3.901	37584851	16732141	25.498	24.586
7) B delta-BHC	4.784	4.130	167.0E6	129.7E6	55.800m	92.185 #
8) B Heptachlo...	5.699	4.728	252.5E6	36442213	84.091	29.681 #
9) A Endosulfan I	6.089	5.099	195.3E6	42531167	67.056m	37.276m#
10) B trans-Chl...	5.957	4.980	306.2E6	84098679	102.282m	69.420m#
11) B cis-Chlor...	6.033	5.046	656.9E6	99610392	210.747	80.450 #
12) B 4,4'-DDE	6.210	5.235	490.2E6	181.1E6	166.870m	160.081
13) MA Dieldrin	6.366	5.370	542.9E6	495.9E6	170.795m	395.057 #
14) MA Endrin	6.597	5.641	645.0E6	183.4E6	238.099m	165.971 #
15) B Endosulfa...	6.813	5.937	392.2E6	221.1E6	135.412m	202.654 #
16) A 4,4'-DDD	6.725	5.787	691.5E6	149.1E6	285.958	154.312m#
17) MA 4,4'-DDT	7.044	6.040	1162.3E6	332.7E6	462.589m	335.391 #
18) B Endrin al...	6.946	6.114	294.0E6	57883602	131.369	65.175m#
19) B Endosulfa...	7.181	6.339	355.8E6	138.9E6	136.478	135.054m
20) A Methoxychlor	7.521	6.617	594.7E6	160.9E6	412.510	291.213m#
21) B Endrin ke...	7.667	6.843	214.2E6	84299311	74.021m	70.697m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
Data File : PD075135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 22:41
Operator : AR\AJ
Sample : 02447-19MSD
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:57:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

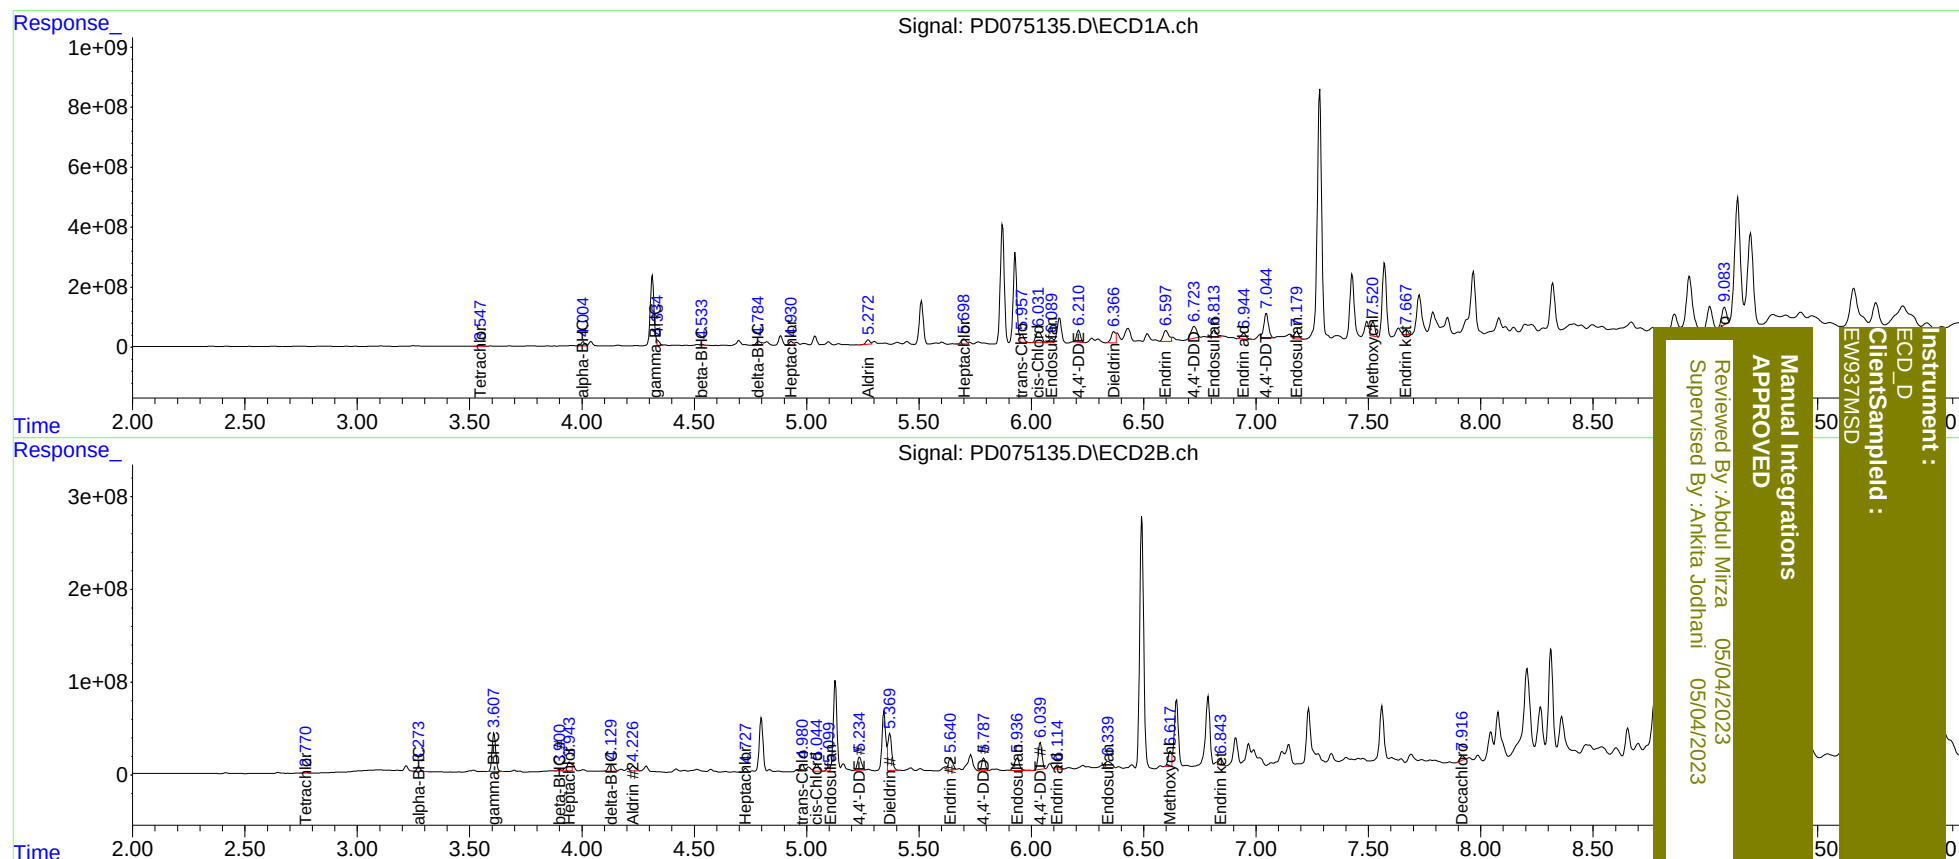

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/04/2023
Supervised By: Ankita Jodhani 05/04/2023

Instrument :
ECD_D
Client Sampled :
EW937MSD