

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
 Data File : PD075134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 22:14
 Operator : AR\AJ
 Sample : 02447-18MS
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW937MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/04/2023
 Supervised By :Ankita Jodhani 05/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:57:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.771	28481351	17495799	12.750	16.877 #
2) SA Decachlor...	9.079	7.916	860.5E6	59220784	360.285m	61.649m#
Target Compounds						
2) A alpha-BHC	4.005	3.274	146.6E6	56450345	39.937	39.203
3) MA gamma-BHC...	4.334	3.607	130.0E6	474.1E6	38.014m	340.698m#
4) MA Heptachlor	4.930	3.943	135.0E6	137.3E6	38.971m	98.432m#
5) MB Aldrin	5.274	4.227	165.5E6	82395827	49.423	62.660 #
6) B beta-BHC	4.534	3.901	38128574	16367623	25.867	24.051
7) B delta-BHC	4.784	4.130	177.0E6	130.5E6	59.141m	92.761 #
8) B Heptachlo...	5.699	4.728	254.2E6	36228647	84.655	29.507 #
9) A Endosulfan I	6.088	5.100	164.1E6	47477608	56.347m	41.611m#
10) B trans-Chl...	5.956	4.979	329.1E6	94566379	109.935m	78.061m#
11) B cis-Chlor...	6.032	5.045	649.4E6	99325267	208.321	80.220 #
12) B 4,4'-DDE	6.209	5.235	491.1E6	181.3E6	167.176m	160.291
13) MA Dieldrin	6.366	5.369	563.9E6	506.3E6	177.420m	403.343 #
14) MA Endrin	6.596	5.641	637.8E6	187.4E6	235.428m	169.512 #
15) B Endosulfa...	6.812	5.937	405.7E6	219.1E6	140.063m	200.886 #
16) A 4,4'-DDD	6.725	5.786	685.6E6	150.0E6	283.505	155.282m#
17) MA 4,4'-DDT	7.045	6.040	1334.8E6	342.2E6	531.262	344.933 #
18) B Endrin al...	6.945	6.114	287.1E6	58118878	128.261	65.440m#
19) B Endosulfa...	7.180	6.338	357.1E6	139.4E6	136.961	135.624m
20) A Methoxychlor	7.521	6.617	617.1E6	204.4E6	428.012	370.038m
21) B Endrin ke...	7.666	6.843	214.0E6	87319628	73.972m	73.230m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050223\
Data File : PD075134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 22:14
Operator : AR\AJ
Sample : 02447-18MS
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:57:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

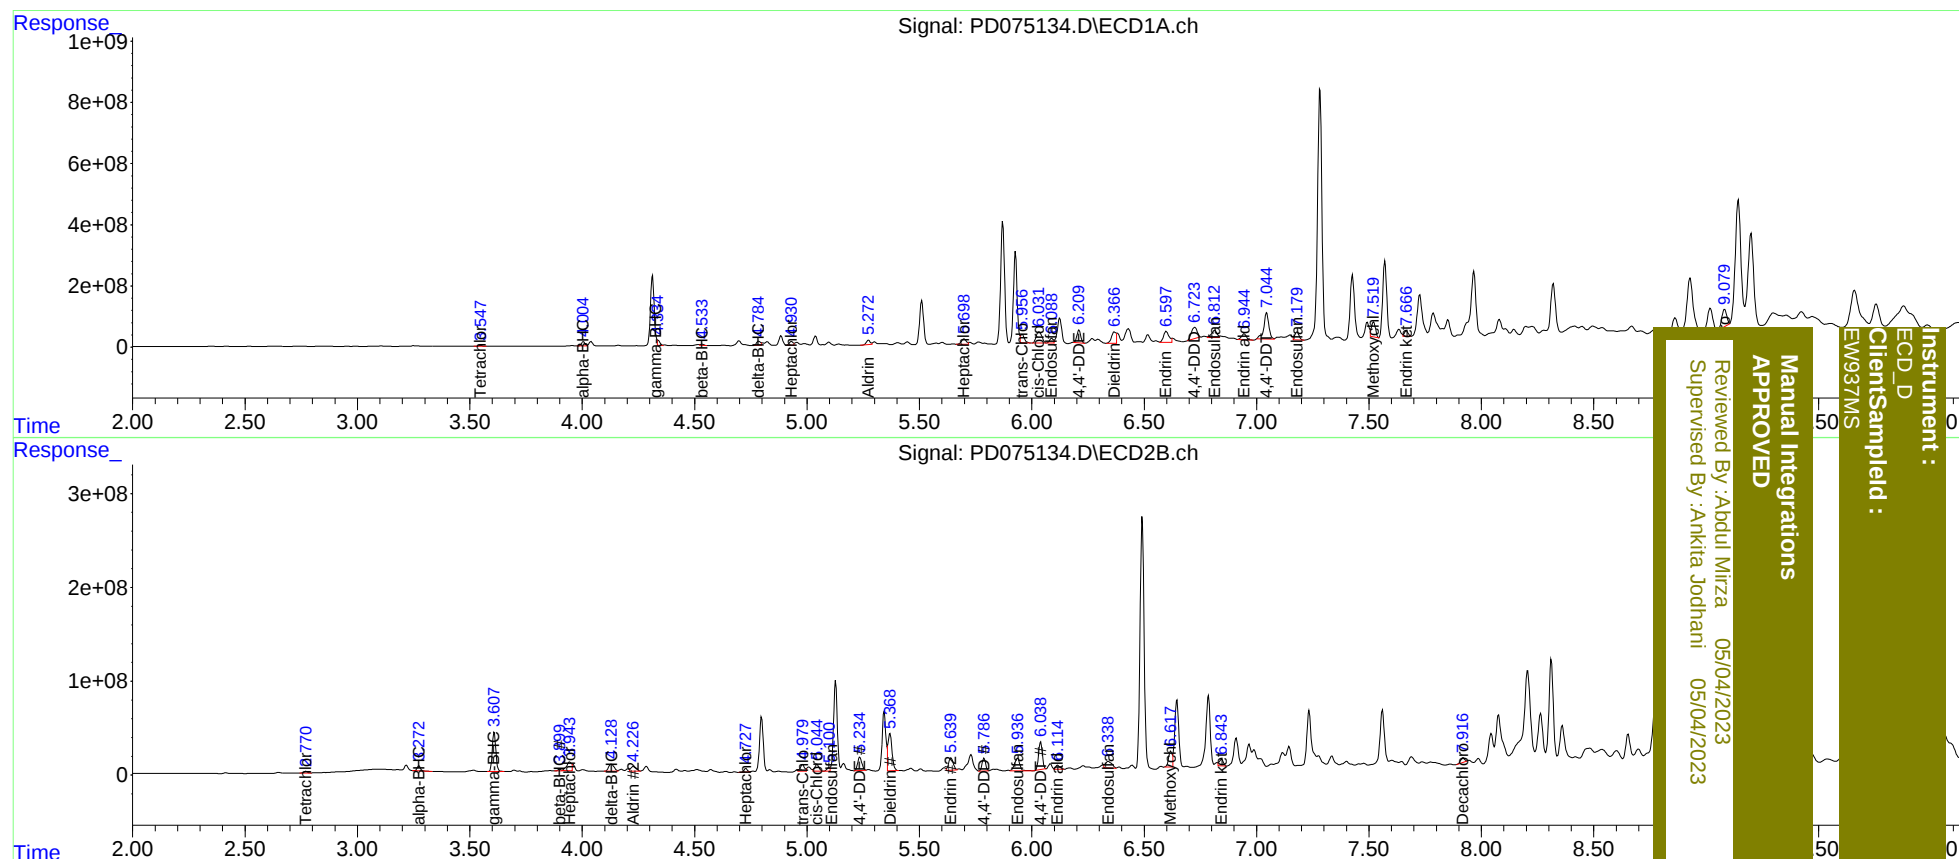

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/04/2023
Supervised By: Ankita Jodhani 05/04/2023

Instrument :
ECD_D
Client Sampled :
EW937MS