

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050224\
 Data File : PD082692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2024 15:13
 Operator : AR\AJ
 Sample : P2238-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 21:06:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 16:11:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.795	17700175	42356192	12.517	12.103
2)	SA Decachlor...	9.120	7.926	21176883	41595012	10.868	11.022m
Target Compounds							
11)	B cis-Chlor...	6.044	5.023	926056	3584099	0.434m	0.742m#
14)	MA Endrin	6.609	5.622	1131523	2191409	0.619m	0.518
17)	MA 4,4'-DDT	7.031	6.039	2005296	3527715	1.247	0.938

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050224\
Data File : PD082692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2024 15:13
Operator : AR\AJ
Sample : P2238-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 21:06:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 16:11:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

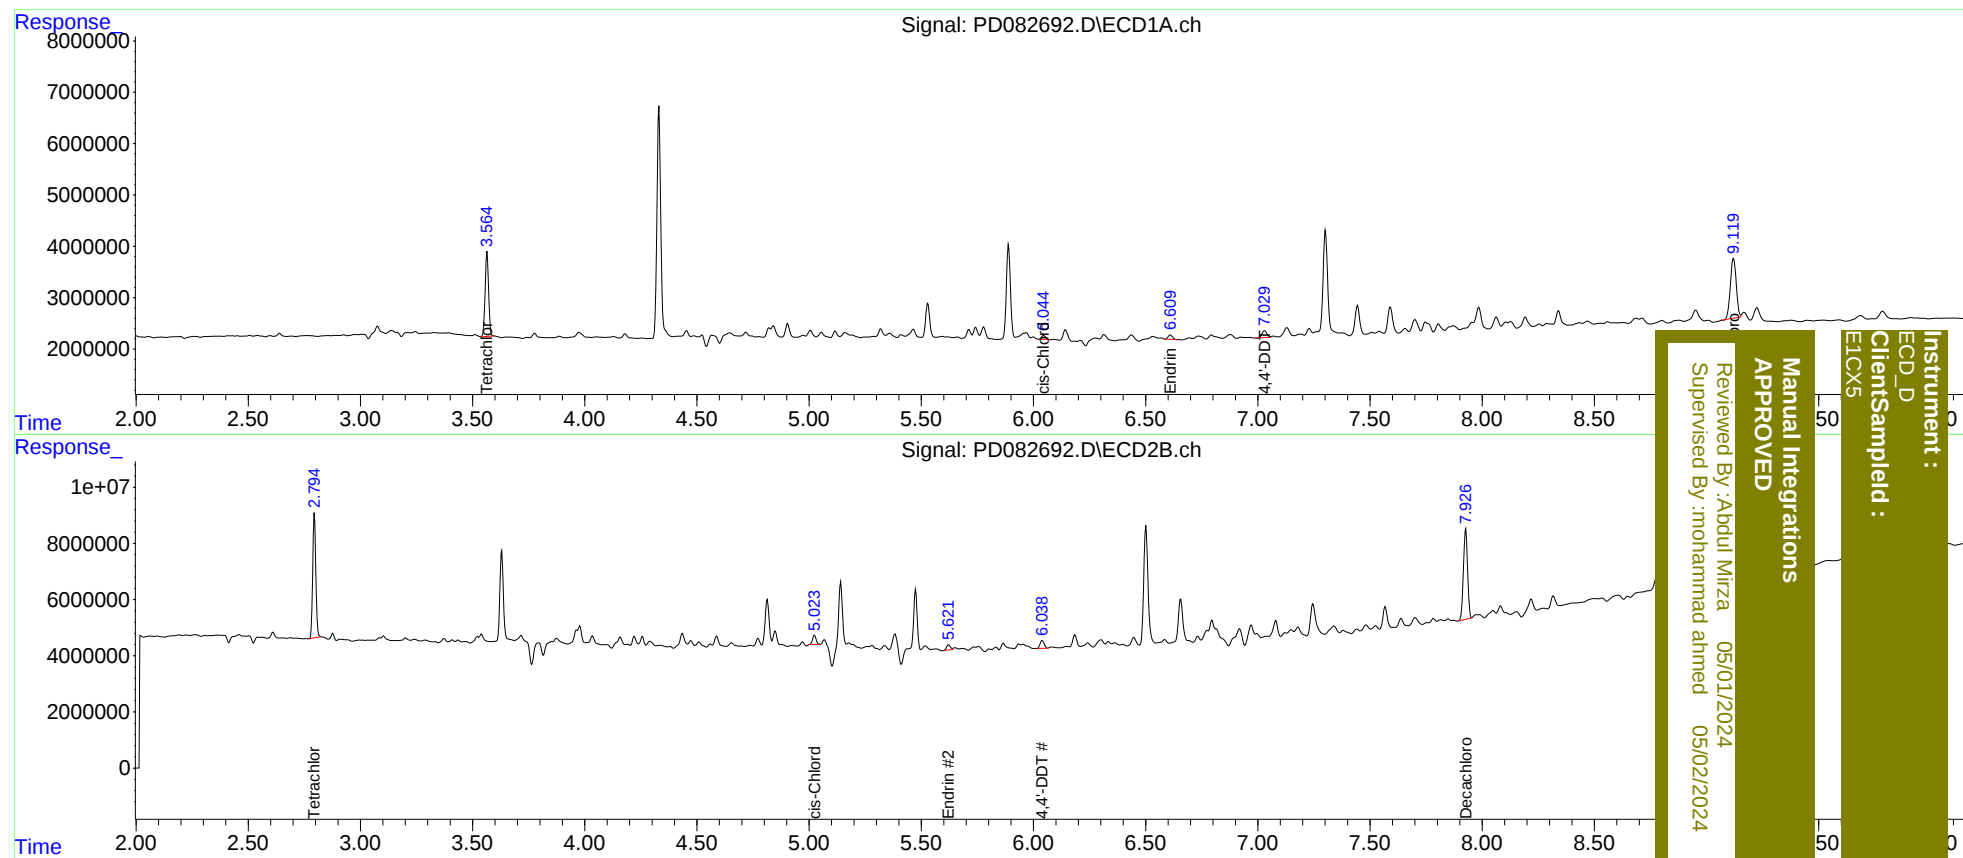

Instrument :
ECD_D
ClientSampled :
EICX5

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/01/2024
Supervised By :mohammad ahmed 05/02/2024