

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050319\
 Data File : PD053174.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2019 23:16
 Operator : AJ\SJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 03:26:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat May 04 03:22:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.510	4.070	97756396	1825.2E6	77.413	71.682
27)	SA Decachlor...	8.305	9.177	201.1E6	2190.4E6	150.841	141.355
Target Compounds							
2)	A alpha-BHC	3.957	4.462	144.4E6	2711.0E6	86.637	75.474
3)	MA gamma-BHC...	4.244	4.749	137.4E6	2389.1E6	84.357	73.818
4)	MA Heptachlor	4.546	5.263	132.4E6	2139.4E6	84.326	73.961
9)	A Endosulfan I	5.589	6.316	118.5E6	1699.6E6	79.171	72.071
13)	MA Dieldrin	5.834	6.574	274.6E6	3503.9E6	171.234	150.171
14)	MA Endrin	6.093	6.792	214.9E6	2453.7E6	170.976	151.514
16)	A 4,4'-DDD	6.218	6.909	169.2E6	2453.6E6	164.753	148.099
17)	MA 4,4'-DDT	6.461	7.208	117.7E6	1624.0E6	190.036	189.545
20)	A Methoxychlor	7.014	7.664	360.0E6	4371.7E6	954.365	867.026


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050319\
Data File : PD053174.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2019 23:16
Operator : AJ\SJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 03:26:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050319CLP.M
Quant Title : GC Extractables
QLast Update : Sat May 04 03:22:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

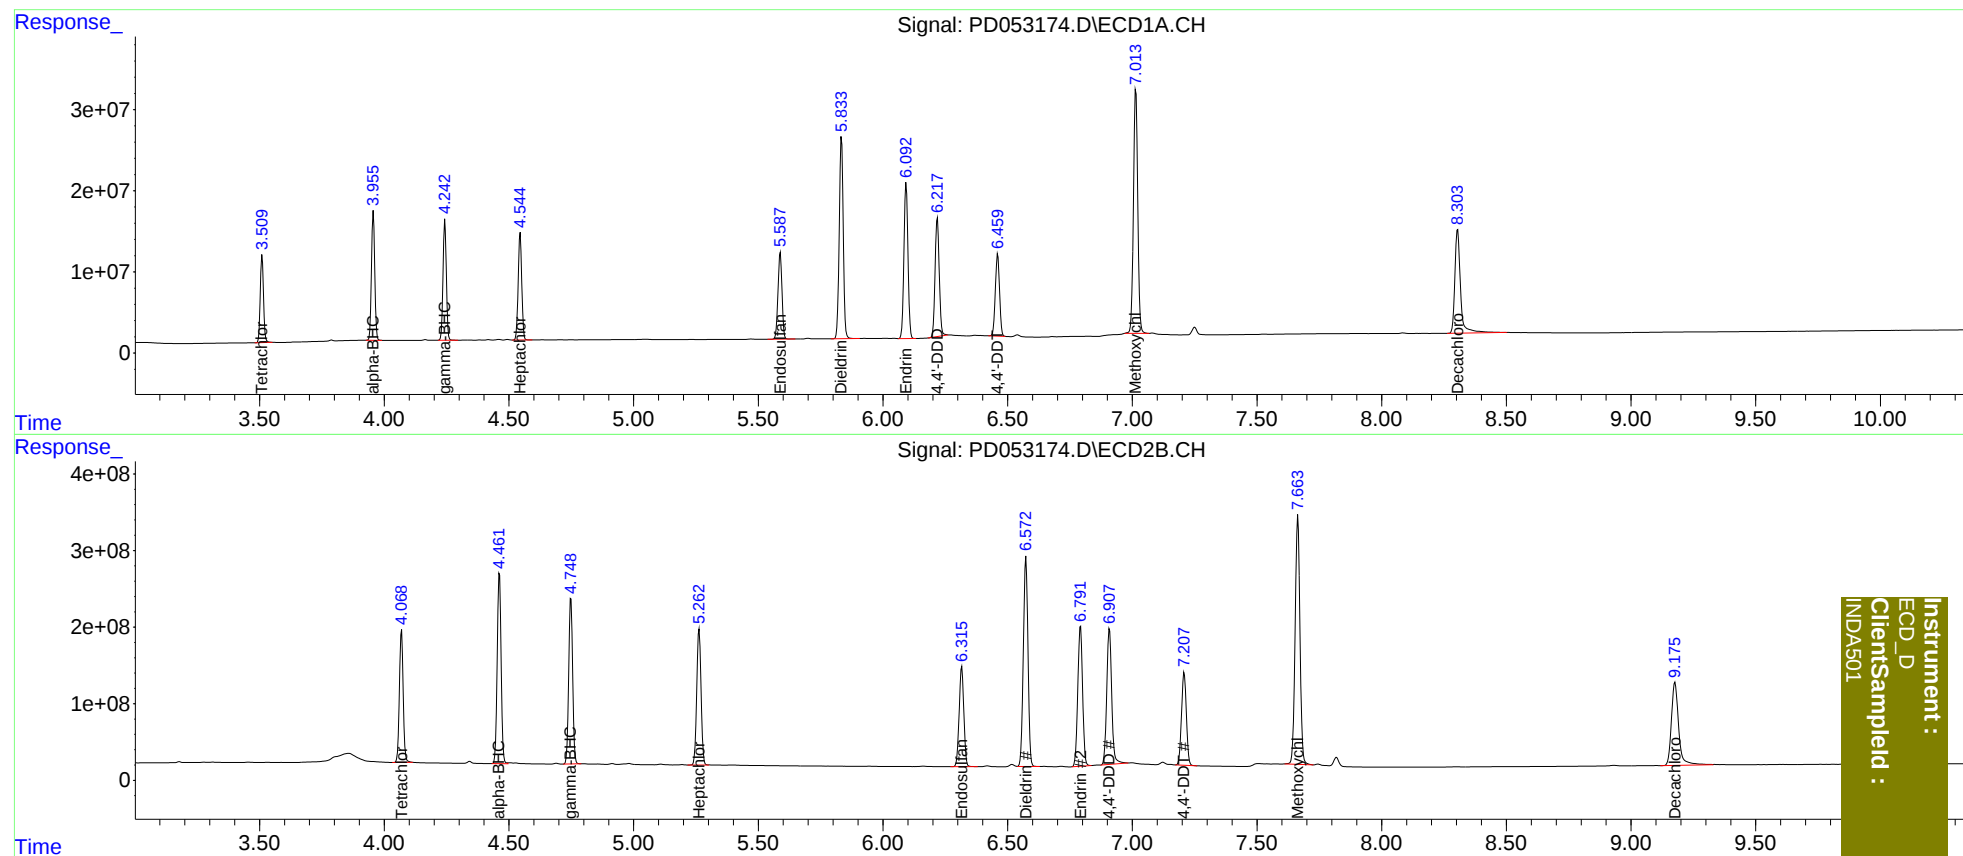


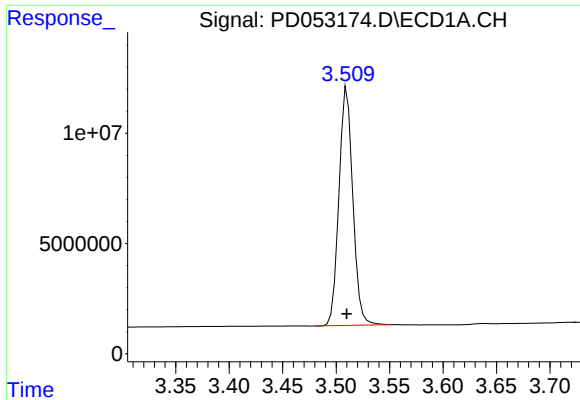

#1 Tetrachloro-m-xylene


R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 97756396
Conc: 77.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

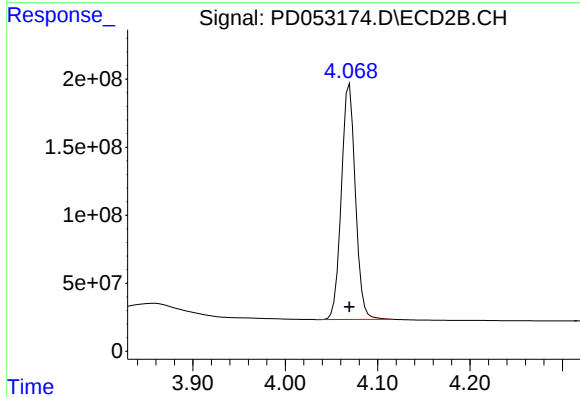


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 1825246898
Conc: 71.68 ng/ml

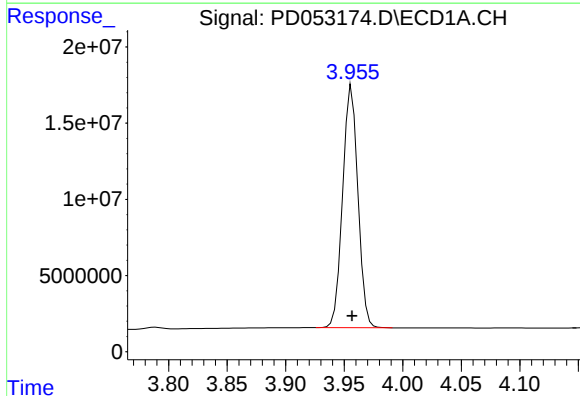


#2 alpha-BHC

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 144430916
Conc: 86.64 ng/ml

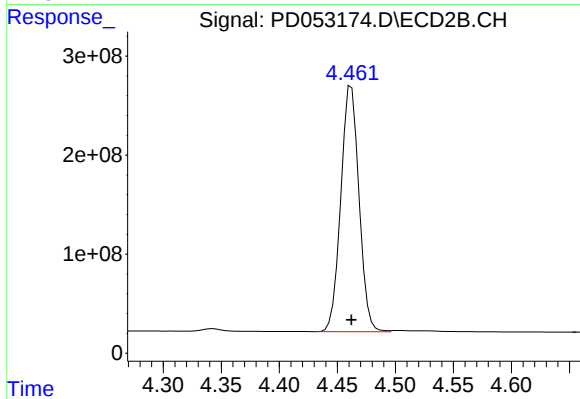

#2 alpha-BHC


R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 2710992788
Conc: 75.47 ng/ml

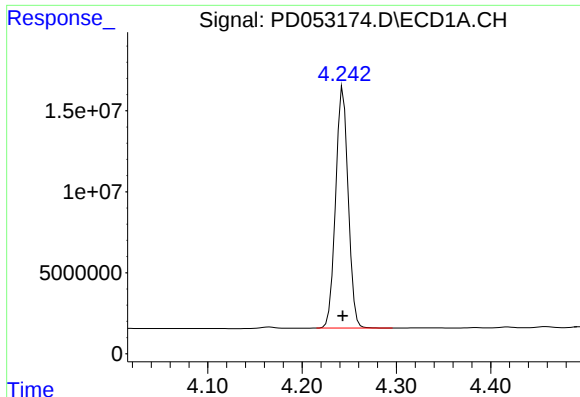

#3 gamma-BHC (Lindane)


R.T.: 4.244 min
Delta R.T.: 0.000 min
Response: 137367227
Conc: 84.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

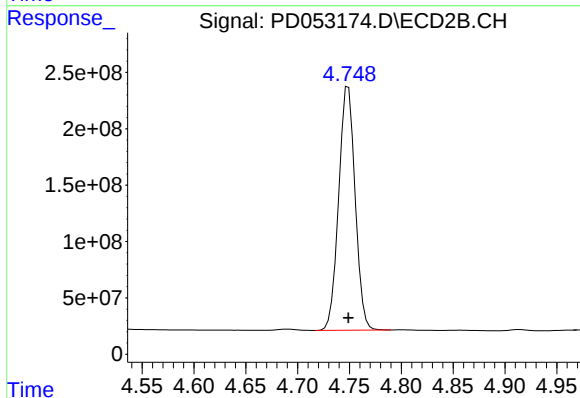


#3 gamma-BHC (Lindane)

R.T.: 4.749 min
Delta R.T.: 0.000 min
Response: 2389127527
Conc: 73.82 ng/ml

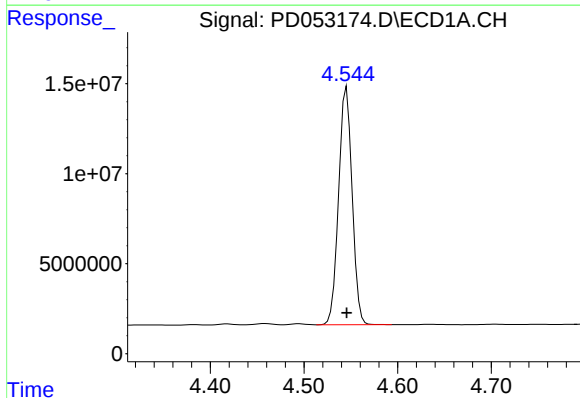


#4 Heptachlor

R.T.: 4.546 min
Delta R.T.: 0.000 min
Response: 132350500
Conc: 84.33 ng/ml

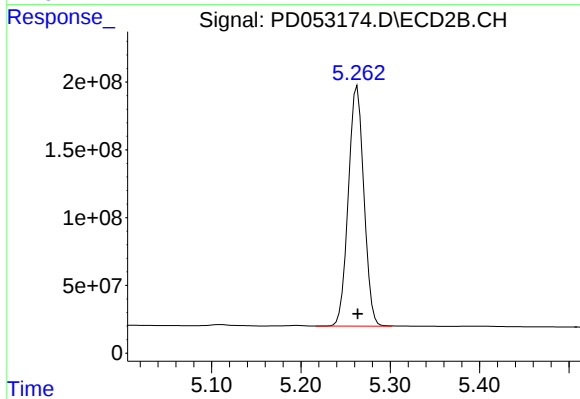

#4 Heptachlor


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 2139370304
Conc: 73.96 ng/ml

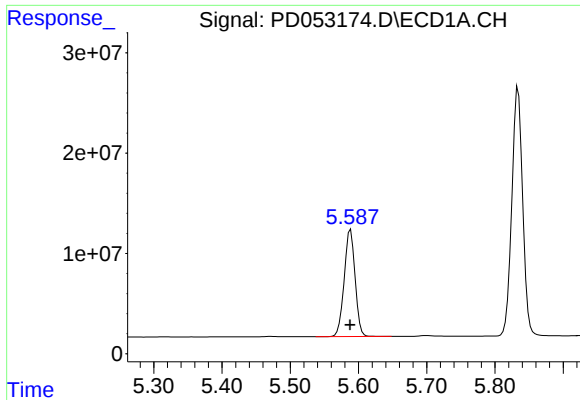

#9 Endosulfan I


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 118450930
Conc: 79.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

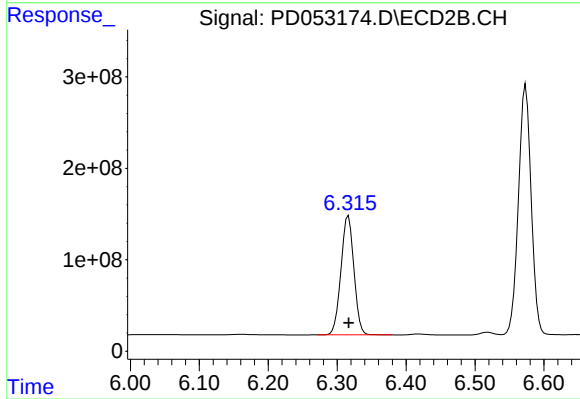


#9 Endosulfan I

R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 1699553440
Conc: 72.07 ng/ml

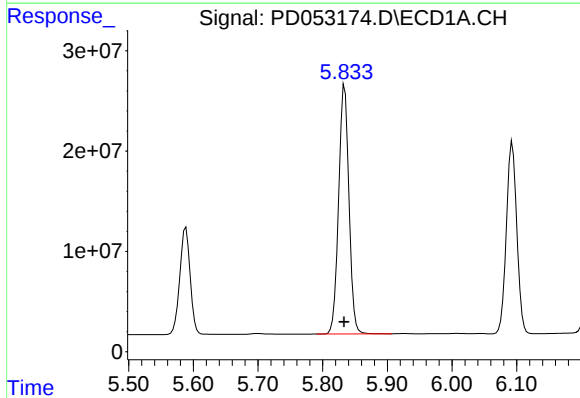


#13 Dieldrin

R.T.: 5.834 min
Delta R.T.: 0.000 min
Response: 274593388
Conc: 171.23 ng/ml

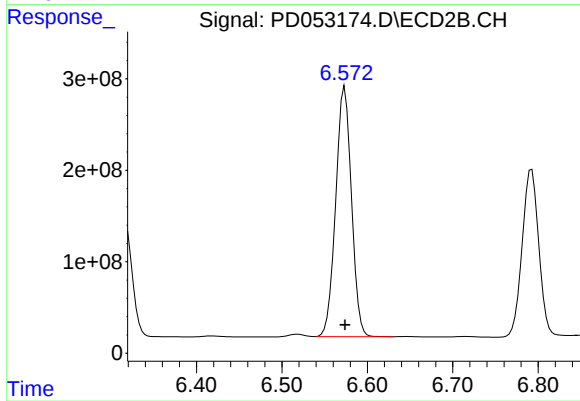

#13 Dieldrin


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 3503921901
Conc: 150.17 ng/ml

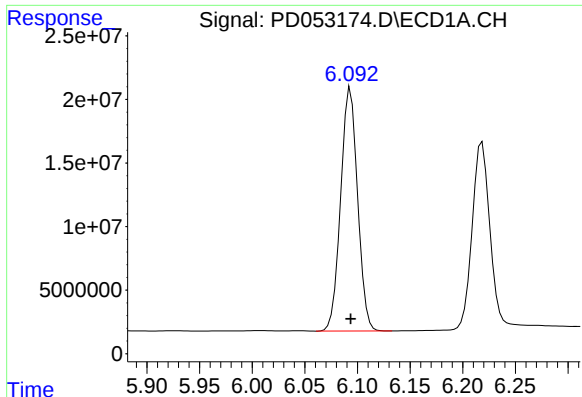

#14 Endrin


R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 214948733
Conc: 170.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

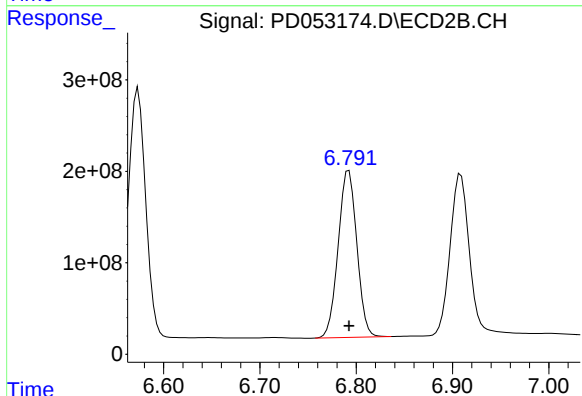


#14 Endrin

R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 2453681905
Conc: 151.51 ng/ml

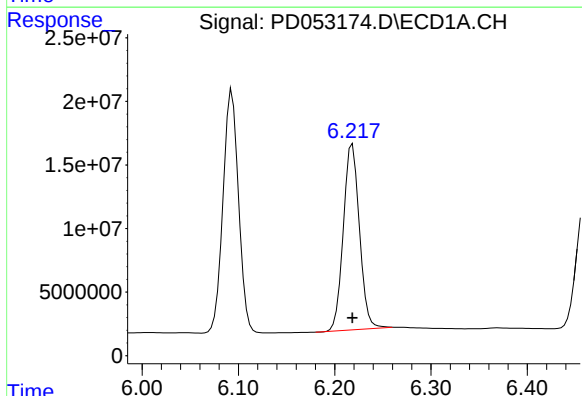


#16 4,4'-DDD

R.T.: 6.218 min
Delta R.T.: 0.000 min
Response: 169168333
Conc: 164.75 ng/ml

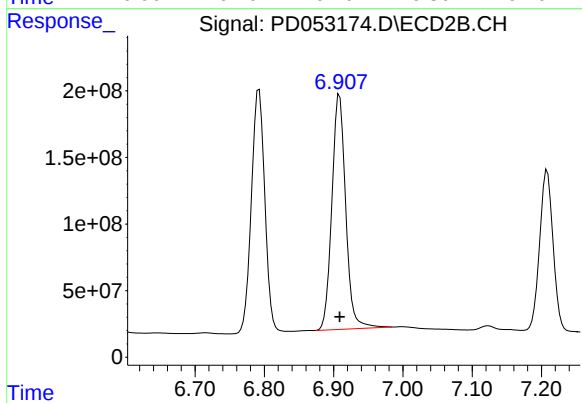

#16 4,4'-DDD


R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 2453599676
Conc: 148.10 ng/ml

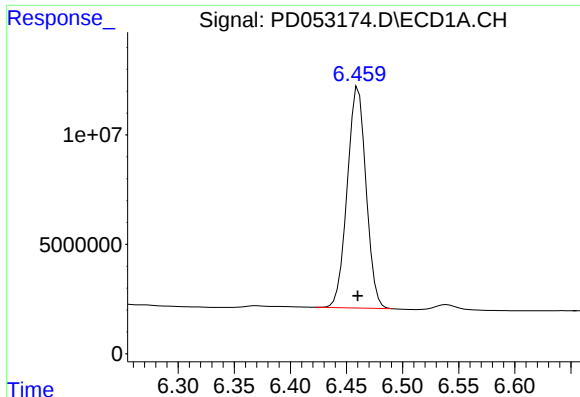

#17 4,4'-DDT


R.T.: 6.461 min
Delta R.T.: 0.000 min
Response: 117731788
Conc: 190.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

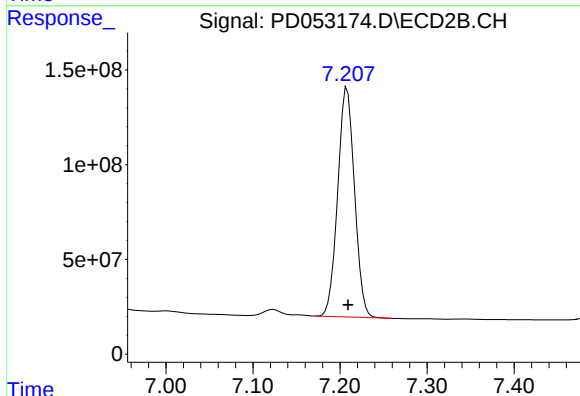


#17 4,4'-DDT

R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 1624018538
Conc: 189.54 ng/ml

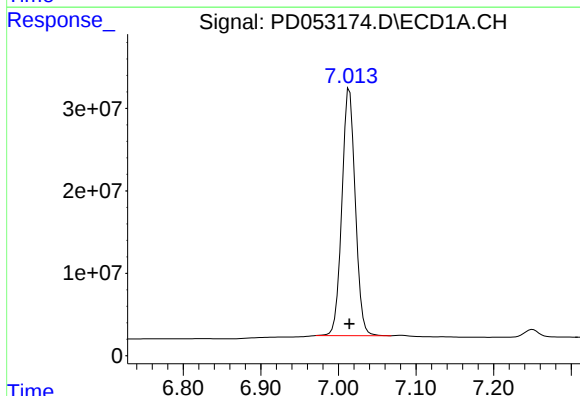


#20 Methoxychlor

R.T.: 7.014 min
Delta R.T.: 0.000 min
Response: 360045913
Conc: 954.37 ng/ml

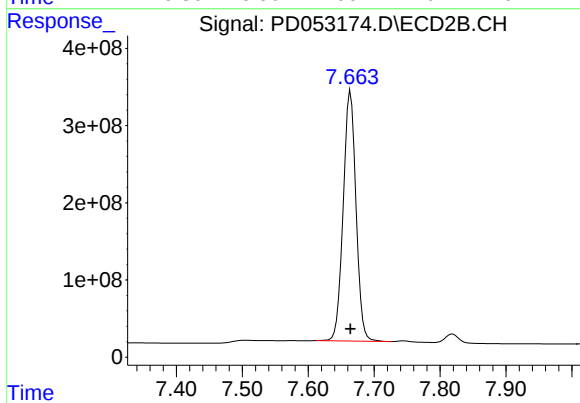

#20 Methoxychlor


R.T.: 7.664 min
Delta R.T.: 0.000 min
Response: 4371655466
Conc: 867.03 ng/ml

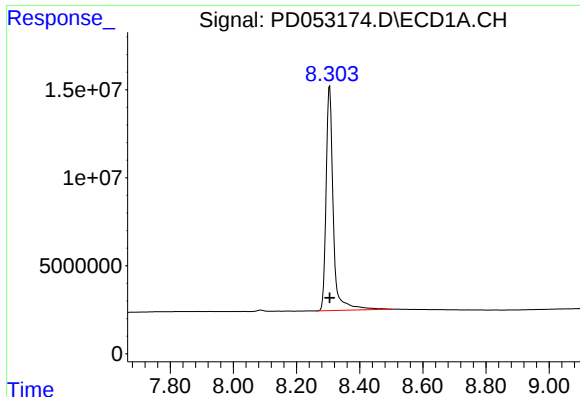

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 201115624
Conc: 150.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

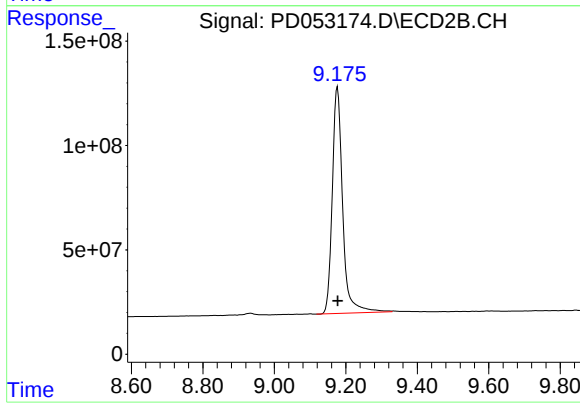

#27 Decachlorobiphenyl

R.T.: 9.177 min
Delta R.T.: -0.001 min
Response: 2190381555
Conc: 141.35 ng/ml