

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050321\
 Data File : PD062677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2021 11:42
 Operator : AR\AJ
 Sample : PB136070BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 PLCS070

Manual Integrations
 APPROVED

Ankita
 5/4/2021 3:16:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 03:50:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	3.973	19253696	254.8E6	20.110	20.982
27)	SA Decachlor...	8.202	9.032	40711749	452.0E6	37.928	41.407
Target Compounds							
2)	A alpha-BHC	3.879	4.361	6596792	103.7E6	4.712	5.484
3)	MA gamma-BHC...	4.163	4.646	6246159	97326269	4.676	5.634
4)	MA Heptachlor	4.464	5.154	6075417	91545980	4.732	5.260
5)	MB Aldrin	4.712	5.459	6014509	91866981	4.617	5.311
6)	B beta-BHC	4.413	4.816	3142430	38207882	5.061	5.005
7)	B delta-BHC	4.618	5.032	6182288	117.4E6	4.543	6.329 #
8)	B Heptachlo...	5.156	5.845	5902811	95032617	4.817	5.925
9)	A Endosulfan I	5.495	6.201	5352147	79208728	4.786	5.401
10)	B trans-Chl...	5.383	6.079	5902279	83284107	4.708	5.085
11)	B cis-Chlor...	5.441	6.151	5766590	77958439	4.696	5.022
12)	B 4,4'-DDE	5.605	6.308	11005916	159.1E6	8.893	10.156
13)	MA Dieldrin	5.738	6.458	11564853	161.4E6	9.175	10.408
14)	MA Endrin	5.996	6.674	10017760	131.8E6	9.468	10.569m
15)	B Endosulfa...	6.269	6.885	9948441	139.9E6	9.592	11.182
16)	A 4,4'-DDD	6.122	6.798	9316236	141.4E6	9.356	11.378
17)	MA 4,4'-DDT	6.363	7.097	7169855	114.2E6	7.655	9.620 #
18)	B Endrin al...	6.438	7.009	9346360	122.2E6	10.475	11.201
19)	B Endosulfa...	6.652	7.232	9071858	128.4E6	9.075	10.065
20)	A Methoxychlor	6.910	7.555	23037255	275.3E6	43.176	48.574m
21)	B Endrin ke...	7.144	7.702	11835042	126.8E6	10.099	10.304

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050321\
Data File : PD062677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2021 11:42
Operator : AR\AJ
Sample : PB136070BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 03:50:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

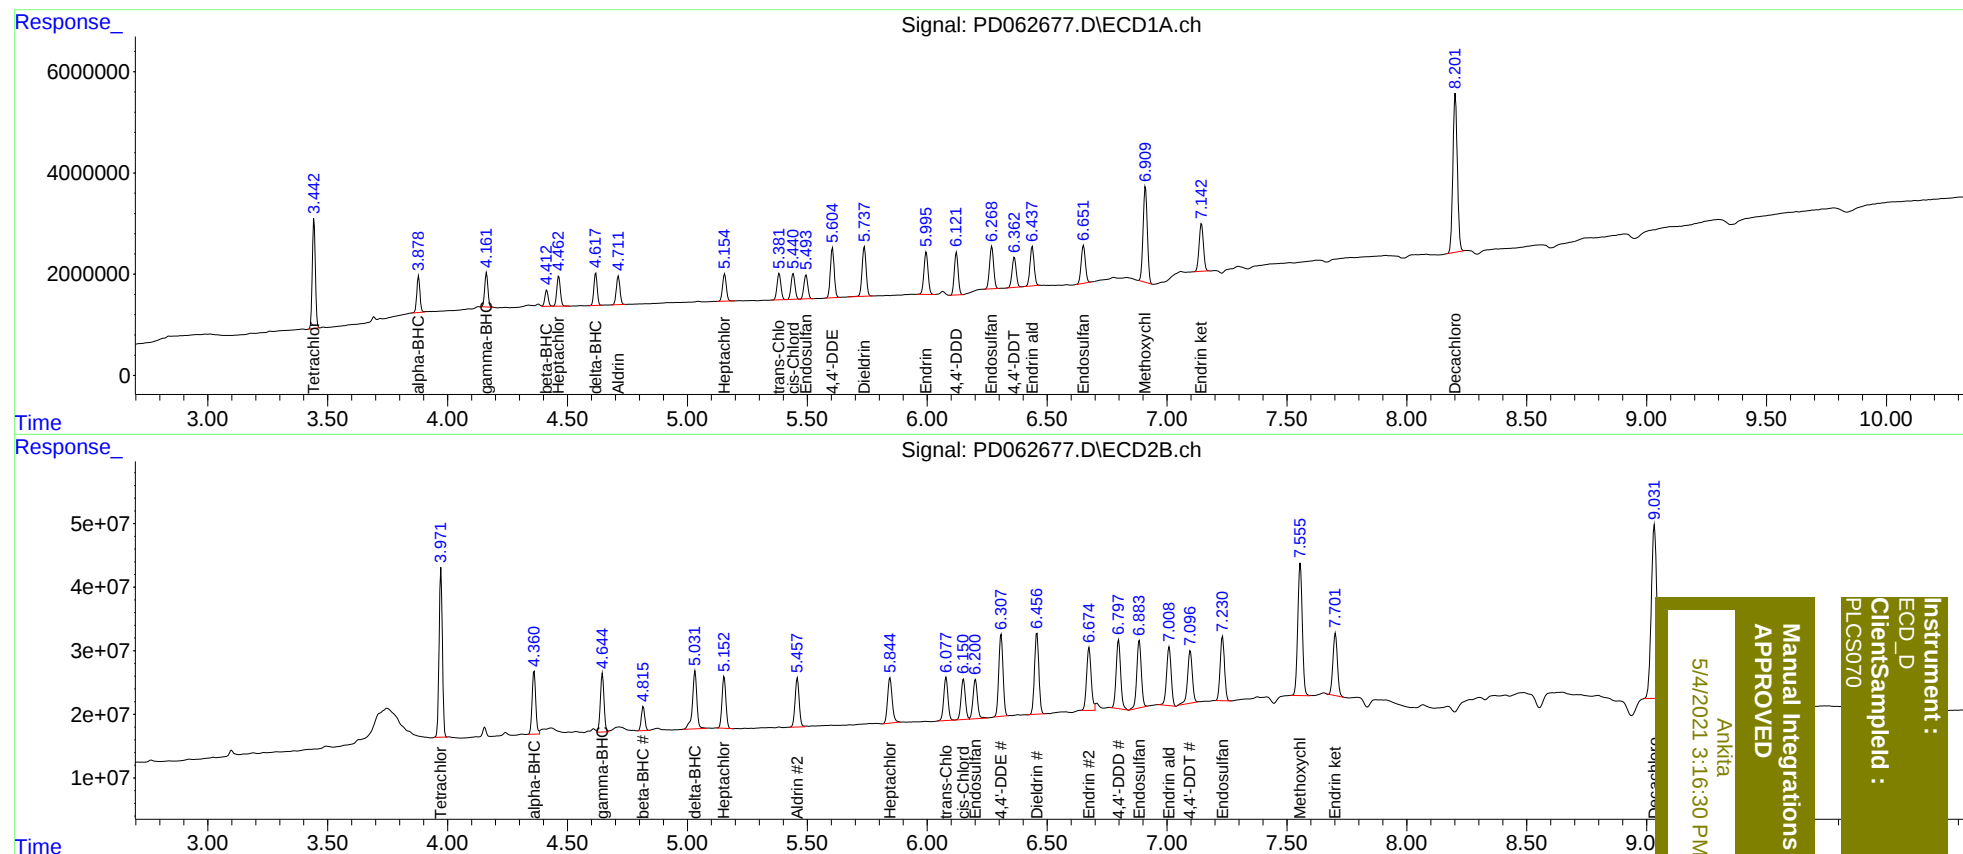

Manual Integrations
APPROVED

Ankita
5/4/2021 3:16:30 PM

Instrument :
ECD_D
ClientSample :
PLCS070