

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
 Data File : PD069383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 10:22
 Operator : AR\AJ
 Sample : N2615-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 01:07:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	20577591	189.5E6	16.242	15.704
27)	SA Decachlor...	8.197	9.365	41207481	210.0E6	30.988	29.863
Target Compounds							
3)	MA gamma-BHC...	4.170	0.000	772025	0	0.427	N.D. #
5)	MB Aldrin	4.716	0.000	2079395	0	1.305	N.D. #
6)	B beta-BHC	4.379f	5.023	9686039	1329745	12.505	0.198 #
7)	B delta-BHC	0.000	5.227	0	24548535	N.D.	2.091
8)	B Heptachlo...	0.000	6.099	0	772583	N.D.	<MDL
9)	A Endosulfan I	5.443f	6.466	812105	-138606	0.557	N.D. #
10)	B trans-Chl...	5.443f	0.000	812105	0	0.542	N.D. #
11)	B cis-Chlor...	5.443	6.431	812105	940769	0.544	<MDL #
15)	B Endosulfa...	0.000	7.121	0	250594	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
Data File : PD069383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 10:22
Operator : AR\AJ
Sample : N2615-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 01:07:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

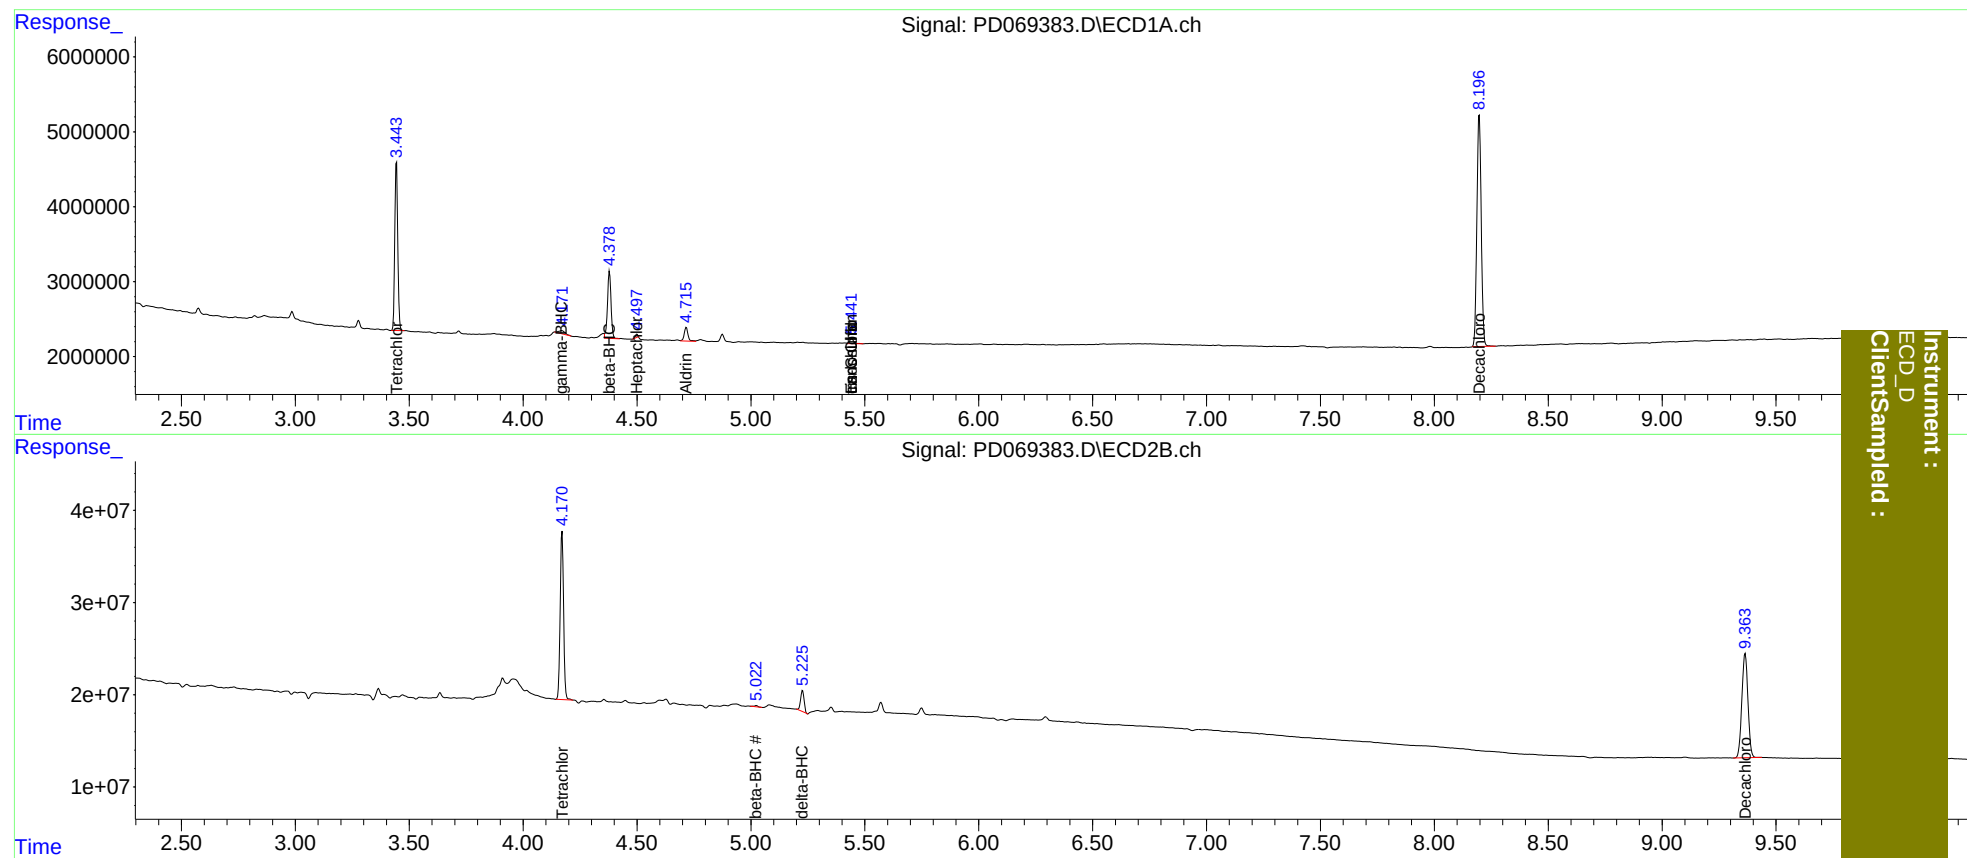


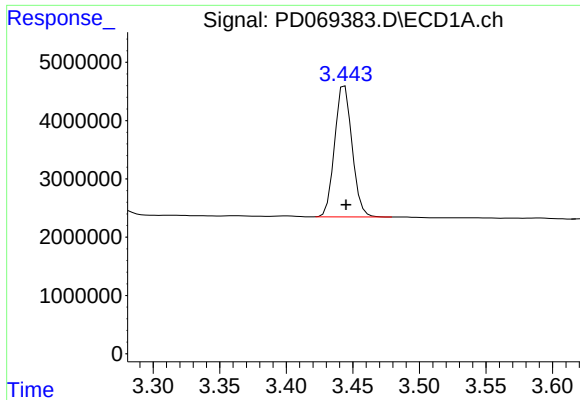

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 20577591
Conc: 16.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

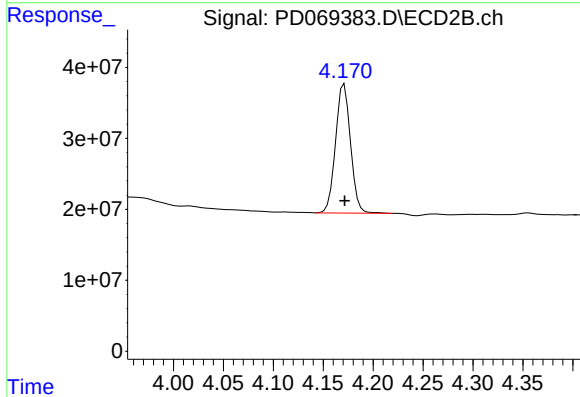


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 189532362
Conc: 15.70 ng/ml

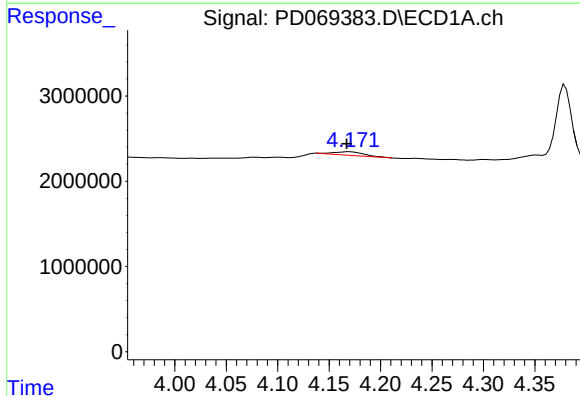


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: 0.003 min
Response: 772025
Conc: 0.43 ng/ml

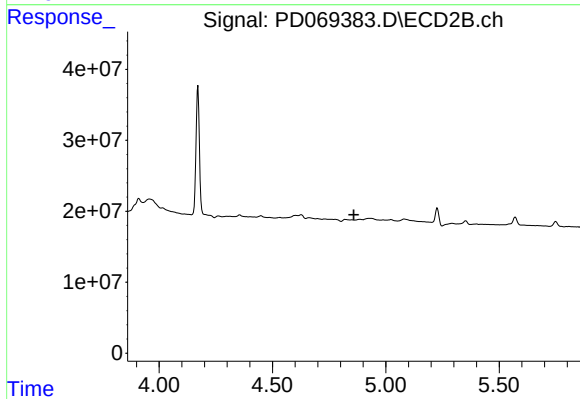

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.859 min
Response: 0
Conc: N.D.

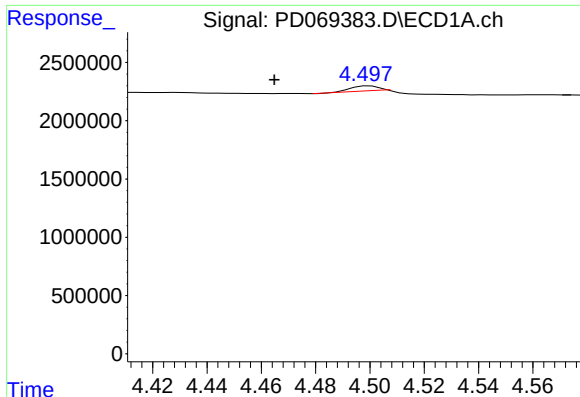

#4 Heptachlor


R.T.: 4.500 min
Delta R.T.: 0.035 min
Response: 274665
Conc: 0.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

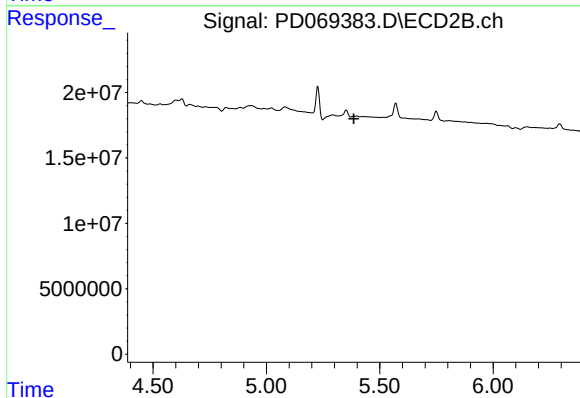


#4 Heptachlor

R.T.: 5.399 min
Delta R.T.: 0.014 min
Response: -5356928
Conc: N.D.

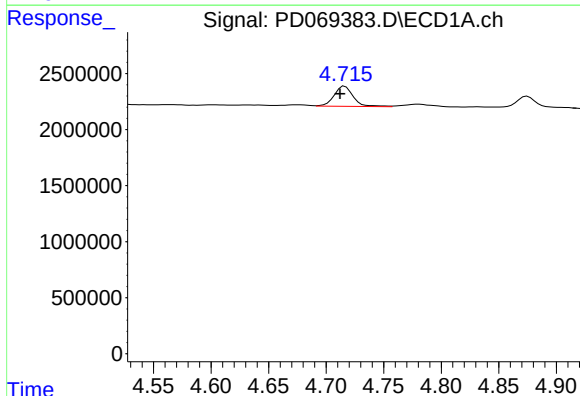


#5 Aldrin

R.T.: 4.716 min
Delta R.T.: 0.004 min
Response: 2079395
Conc: 1.31 ng/ml

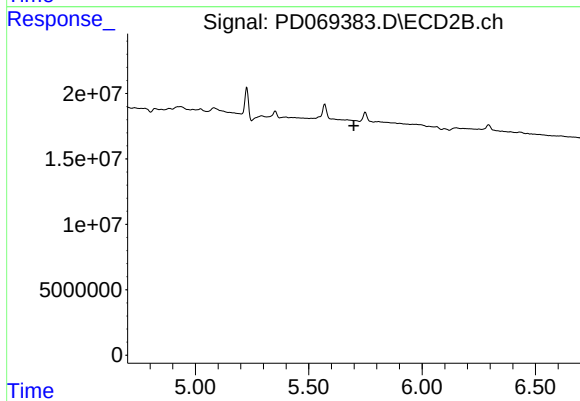

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.698 min
Response: 0
Conc: N.D.

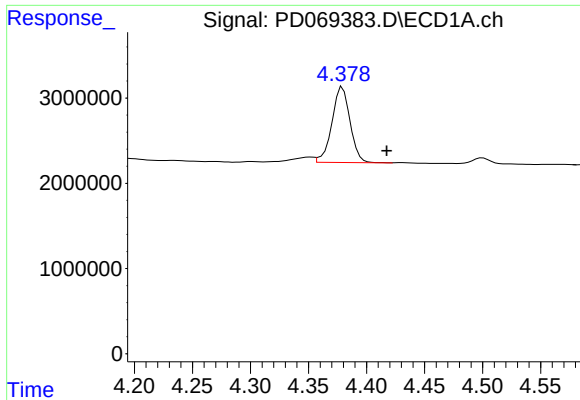

#6 beta-BHC


R.T.: 4.379 min
Delta R.T.: -0.038 min
Response: 9686039
Conc: 12.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

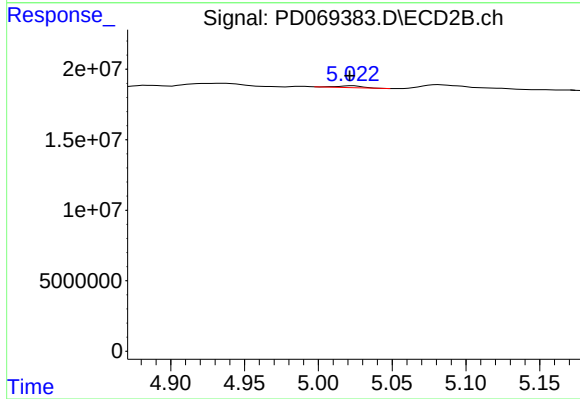


#6 beta-BHC

R.T.: 5.023 min
Delta R.T.: 0.002 min
Response: 1329745
Conc: 0.20 ng/ml

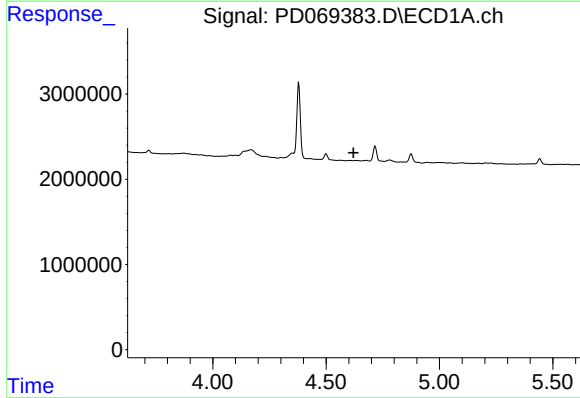


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.621 min
Response: 0
Conc: N.D.

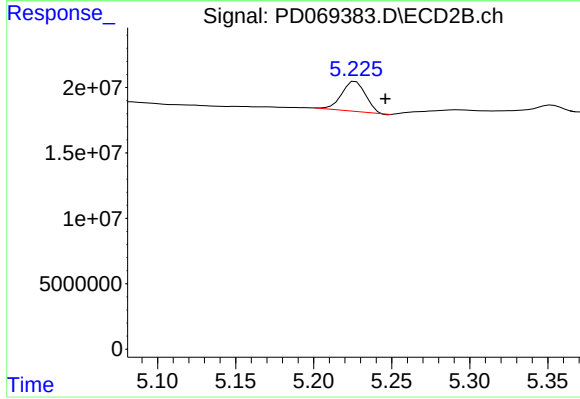

#7 delta-BHC


R.T.: 5.227 min
Delta R.T.: -0.019 min
Response: 24548535
Conc: 2.09 ng/ml

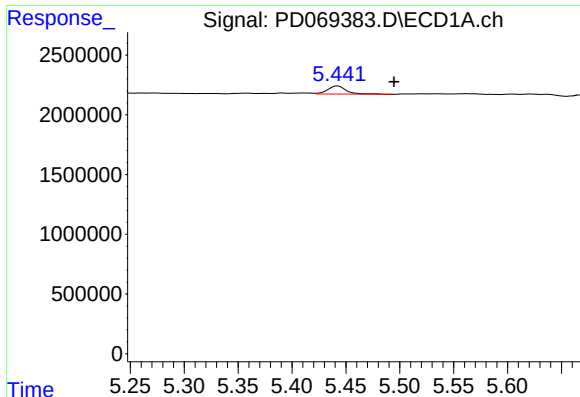

#9 Endosulfan I


R.T.: 5.443 min
Delta R.T.: -0.052 min
Response: 812105
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

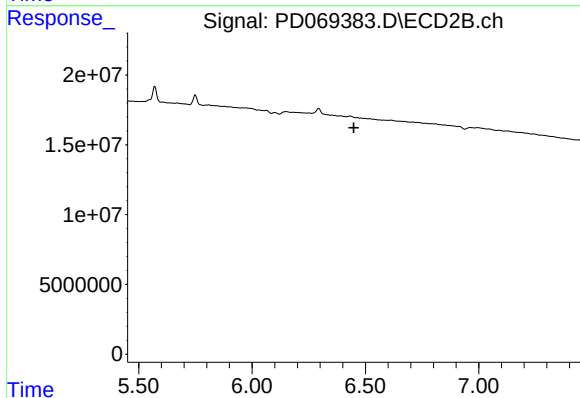


#9 Endosulfan I

R.T.: 6.466 min
Delta R.T.: 0.017 min
Response: -138606
Conc: N.D.

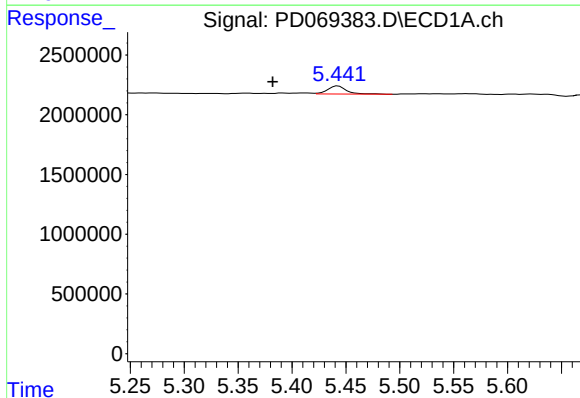


#10 trans-Chlordane

R.T.: 5.443 min
Delta R.T.: 0.061 min
Response: 812105
Conc: 0.54 ng/ml

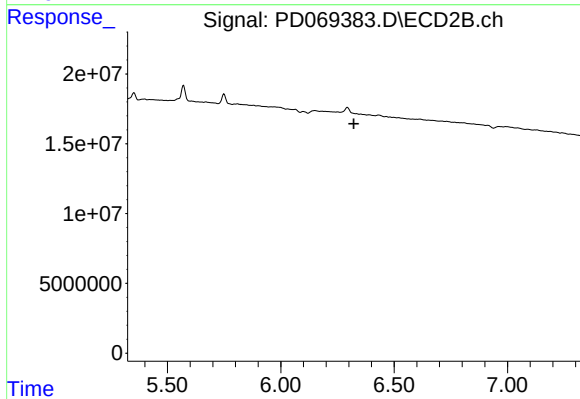

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

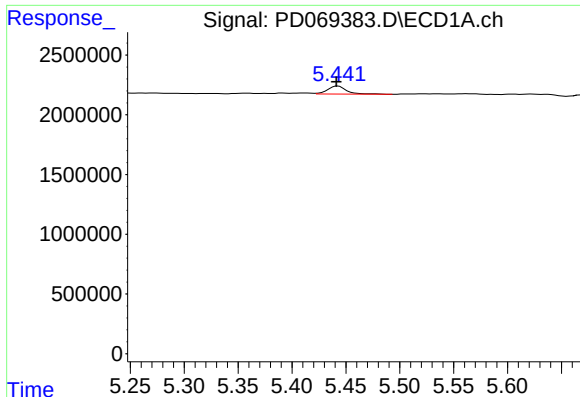

#11 cis-Chlordane


R.T.: 5.443 min
Delta R.T.: 0.002 min
Response: 812105
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

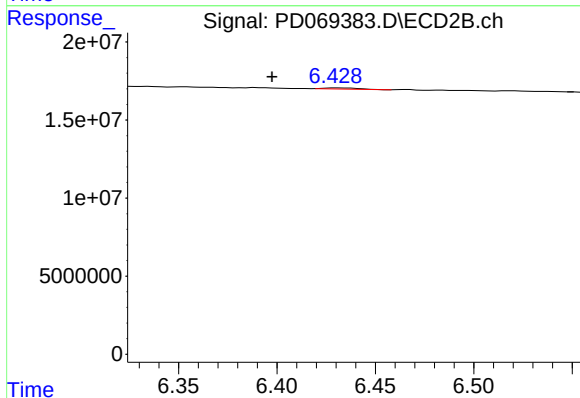


#11 cis-Chlordane

R.T.: 6.431 min
Delta R.T.: 0.033 min
Response: 940769
Conc: N.D.

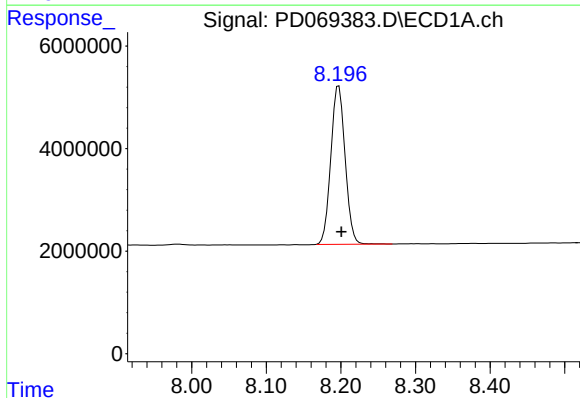

#27 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.004 min
Response: 41207481
Conc: 30.99 ng/ml

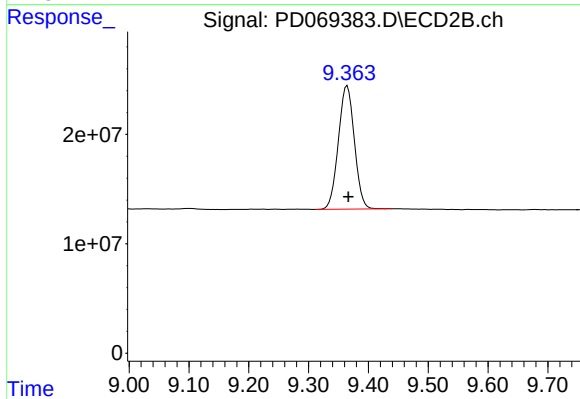

#27 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.002 min
Response: 209999258
Conc: 29.86 ng/ml