

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
 Data File : PD069406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 17:54
 Operator : AR\AJ
 Sample : N2615-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 01:20:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	21176473	215.2E6	16.714	17.826
2)	SA Decachlor...	8.197	9.365	37505943	221.8E6	28.204	31.545
Target Compounds							
3)	MA gamma-BHC...	4.170	0.000	1767627	0	0.977	N.D. #
4)	MA Heptachlor	0.000	5.367	0	3941260	N.D.	0.260
5)	MB Aldrin	0.000	5.652f	0	325733	N.D.	<MDL
6)	B beta-BHC	0.000	5.026	0	564677	N.D.	<MDL
7)	B delta-BHC	4.571f	5.221	552695	4110999	0.346	0.350
9)	A Endosulfan I	0.000	6.464	0	165095	N.D.	<MDL
10)	B trans-Chl...	0.000	6.276f	0	533113	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.427	0	775159	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.611f	0	468008	N.D.	<MDL
15)	B Endosulfa...	6.216f	7.100	265708	4028865	0.206	0.420 #
16)	A 4,4'-DDD	6.068f	7.100f	283323	4028865	0.232	0.430 #
17)	MA 4,4'-DDT	6.366	7.285f	401576	277843	0.327	<MDL #
18)	B Endrin al...	0.000	7.285	0	277843	N.D.	<MDL
20)	A Methoxychlor	0.000	7.814	0	622018	N.D.	0.151
22)	Toxaphene-1	0.000	6.611	0	468008	N.D.	9.921
23)	Toxaphene-2	6.216	6.828f	265708	380737	26.671	3.600 #
24)	Toxaphene-3	6.366f	0.000	401576	0	16.944	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
Data File : PD069406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 17:54
Operator : AR\AJ
Sample : N2615-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 01:20:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

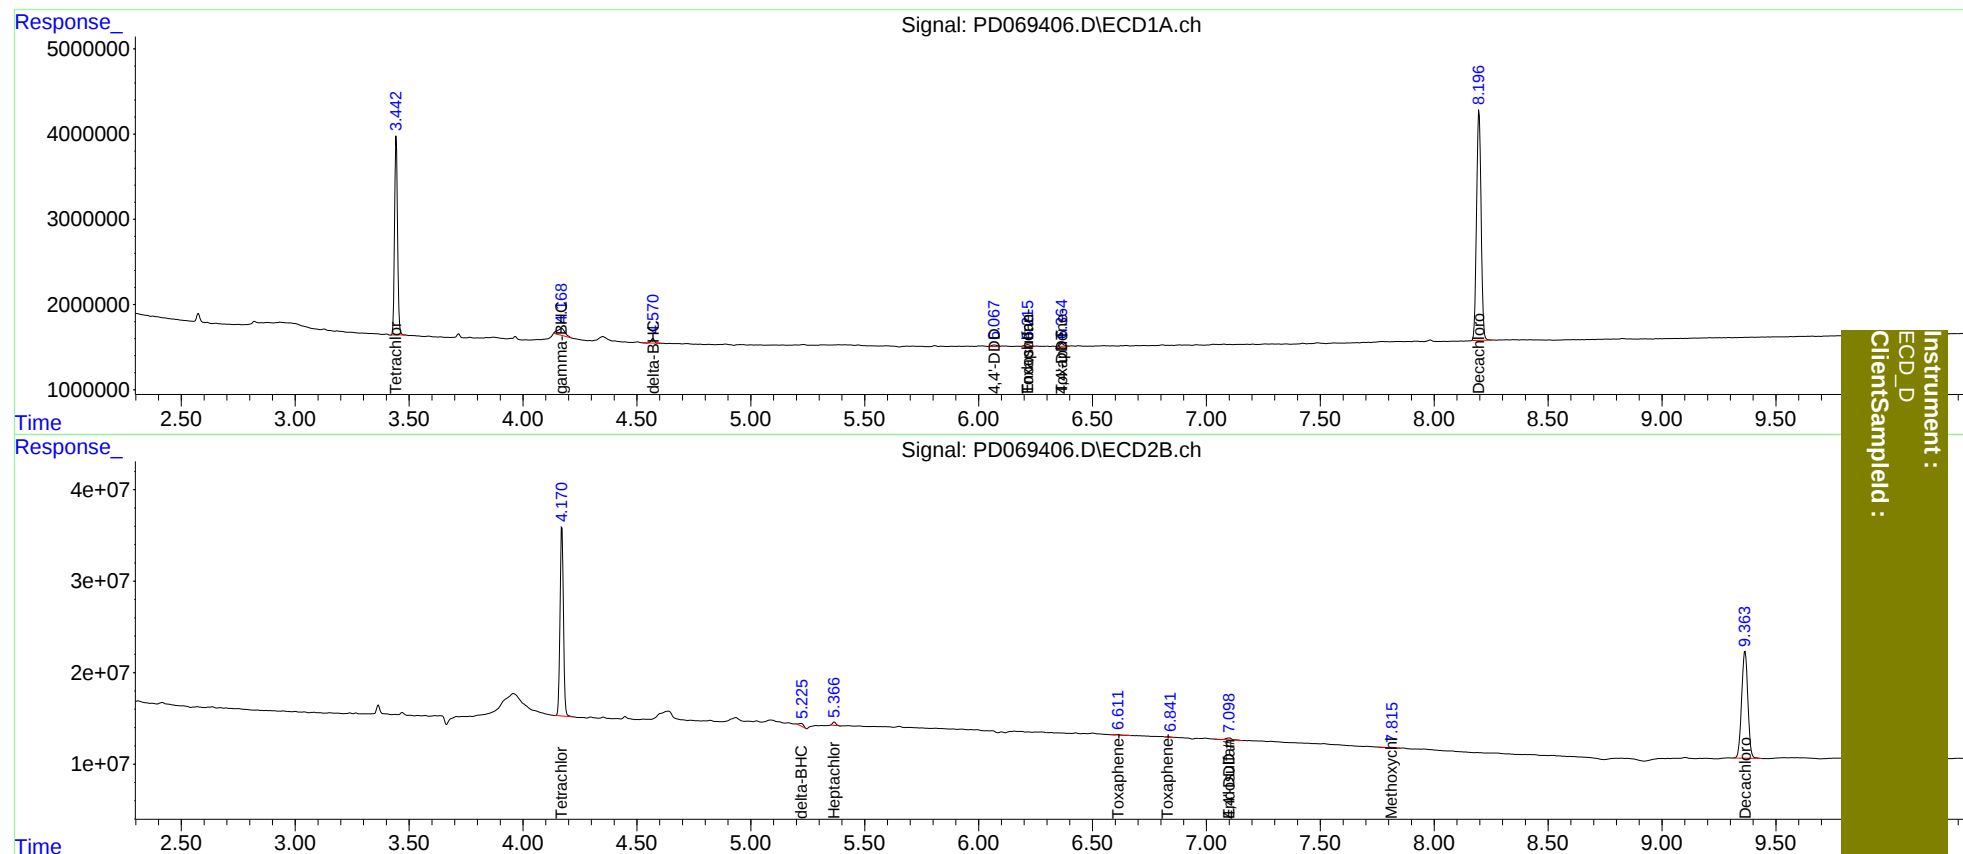


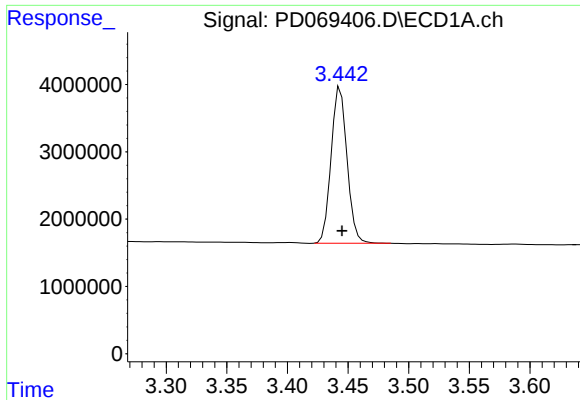

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 21176473
Conc: 16.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

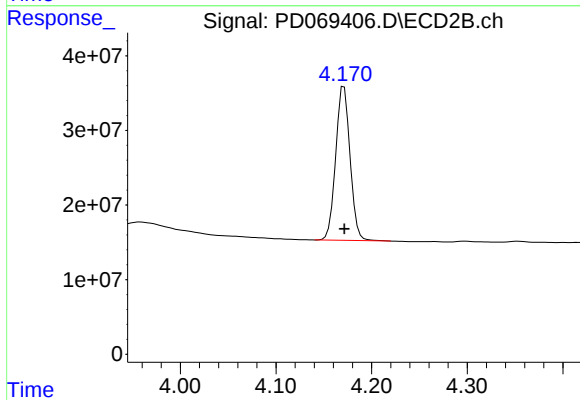


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 215150467
Conc: 17.83 ng/ml

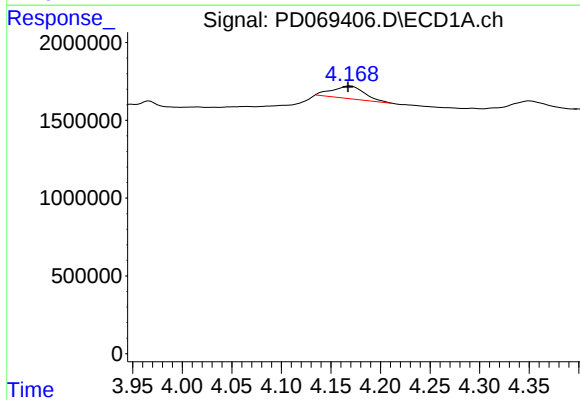


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: 0.002 min
Response: 1767627
Conc: 0.98 ng/ml

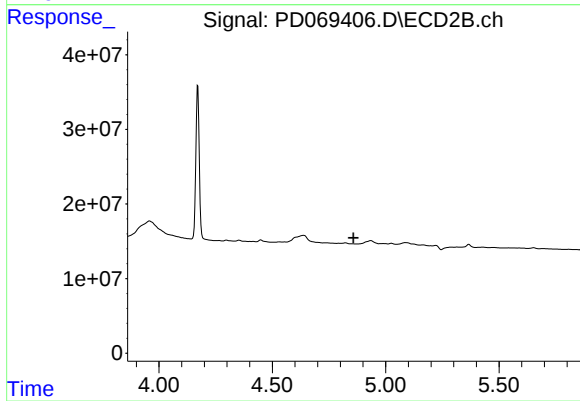

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.859 min
Response: 0
Conc: N.D.

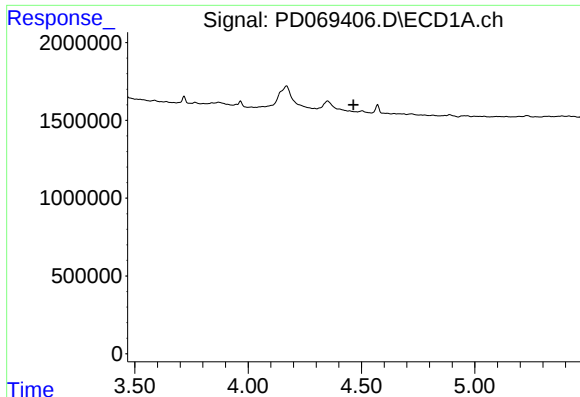

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

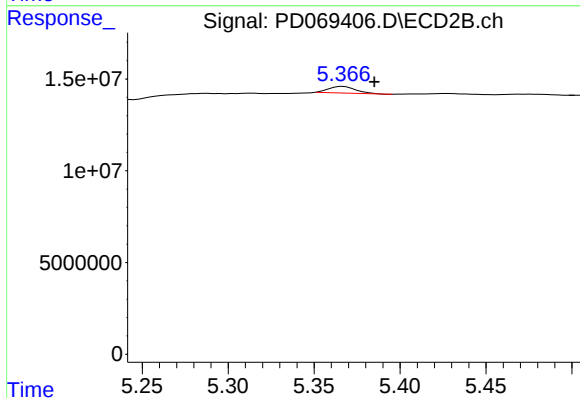


#4 Heptachlor

R.T.: 5.367 min
Delta R.T.: -0.018 min
Response: 3941260
Conc: 0.26 ng/ml

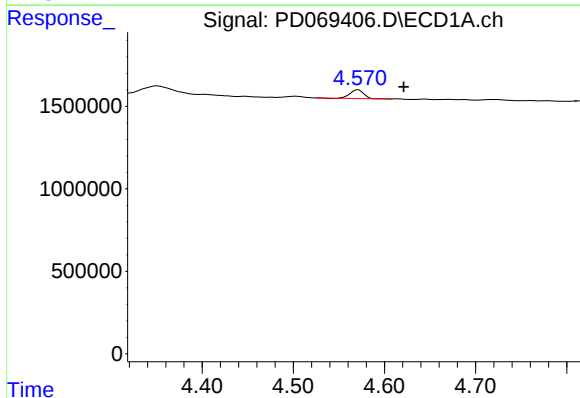


#7 delta-BHC

R.T.: 4.571 min
Delta R.T.: -0.050 min
Response: 552695
Conc: 0.35 ng/ml

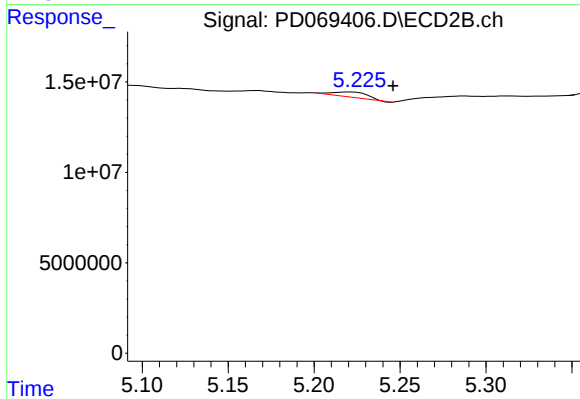

#7 delta-BHC


R.T.: 5.221 min
Delta R.T.: -0.024 min
Response: 4110999
Conc: 0.35 ng/ml

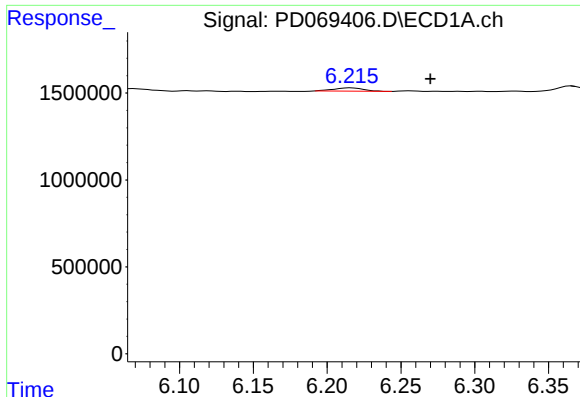

#15 Endosulfan II


R.T.: 6.216 min
Delta R.T.: -0.054 min
Response: 265708
Conc: 0.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

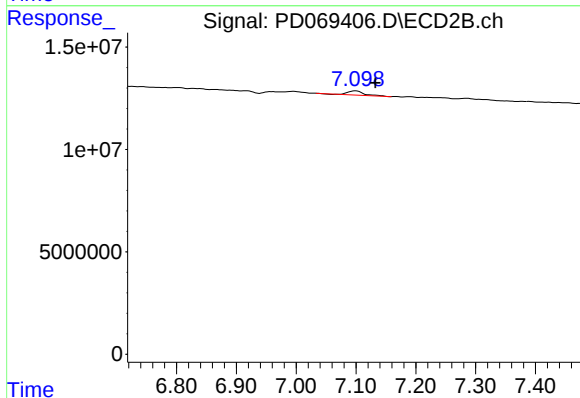


#15 Endosulfan II

R.T.: 7.100 min
Delta R.T.: -0.033 min
Response: 4028865
Conc: 0.42 ng/ml

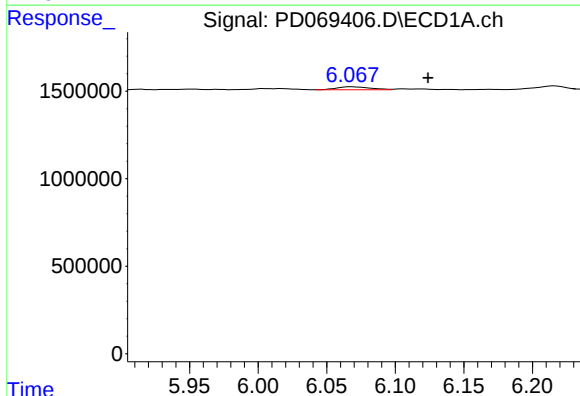


#16 4,4'-DDD

R.T.: 6.068 min
Delta R.T.: -0.056 min
Response: 283323
Conc: 0.23 ng/ml

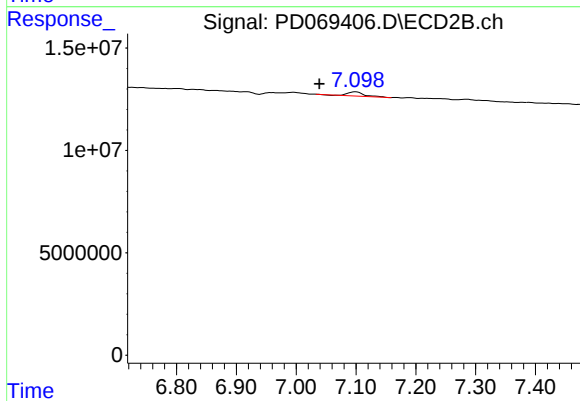

#16 4,4'-DDD


R.T.: 7.100 min
Delta R.T.: 0.061 min
Response: 4028865
Conc: 0.43 ng/ml

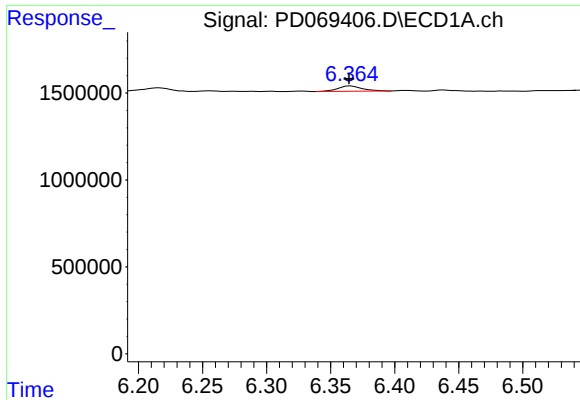

#17 4,4'-DDT


R.T.: 6.366 min
Delta R.T.: 0.002 min
Response: 401576
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

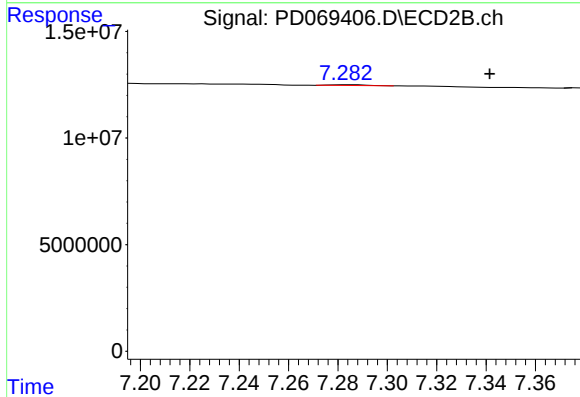


#17 4,4'-DDT

R.T.: 7.285 min
Delta R.T.: -0.057 min
Response: 277843
Conc: N.D.

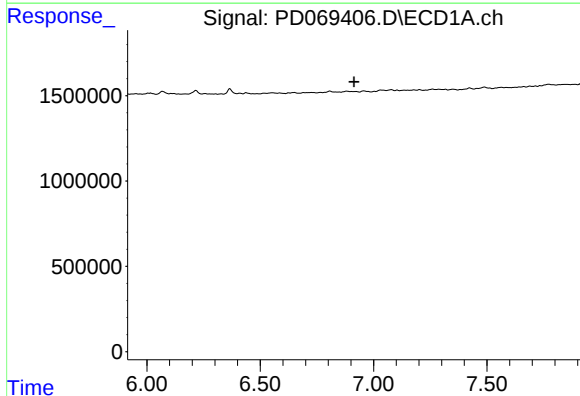


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.914 min
Response: 0
Conc: N.D.

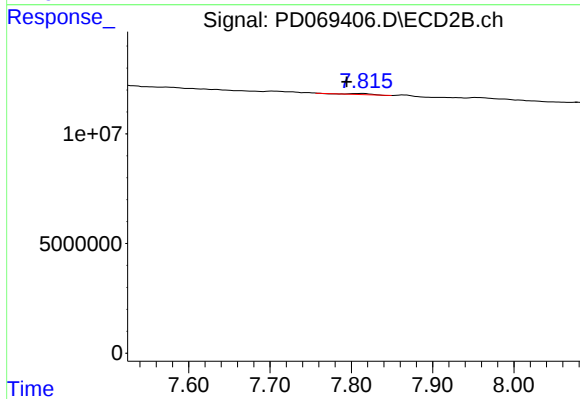

#20 Methoxychlor


R.T.: 7.814 min
Delta R.T.: 0.020 min
Response: 622018
Conc: 0.15 ng/ml

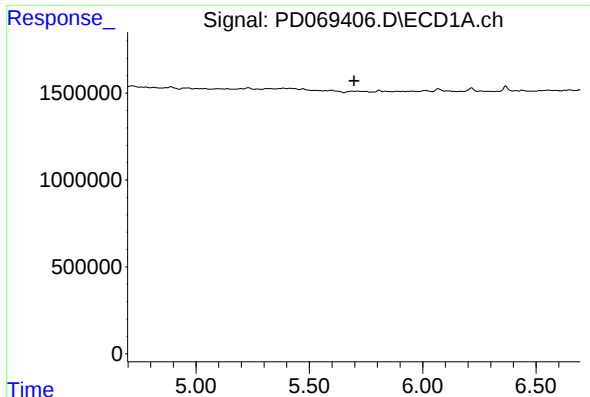

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.697 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

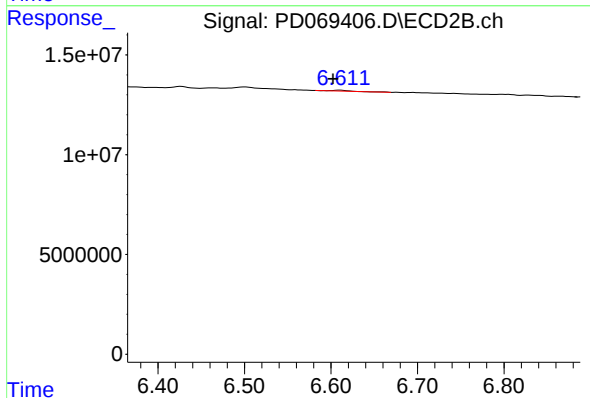


#22 Toxaphene-1

R.T.: 6.611 min
Delta R.T.: 0.009 min
Response: 468008
Conc: 9.92 ng/ml

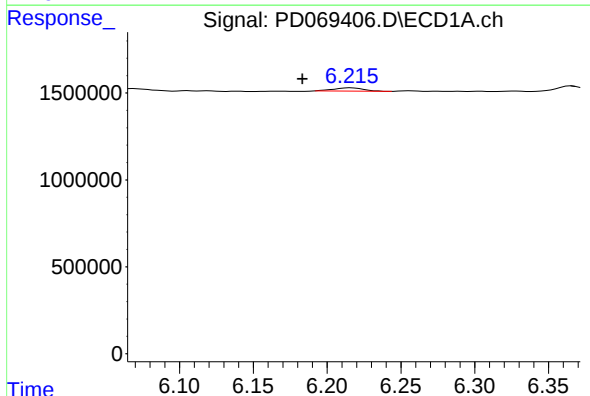


#23 Toxaphene-2

R.T.: 6.216 min
Delta R.T.: 0.033 min
Response: 265708
Conc: 26.67 ng/ml

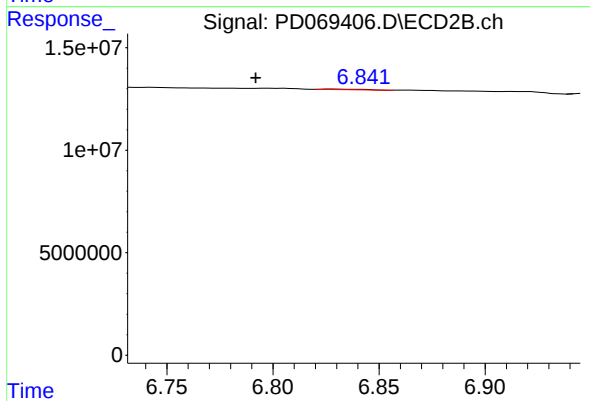

#23 Toxaphene-2


R.T.: 6.828 min
Delta R.T.: 0.036 min
Response: 380737
Conc: 3.60 ng/ml

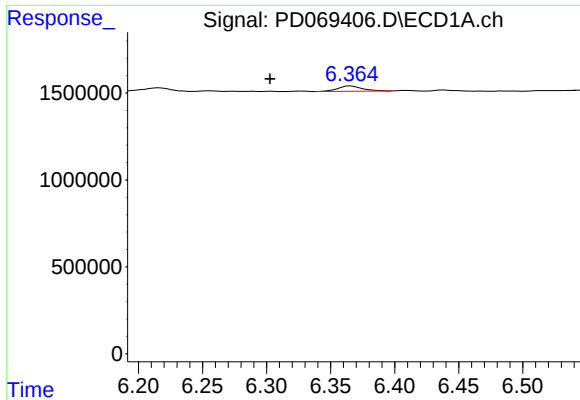

#24 Toxaphene-3


R.T.: 6.366 min
Delta R.T.: 0.063 min
Response: 401576
Conc: 16.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

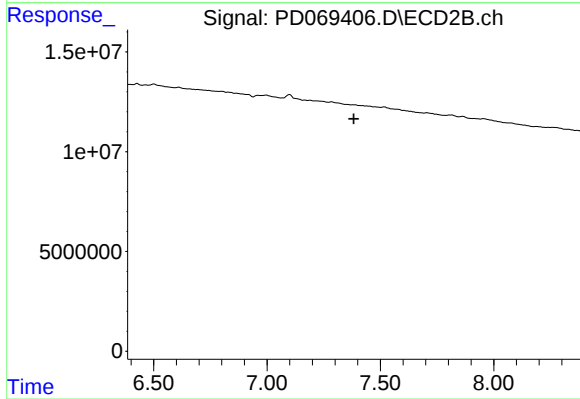


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.382 min
Response: 0
Conc: N.D.

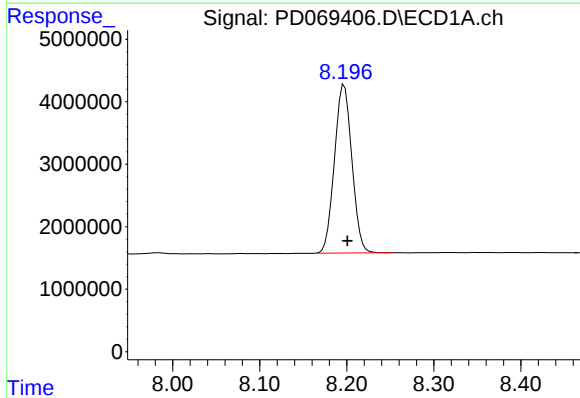

#27 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.004 min
Response: 37505943
Conc: 28.20 ng/ml

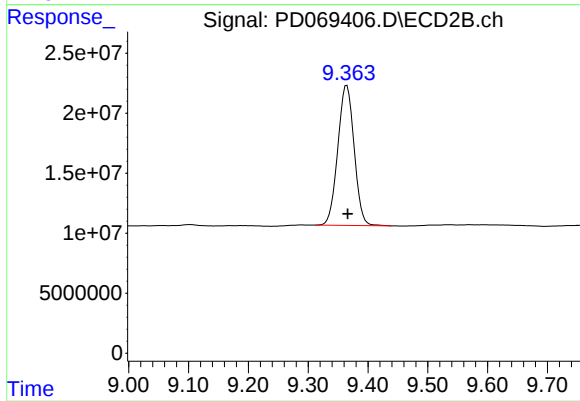

#27 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.002 min
Response: 221830674
Conc: 31.55 ng/ml